
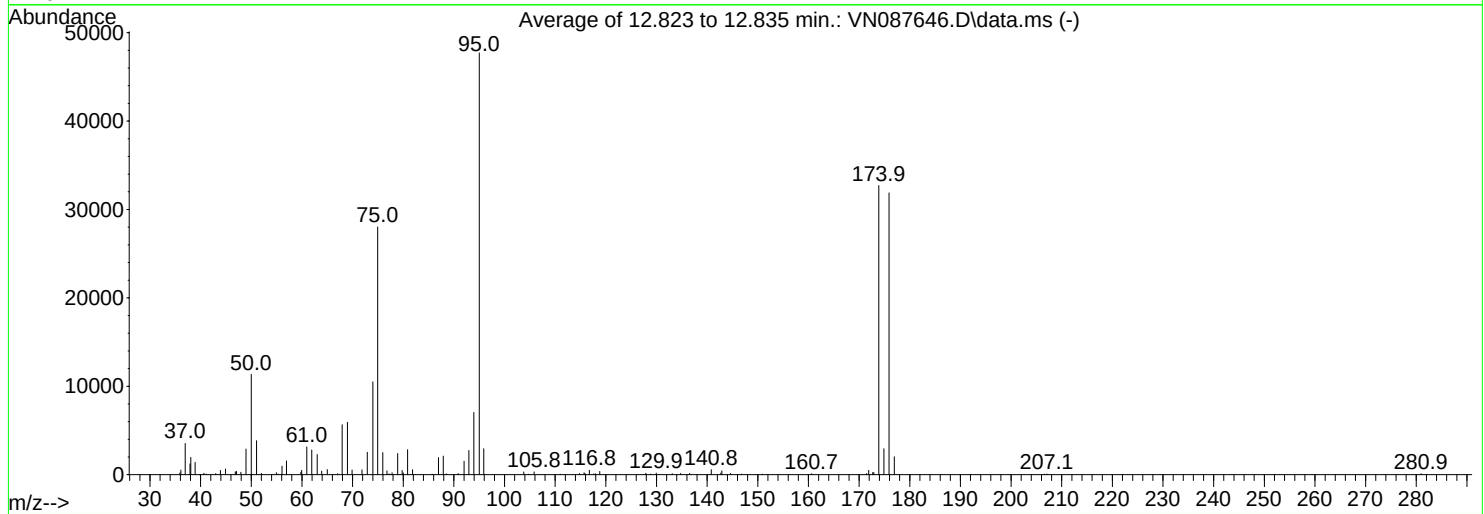


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082525\
Data File : VN087646.D
Acq On : 25 Aug 2025 08:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

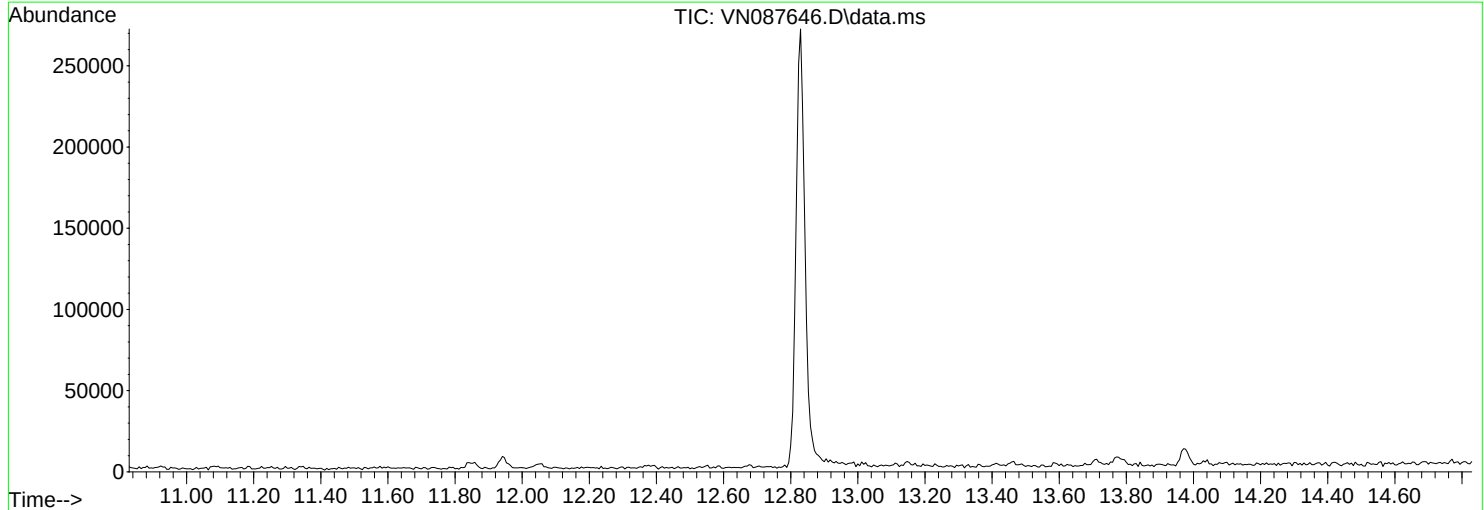

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	11343	PASS
75	95	30	60	58.7	28016	PASS
95	95	100	100	100.0	47715	PASS
96	95	5	9	6.1	2933	PASS
173	174	0.00	2	0.8	254	PASS
174	95	50	100	68.5	32707	PASS
175	174	5	9	9.0	2932	PASS
176	174	95	101	97.4	31869	PASS
177	176	5	9	6.4	2024	PASS

Average of 12.823 to 12.835 min.: VN087646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	209	44.90	640	56.95	1567	69.90	520
36.10	532	46.85	329	59.80	260	71.85	549
36.95	3536	47.10	355	59.95	485	72.90	253
37.90	1208	47.95	278	60.95	3137	74.00	1049
38.05	1949	48.95	2894	61.95	2781	74.95	28016
38.90	1396	50.00	11343	63.00	2291	75.95	2507
39.80	10	51.05	3842	63.90	399	76.80	427
40.65	170	52.00	139	65.00	572	77.20	94
41.10	79	54.95	218	67.05	112	77.80	211
43.00	129	55.30	57	67.95	5649	78.90	2397
43.90	472	56.05	967	69.00	5915	79.80	471

Average of 12.823 to 12.835 min.: VN087646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	198	95.00	47715	117.90	107	144.60	124
80.85	2817	95.90	2933	118.80	368	146.80	66
81.85	566	103.80	315	127.90	159	150.90	51
85.70	52	104.70	52	128.80	58	160.65	112
86.95	1931	105.85	311	129.95	181	171.50	137
87.90	2103	111.00	53	133.10	106	171.90	489
88.50	86	114.80	136	134.75	131	172.70	235
90.85	133	115.70	223	136.55	146	172.90	254
92.00	1516	115.90	137	140.80	555	173.90	32707
92.95	2730	116.75	497	142.70	181	174.90	2932
93.95	7050	117.60	64	142.90	445	175.90	31869

Average of 12.823 to 12.835 min.: VN087646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.95	2024						
206.60	60						
207.10	71						
280.95	112						