


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082825\
Data File : BN037647.D
Acq On : 28 Aug 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

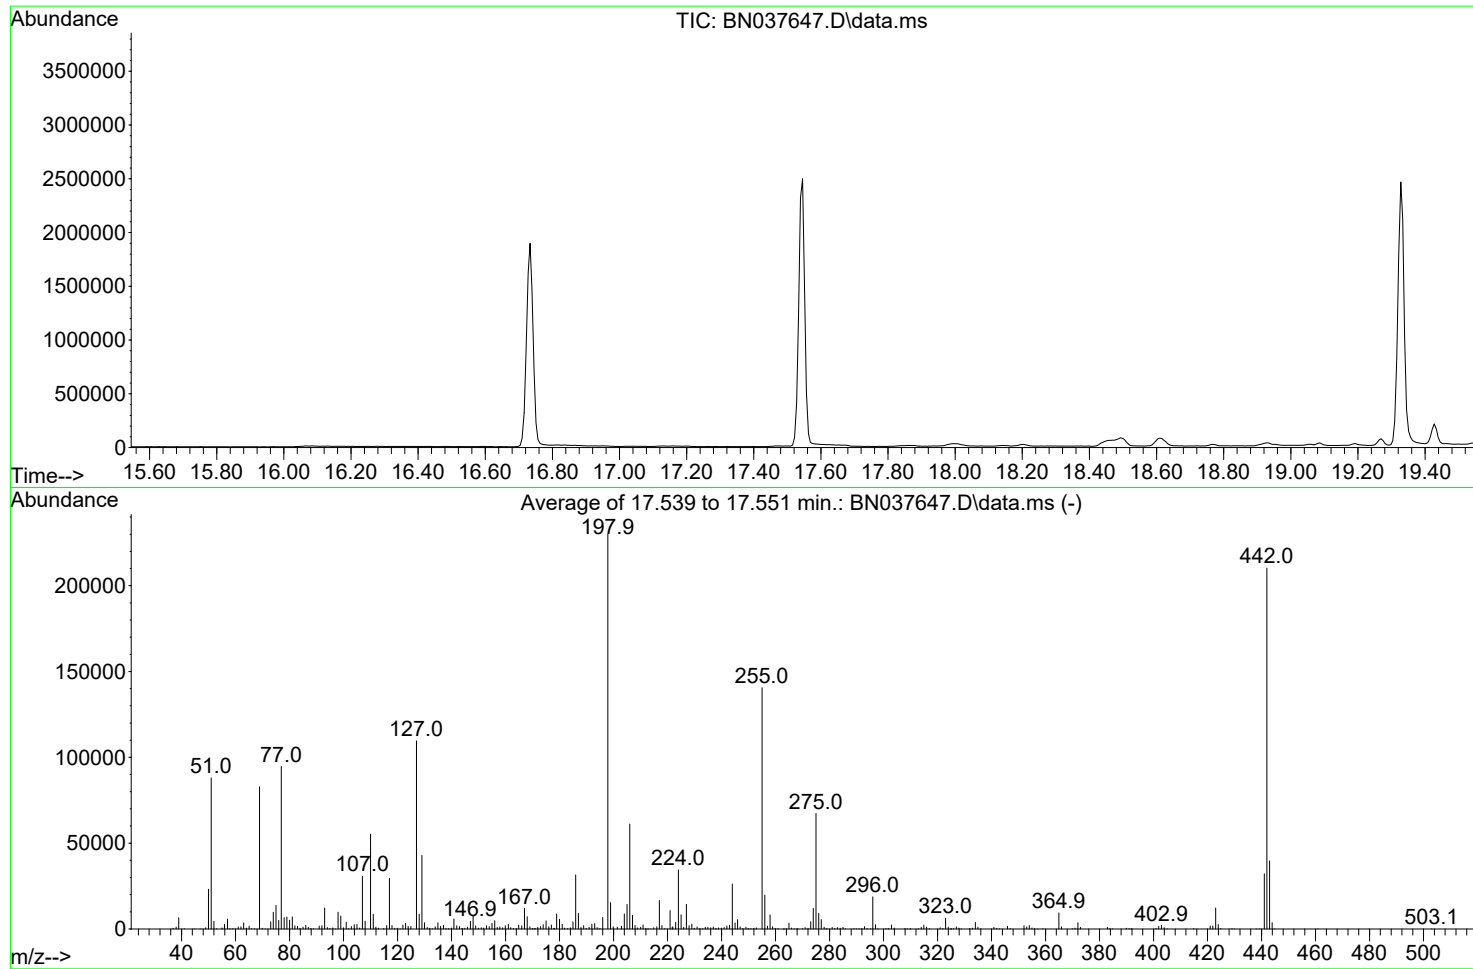

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	82843	PASS
70	69	0.00	2	0.6	459	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	230016	PASS
199	198	5	9	6.7	15374	PASS
365	198	1	100	4.1	9400	PASS
441	443	0.01	150	81.1	32195	PASS
442	442	100	100	100.0	210197	PASS
443	442	15	24	18.9	39704	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/28/2025	BNA_N	<u>BN037647.D</u>
Compound Name	Response	Retention Time
DDT	857903	20.574
DDD	7681	20.12
DDE	1126	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8807	866710	1.02

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082825\
Data File : BN037647.D
Acq On : 28 Aug 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 04:47:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

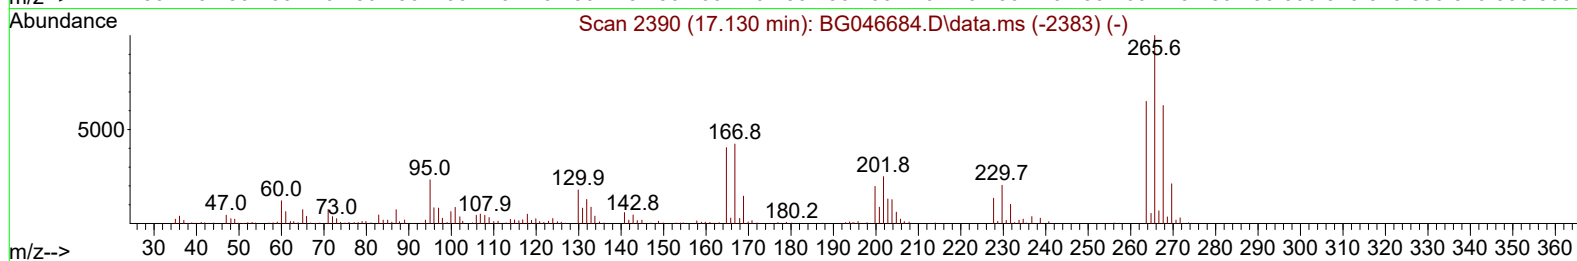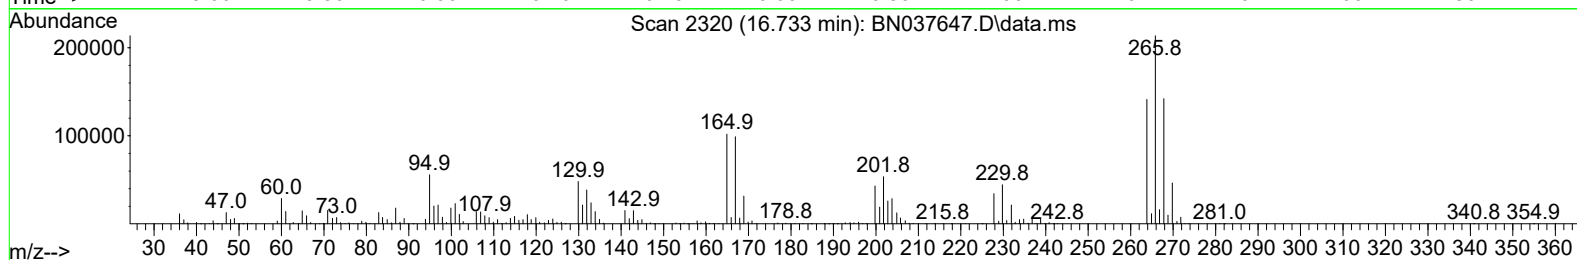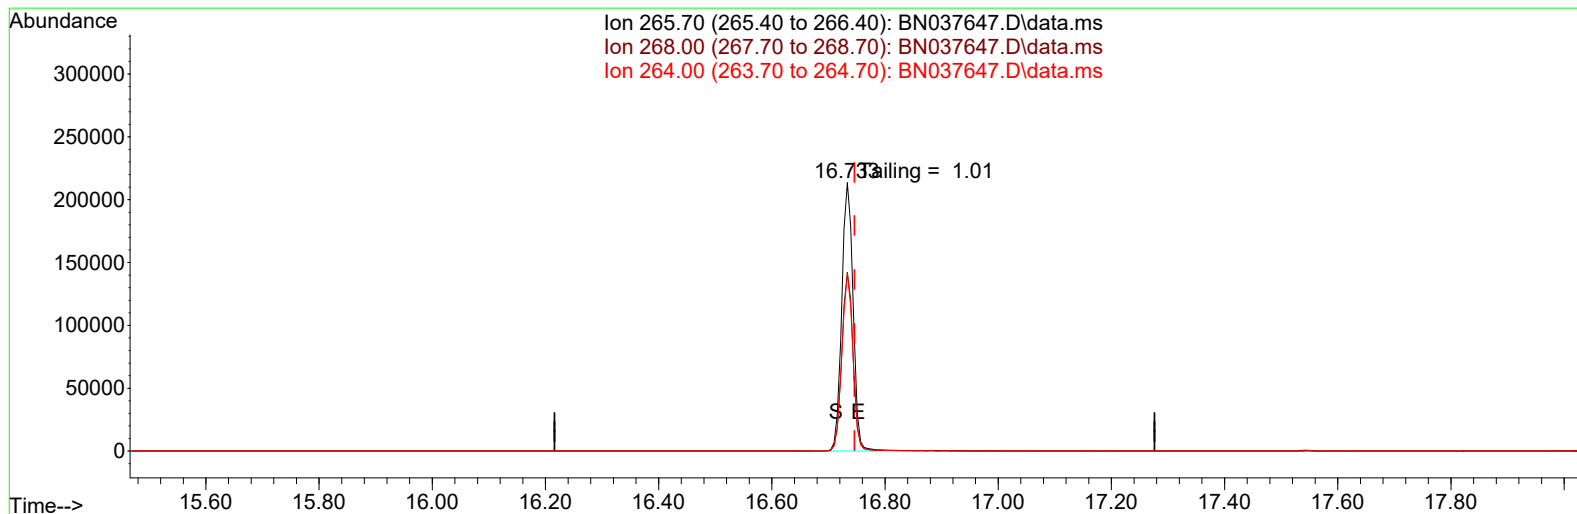

TIC: BN037647.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.013) 27093.45 ng




response 295758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.56
264.00	61.60	66.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082825\
Data File : BN037647.D
Acq On : 28 Aug 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 04:47:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

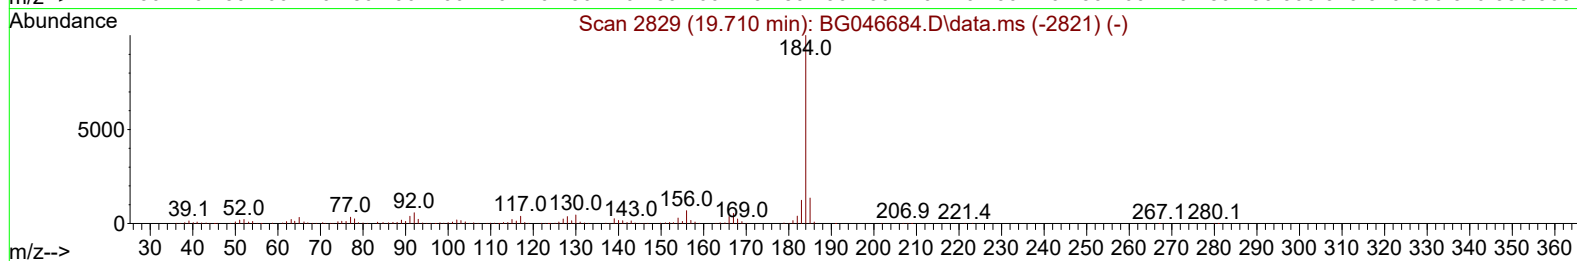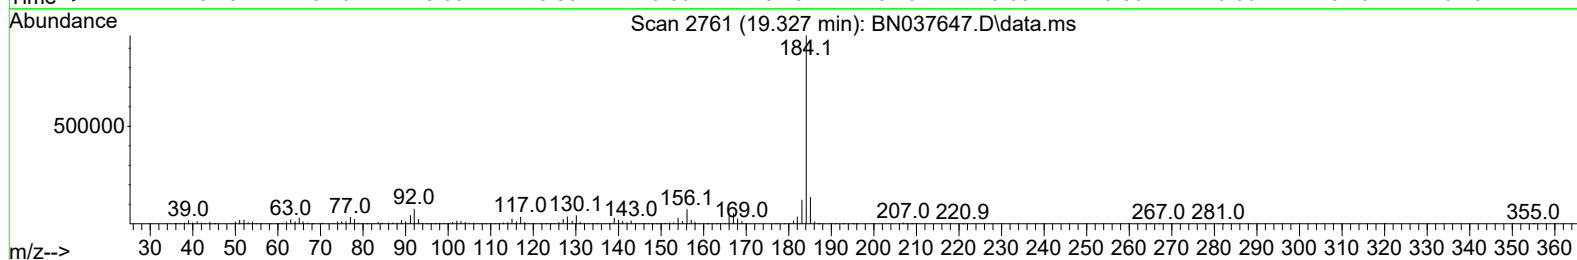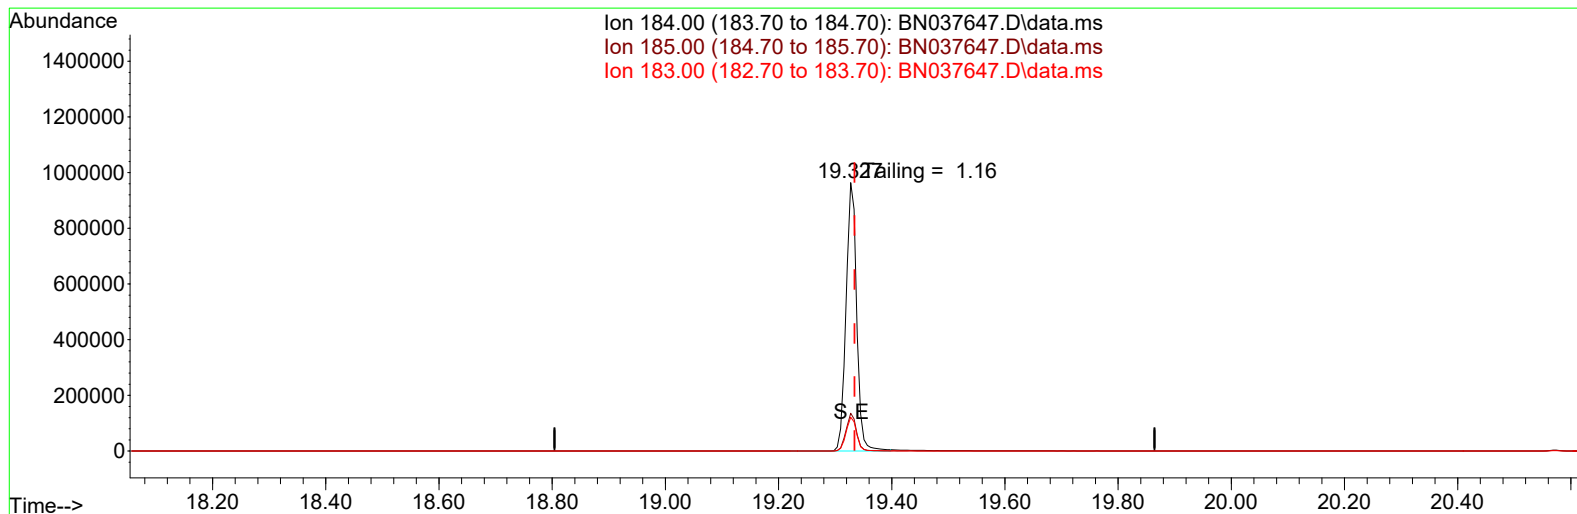

TIC: BN037647.D\data.ms

(77) Benzidine

19.327min (-0.007) 0.00 ng

response 1266888

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.62
0.00	0.00	0.00