
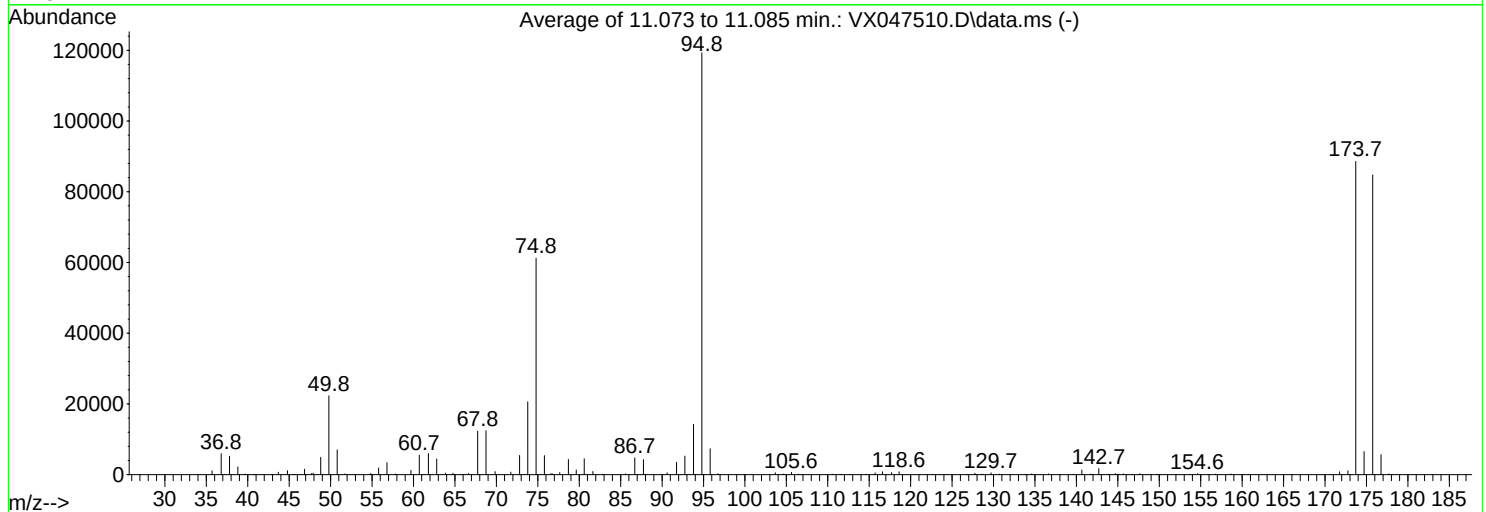


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082525\
Data File : VX047510.D
Acq On : 25 Aug 2025 08:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Title : SW846 8260
Last Update : Mon Aug 18 04:18:28 2025

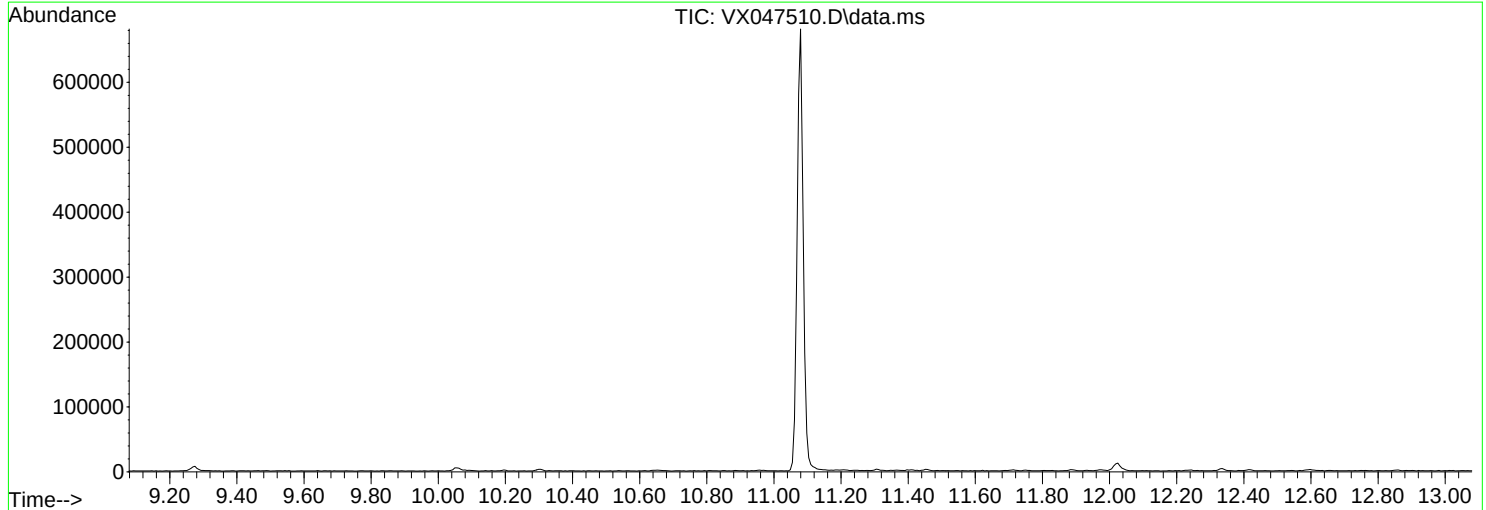

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	22289	PASS
75	95	30	60	51.3	61211	PASS
95	95	100	100	100.0	119288	PASS
96	95	5	9	6.2	7337	PASS
173	174	0.00	2	1.2	1104	PASS
174	95	50	100	74.3	88611	PASS
175	174	5	9	7.4	6518	PASS
176	174	95	101	95.6	84741	PASS
177	176	5	9	6.7	5649	PASS