

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082225\
 Data File : VX047506.D
 Acq On : 22 Aug 2025 18:09
 Operator : JC/MD
 Sample : Q2939-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAGEMENT

Quant Time: Aug 25 01:32:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	213181	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	431357	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	429628	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	224982	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	168690	56.540	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	113.080%
35) Dibromofluoromethane	5.403	113	139409	49.797	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.600%
50) Toluene-d8	8.653	98	481525	48.122	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.240%
62) 4-Bromofluorobenzene	11.079	95	201692	54.622	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	109.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082225\
Data File : VX047506.D
Acq On : 22 Aug 2025 18:09
Operator : JC/MD
Sample : Q2939-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Quant Time: Aug 25 01:32:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




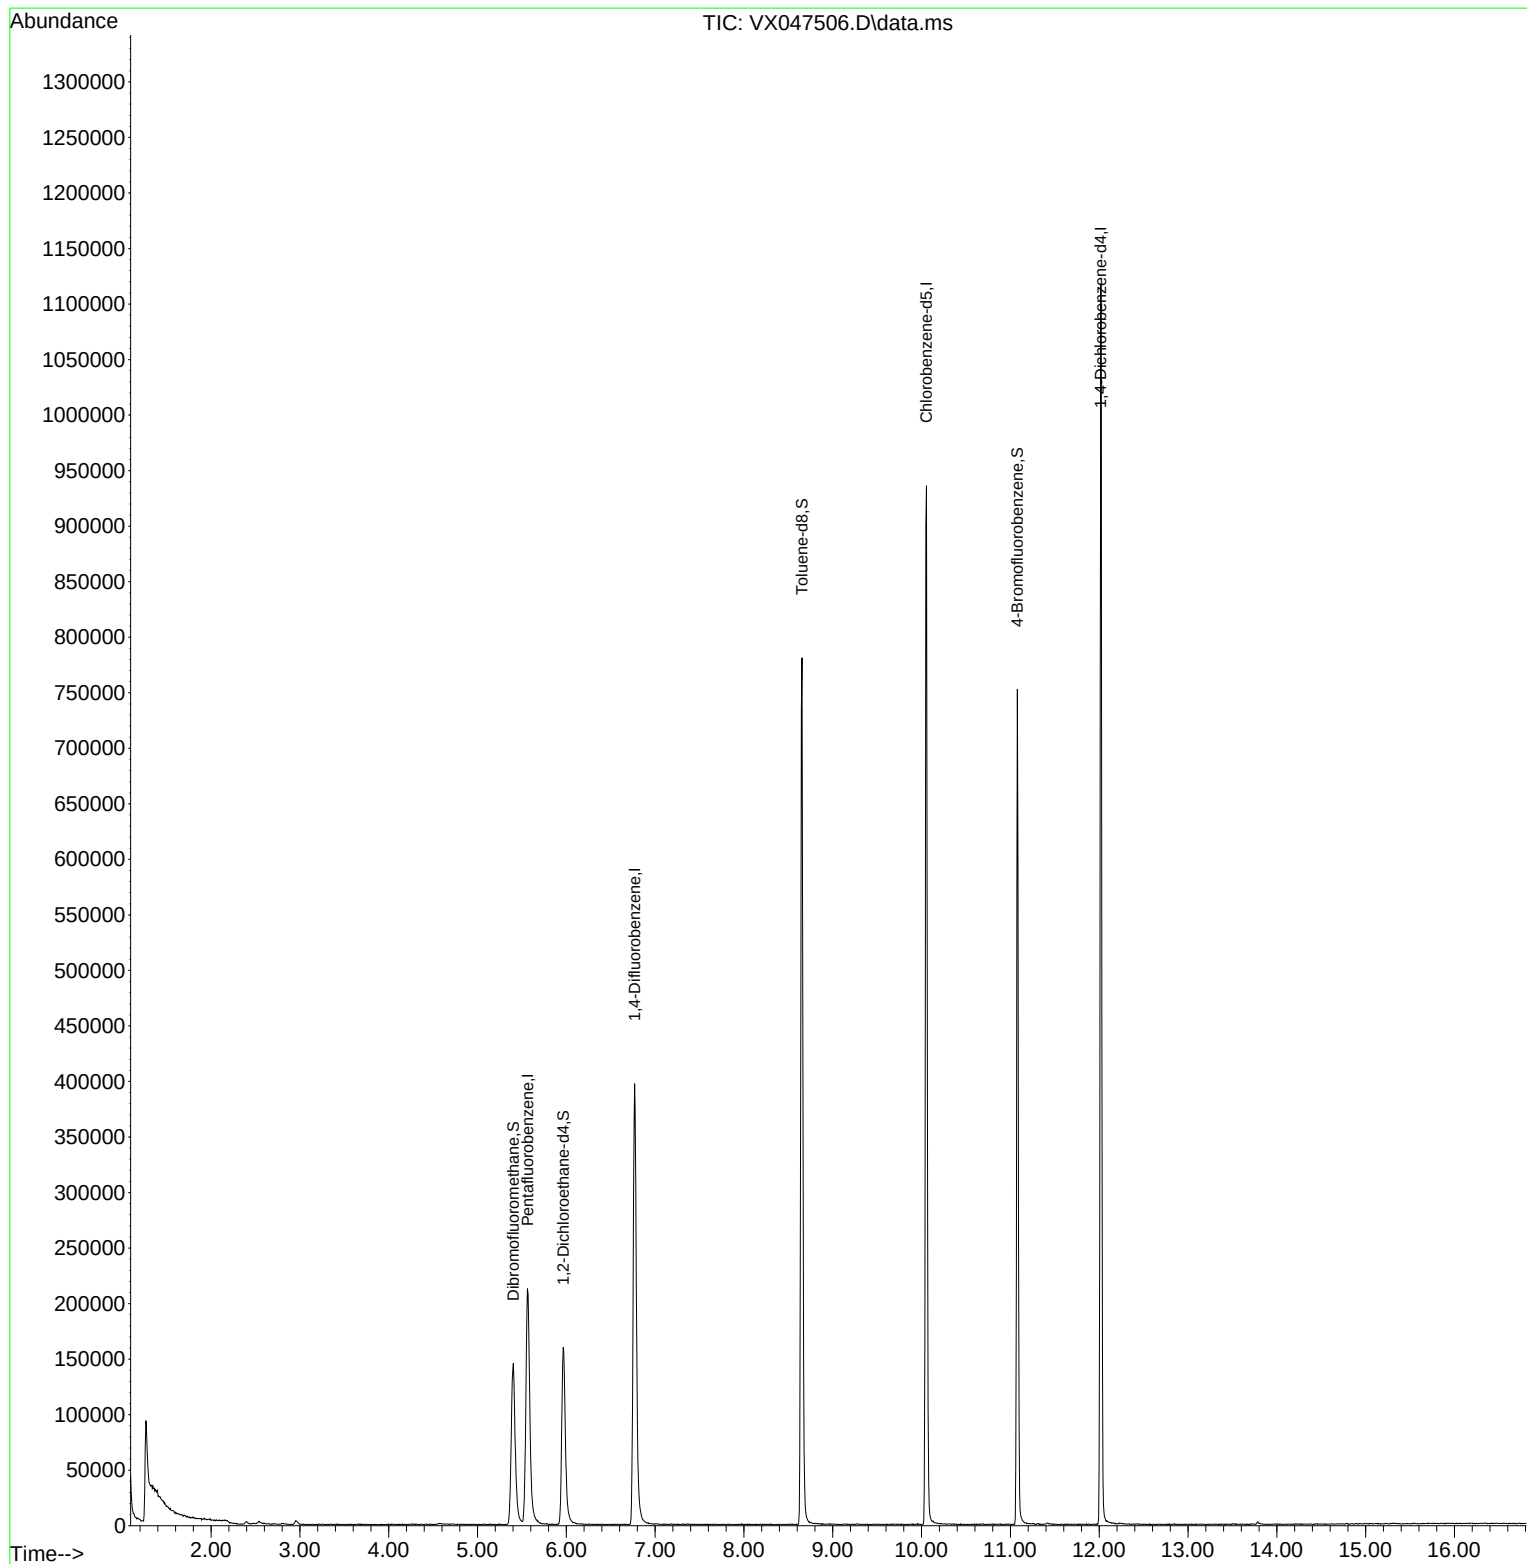


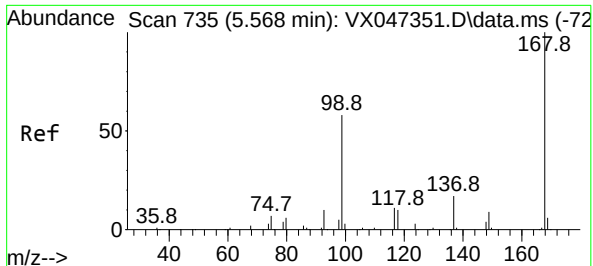

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT


Tgt Ion:168 Resp: 213181
Ion Ratio Lower Upper
168 100
99 59.9 47.9 71.9

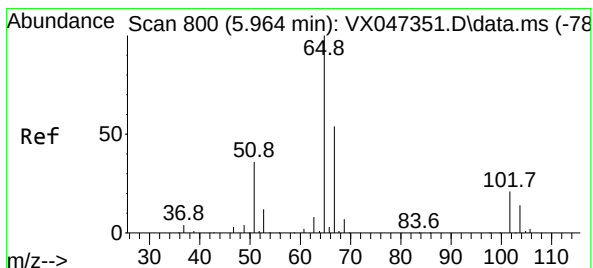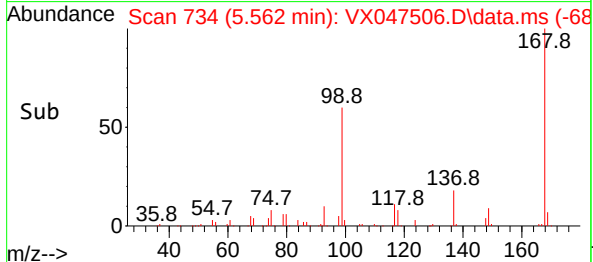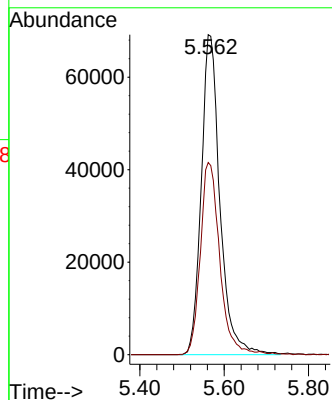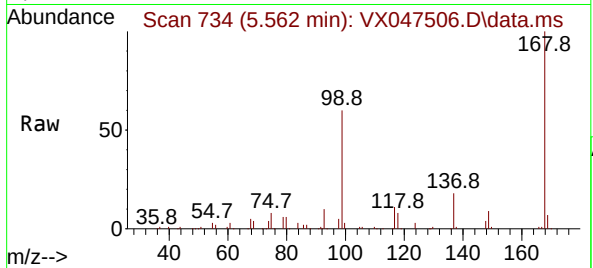

#33
1,2-Dichloroethane-d4
Concen: 56.540 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09

Tgt Ion: 65 Resp: 168690
Ion Ratio Lower Upper
65 100
67 51.9 0.0 106.0


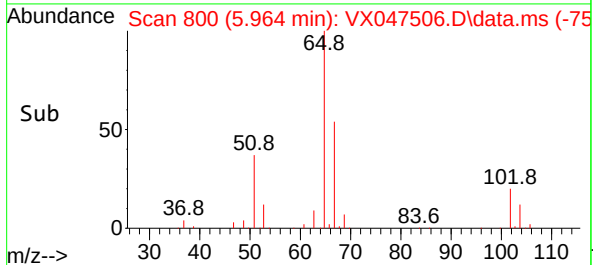
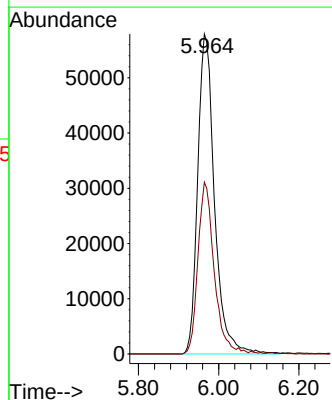
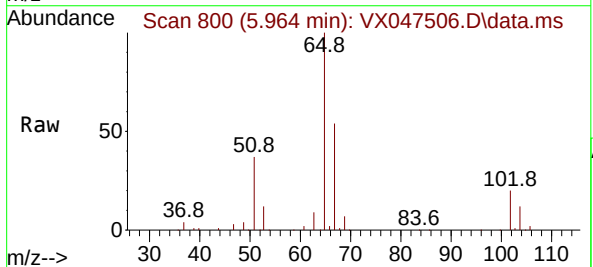


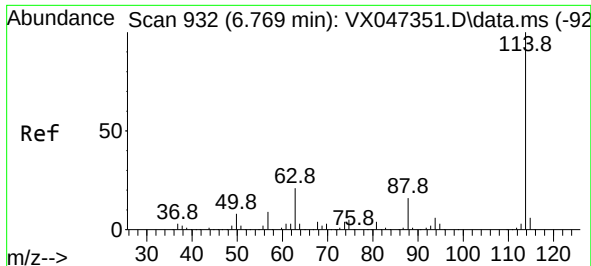

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT


Tgt Ion:114 Resp: 431357
Ion Ratio Lower Upper
114 100
63 25.1 0.0 42.4
88 16.2 0.0 33.0

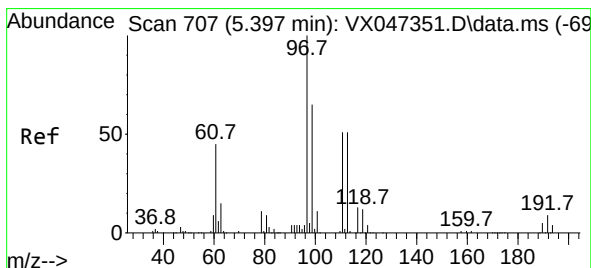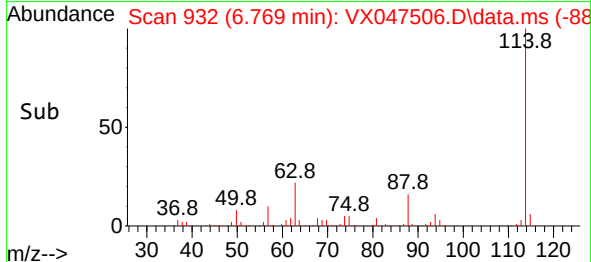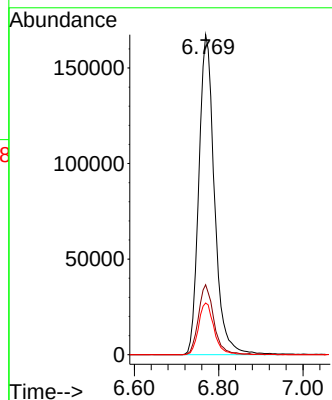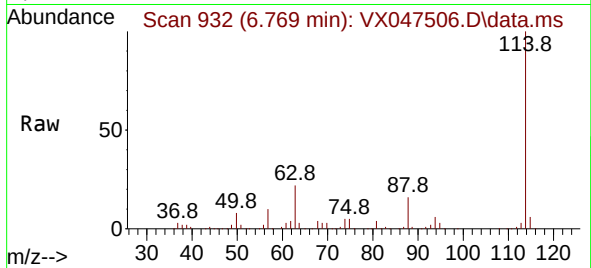

#35
Dibromofluoromethane
Concen: 49.797 ug/l
RT: 5.403 min Scan# 708
Delta R.T. 0.006 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09

Tgt Ion:113 Resp: 139409
Ion Ratio Lower Upper
113 100
111 100.8 81.4 122.2
192 17.5 14.1 21.1


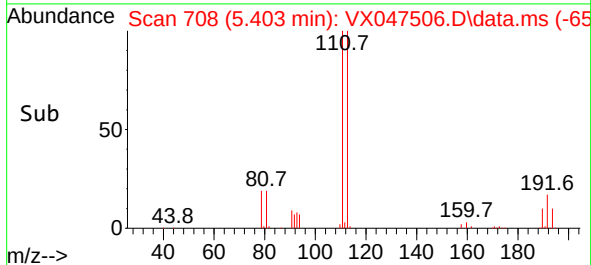
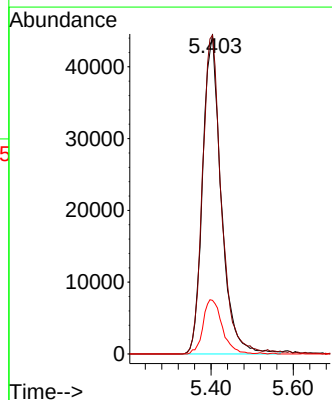
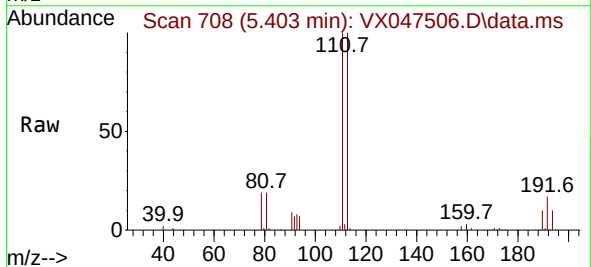


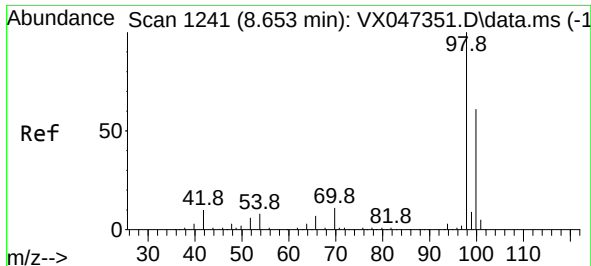

#50
Toluene-d8
Concen: 48.122 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09




Instrument : MSVOA_X
ClientSampleId : STORAGE-BLANK-SAMPLE-MANAGEMENT


Tgt Ion: 98 Resp: 481525
Ion Ratio Lower Upper
98 100
100 65.3 53.9 80.9

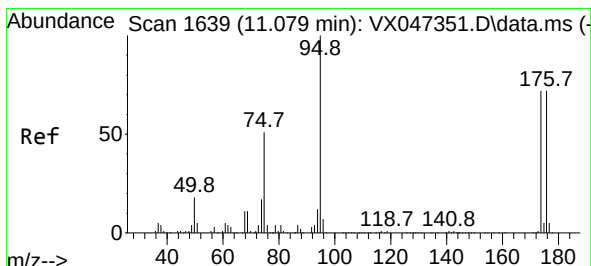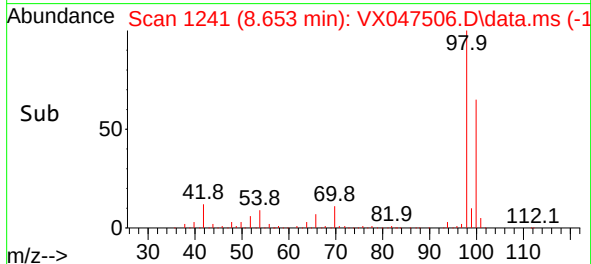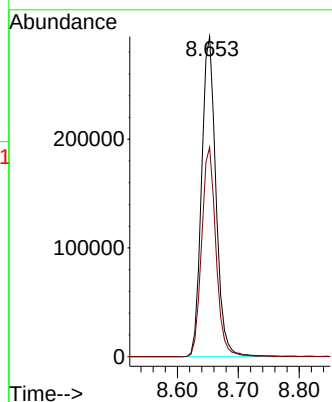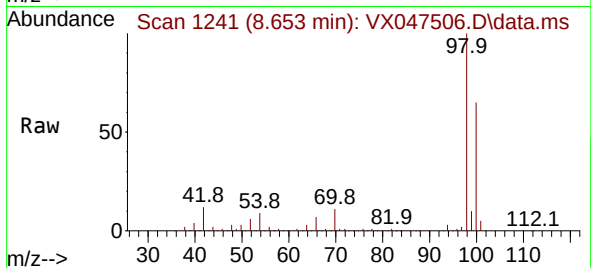

#62
4-Bromofluorobenzene
Concen: 54.622 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09

Tgt Ion: 95 Resp: 201692
Ion Ratio Lower Upper
95 100
174 73.9 0.0 148.0
176 71.6 0.0 145.4


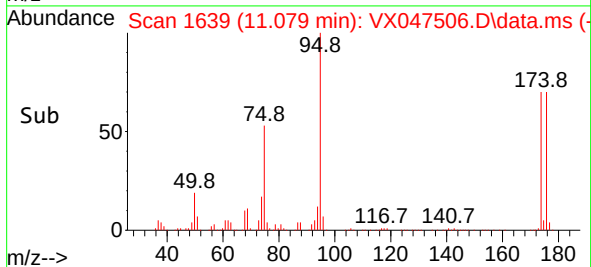
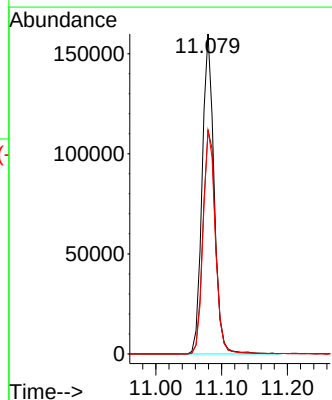
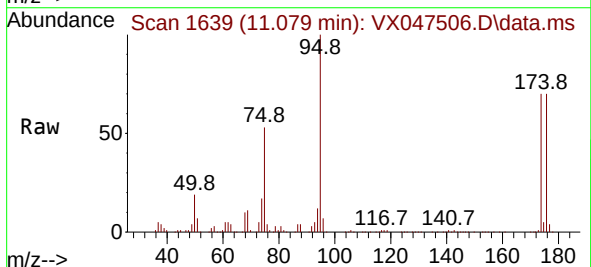


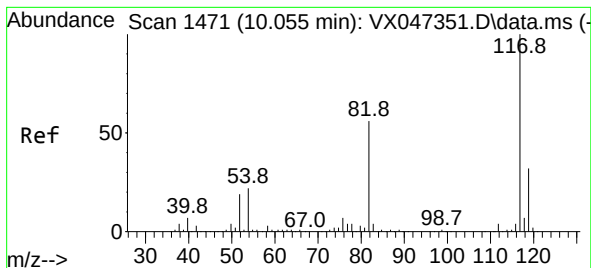

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Tgt Ion:117 Resp: 429628
Ion Ratio Lower Upper
117 100
82 55.7 45.0 67.4
119 32.1 25.8 38.8

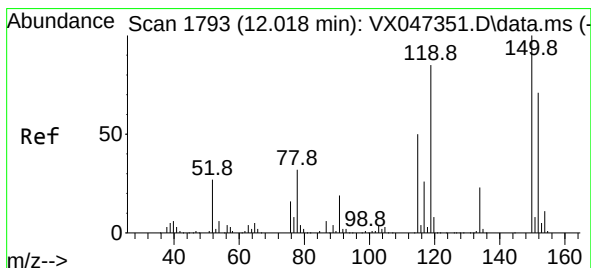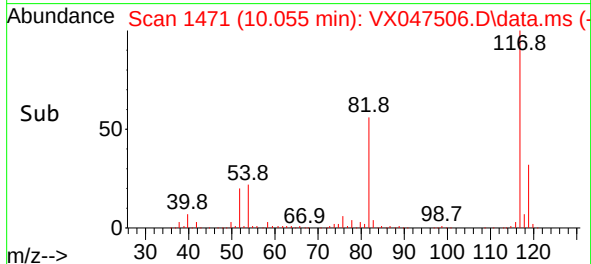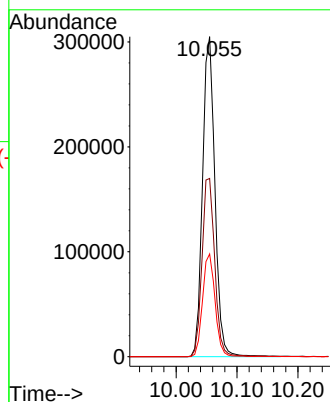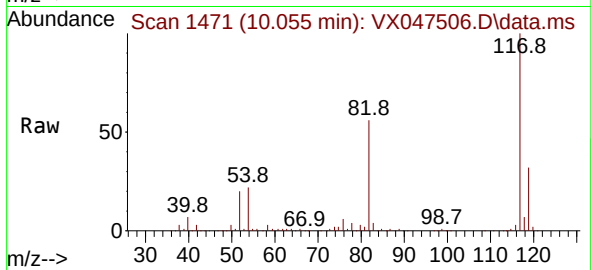

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047506.D
Acq: 22 Aug 2025 18:09

Tgt Ion:152 Resp: 224982
Ion Ratio Lower Upper
152 100
115 61.6 44.6 133.8
150 157.3 0.0 349.8

