


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN082825\  
Data File : VN087675.D  
Acq On : 28 Aug 2025 11:00  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N082125W.M  
Title : SW846 8260  
Last Update : Fri Aug 22 02:55:42 2025

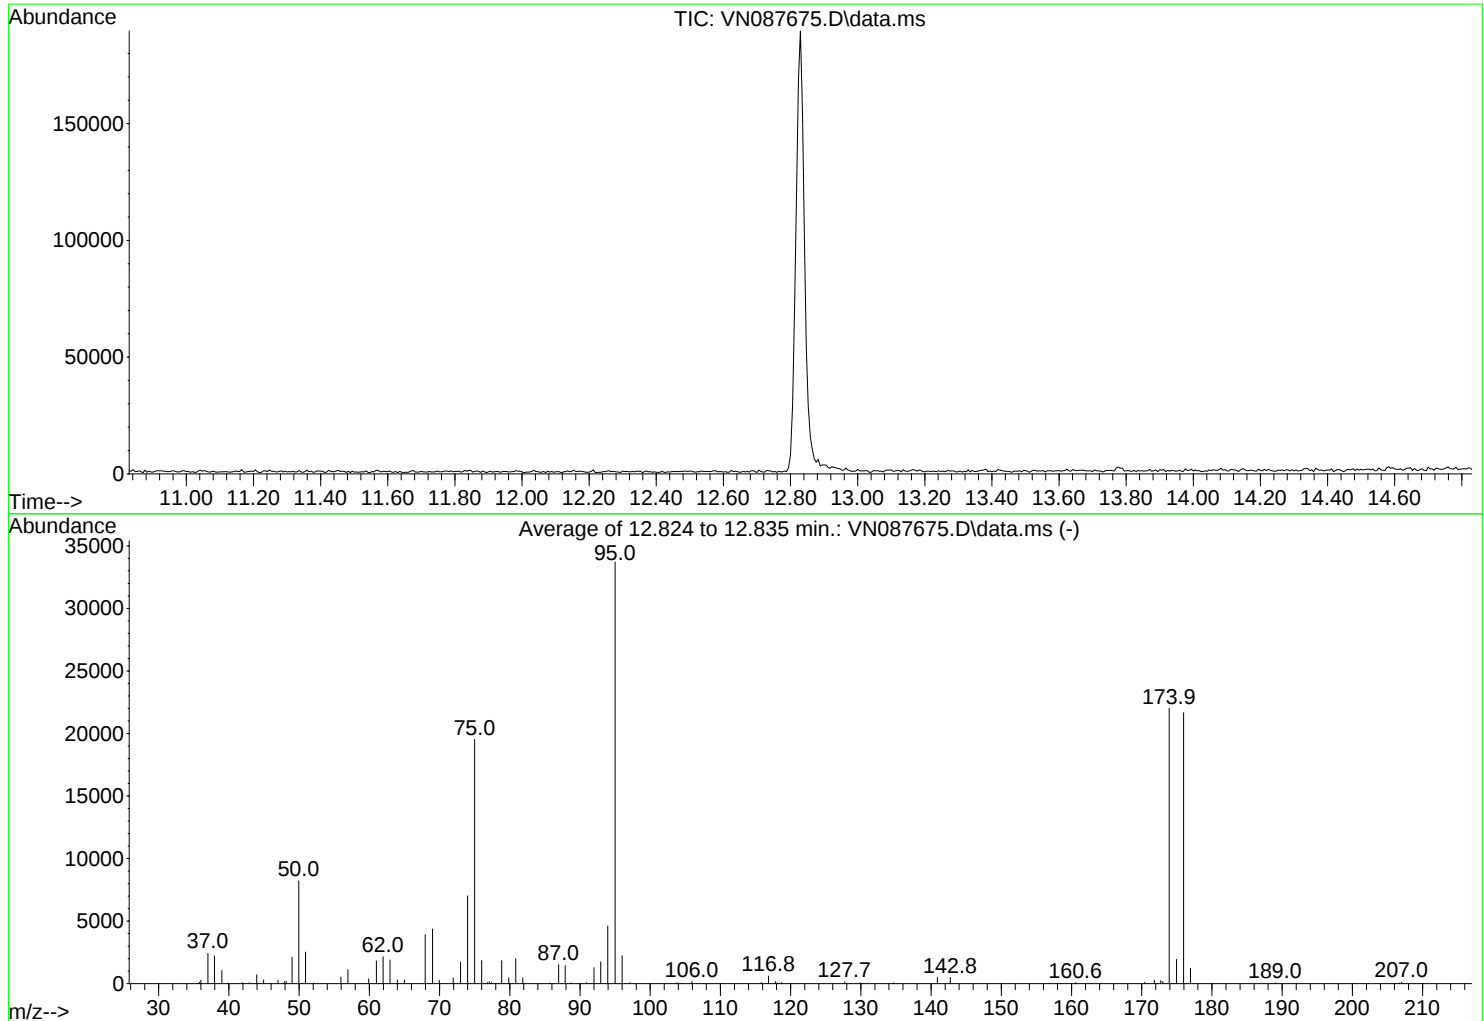

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 24.4         | 8213       | PASS                |
| 75             | 95              | 30              | 60              | 57.9         | 19520      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 33725      | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 2230       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 243        | PASS                |
| 174            | 95              | 50              | 100             | 65.2         | 22000      | PASS                |
| 175            | 174             | 5               | 9               | 8.8          | 1947       | PASS                |
| 176            | 174             | 95              | 101             | 98.5         | 21661      | PASS                |
| 177            | 176             | 5               | 9               | 5.7          | 1232       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.80 | 113    | 47.90 | 161    | 62.95 | 1895   | 76.80 | 81     |
| 36.00 | 277    | 48.15 | 218    | 64.00 | 296    | 77.10 | 15     |
| 37.00 | 2421   | 49.00 | 2103   | 65.00 | 292    | 77.40 | 8      |
| 37.95 | 2217   | 49.95 | 8213   | 67.95 | 3924   | 78.85 | 184    |
| 39.00 | 1053   | 50.90 | 2518   | 69.00 | 4369   | 79.85 | 460    |
| 39.80 | 54     | 52.10 | 52     | 69.95 | 287    | 80.85 | 1997   |
| 41.90 | 75     | 55.95 | 539    | 71.95 | 447    | 81.85 | 462    |
| 42.90 | 67     | 56.95 | 1119   | 73.00 | 1711   | 85.70 | 54     |
| 43.95 | 706    | 59.90 | 385    | 74.00 | 7007   | 86.95 | 1525   |
| 44.95 | 290    | 61.00 | 1820   | 75.00 | 19520  | 87.90 | 1440   |
| 47.00 | 257    | 61.95 | 2153   | 76.00 | 1846   | 88.70 | 68     |

Average of 12.824 to 12.835 min.: VN087675.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 90.90  | 89     | 117.85 | 173    | 172.70 | 243    |     |        |
| 92.00  | 1281   | 118.10 | 53     | 173.00 | 164    |     |        |
| 92.95  | 1738   | 118.70 | 84     | 173.90 | 22000  |     |        |
| 93.95  | 4607   | 127.70 | 144    | 174.95 | 1947   |     |        |
| 95.00  | 33725  | 129.90 | 58     | 175.95 | 21661  |     |        |
| 96.00  | 2230   | 134.70 | 64     | 176.95 | 1232   |     |        |
| 97.10  | 72     | 140.90 | 486    | 189.00 | 65     |     |        |
| 103.80 | 81     | 142.75 | 488    | 206.70 | 55     |     |        |
| 105.95 | 171    | 160.60 | 86     | 207.00 | 109    |     |        |
| 115.80 | 89     | 170.40 | 85     |        |        |     |        |
| 116.85 | 616    | 171.80 | 268    |        |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB