


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082925\
Data File : VN087692.D
Acq On : 29 Aug 2025 11:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

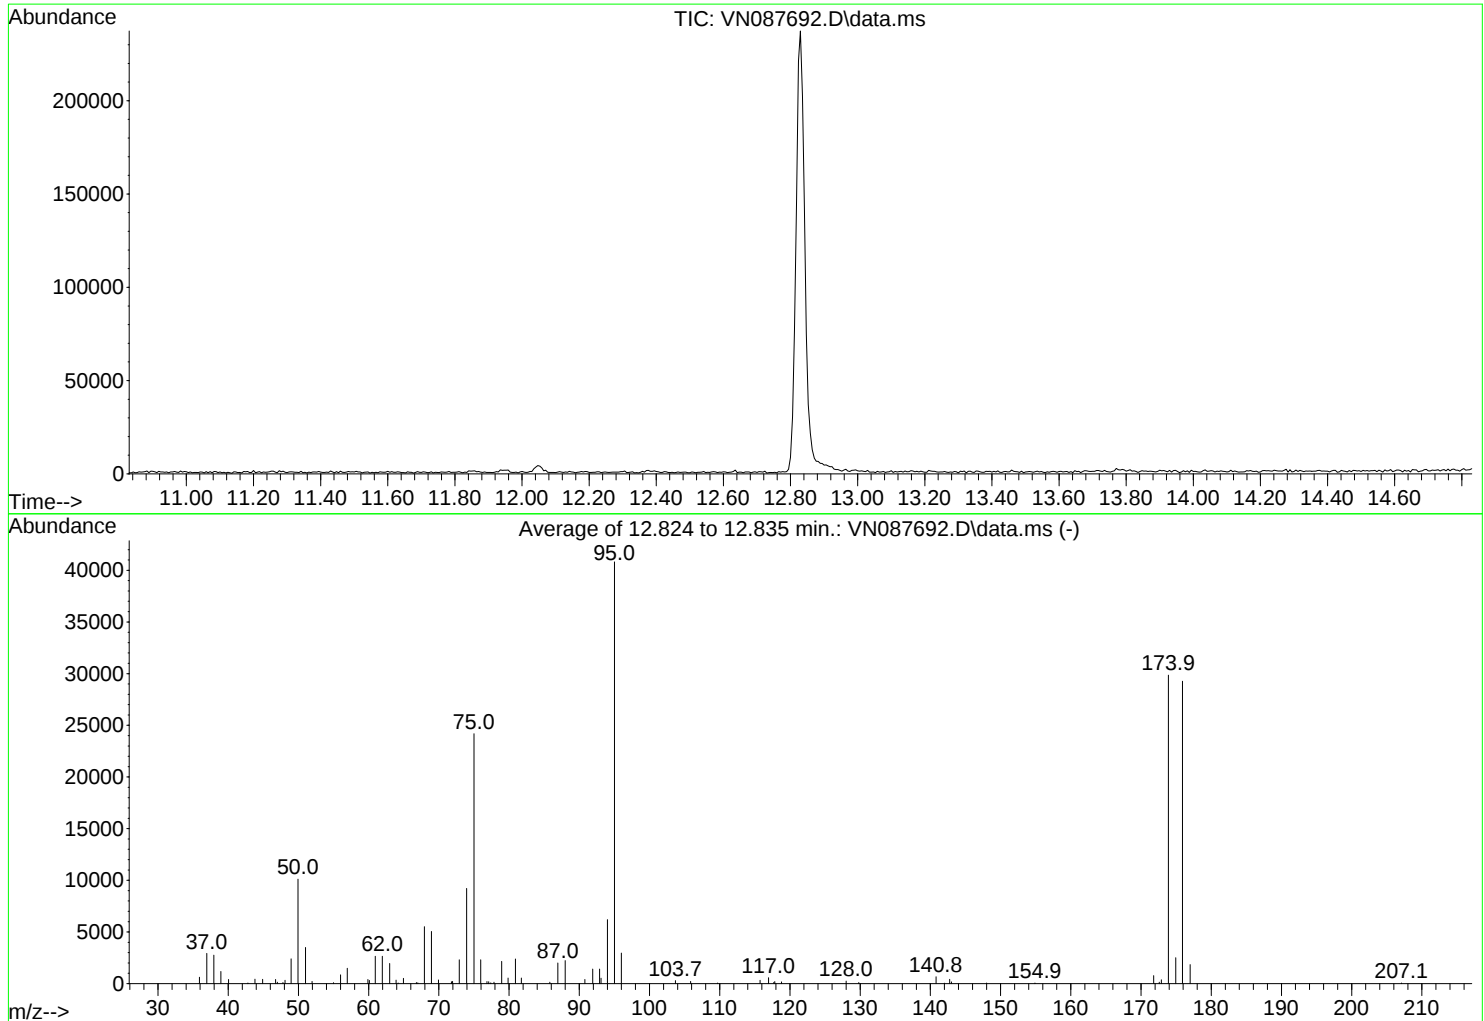

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	10113	PASS
75	95	30	60	59.3	24195	PASS
95	95	100	100	100.0	40819	PASS
96	95	5	9	7.3	2961	PASS
173	174	0.00	2	1.2	372	PASS
174	95	50	100	73.1	29851	PASS
175	174	5	9	8.4	2509	PASS
176	174	95	101	98.1	29272	PASS
177	176	5	9	6.3	1838	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	623	48.10	331	61.95	2647	71.95	221
36.95	2925	48.95	2403	63.00	1956	72.90	2306
37.95	2757	49.95	10113	63.90	334	73.95	921
38.95	1179	51.00	3496	64.20	57	75.00	2419
40.05	411	51.95	217	64.95	513	75.95	2306
42.80	65	55.00	98	66.80	107	76.85	197
43.80	435	56.00	856	67.00	84	77.10	185
44.90	420	56.95	1483	67.95	5511	77.40	82
46.75	404	59.90	396	68.95	5042	77.85	145
47.00	143	60.10	307	69.95	362	78.95	2153
47.80	117	60.95	2647	71.80	187	79.85	540

Average of 12.824 to 12.835 min.: VN087692.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	2382	96.00	2961	140.80	671	175.90	29272
81.75	536	103.70	292	142.00	54	177.00	1838
85.80	139	105.85	214	142.75	412	207.10	56
86.95	1998	109.70	67	143.00	177		
88.00	2230	115.75	321	148.00	63		
90.80	401	116.95	569	154.90	62		
91.90	1411	117.70	124	171.80	777		
92.90	1404	117.85	197	172.60	146		
93.10	521	118.80	179	172.90	372		
94.00	6188	128.00	242	173.90	29851		
95.00	40819	129.80	117	174.95	2509		

Instrument :

MSVOA_N

ClientSampleId :

BFB