
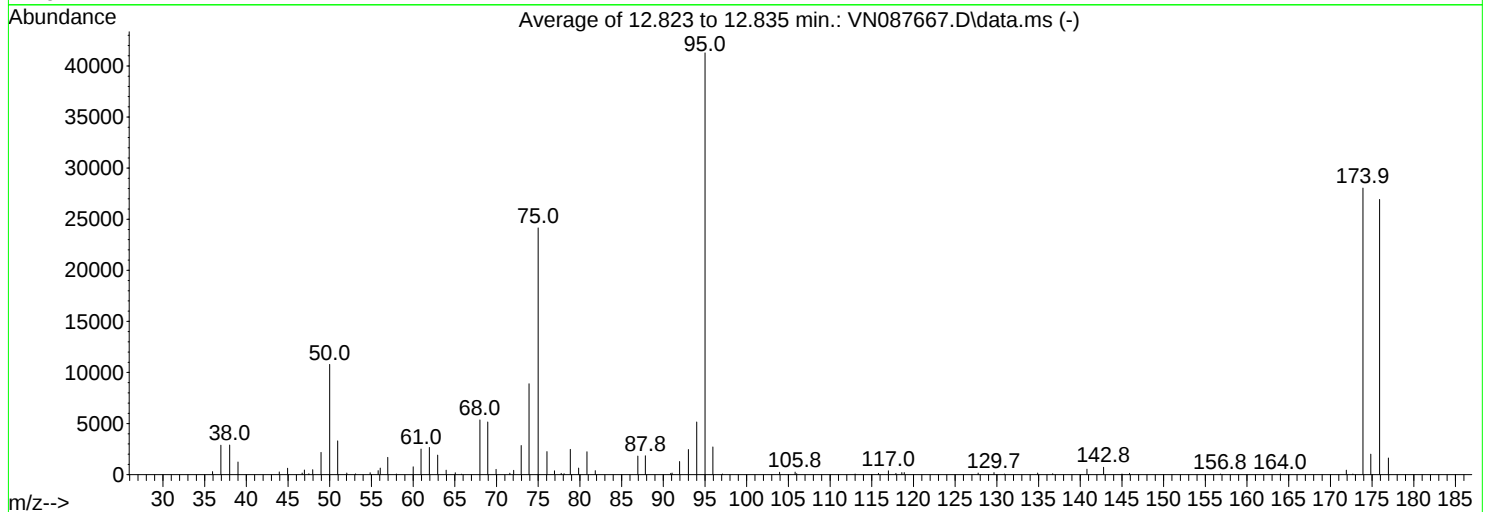


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082625\
Data File : VN087667.D
Acq On : 26 Aug 2025 12:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

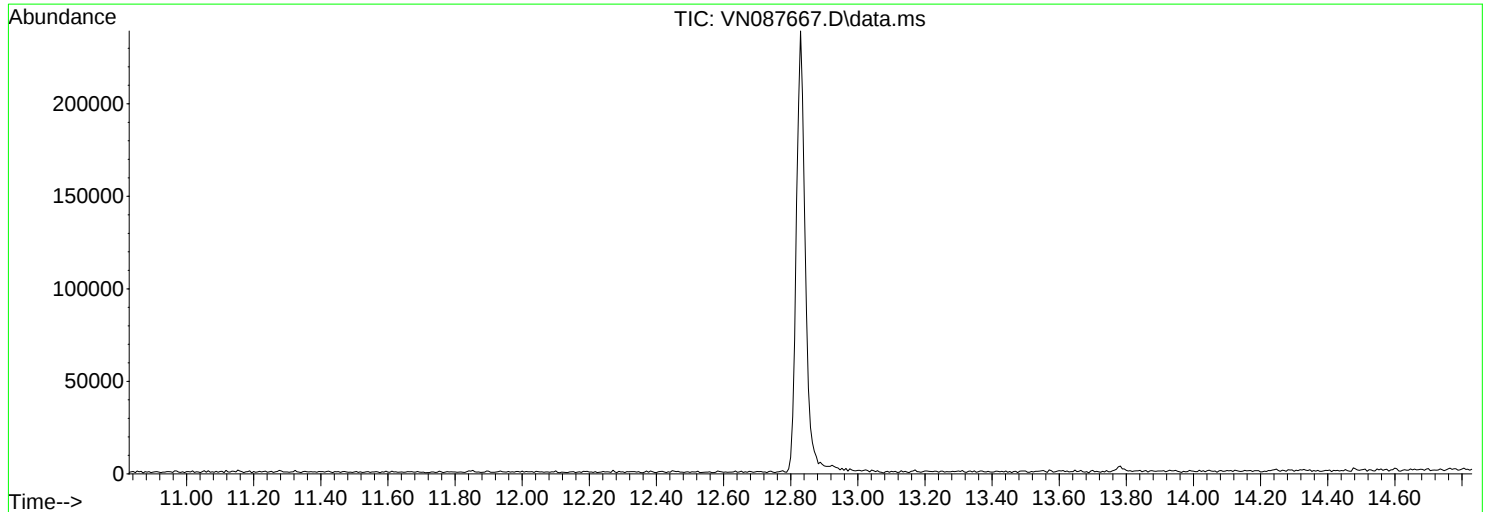

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.1	10787	PASS
75	95	30	60	58.5	24157	PASS
95	95	100	100	100.0	41285	PASS
96	95	5	9	6.6	2707	PASS
173	174	0.00	2	0.2	65	PASS
174	95	50	100	67.9	28043	PASS
175	174	5	9	7.2	2010	PASS
176	174	95	101	96.0	26933	PASS
177	176	5	9	6.0	1625	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	296	50.00	10787	61.95	2660	73.90	889
36.95	2879	50.95	3313	62.95	1912	75.00	2415
38.00	2894	52.05	162	63.95	432	76.05	224
39.00	1234	53.10	74	65.05	192	76.95	37
43.95	270	54.85	183	65.80	54	77.75	118
44.95	627	55.80	388	68.00	5351	78.10	100
46.70	158	56.05	636	68.95	5157	78.85	2481
46.95	460	56.95	1695	69.95	522	79.85	636
47.50	88	58.00	65	71.60	142	80.85	2241
47.95	489	60.00	767	72.05	426	81.85	398
48.95	2172	60.95	2511	72.95	2853	86.95	1810

Average of 12.823 to 12.835 min.: VN087667.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.85	1851	106.00	94	136.70	90	175.90	26933
90.90	128	113.00	57	140.80	526	176.95	1625
91.05	164	115.80	118	142.80	715		
91.95	1289	117.00	383	145.00	70		
93.00	2456	117.90	133	145.90	125		
94.00	5156	118.60	203	156.80	64		
95.00	41285	118.90	211	164.00	60		
95.95	2707	127.75	157	171.90	441		
97.10	69	129.65	207	172.70	65		
103.95	235	130.90	61	173.90	28043		
105.80	255	134.90	163	174.85	2010		

Instrument :

MSVOA_N

ClientSampleId :

BFB