


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090225\
Data File : BG064239.D
Acq On : 2 Sep 2025 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

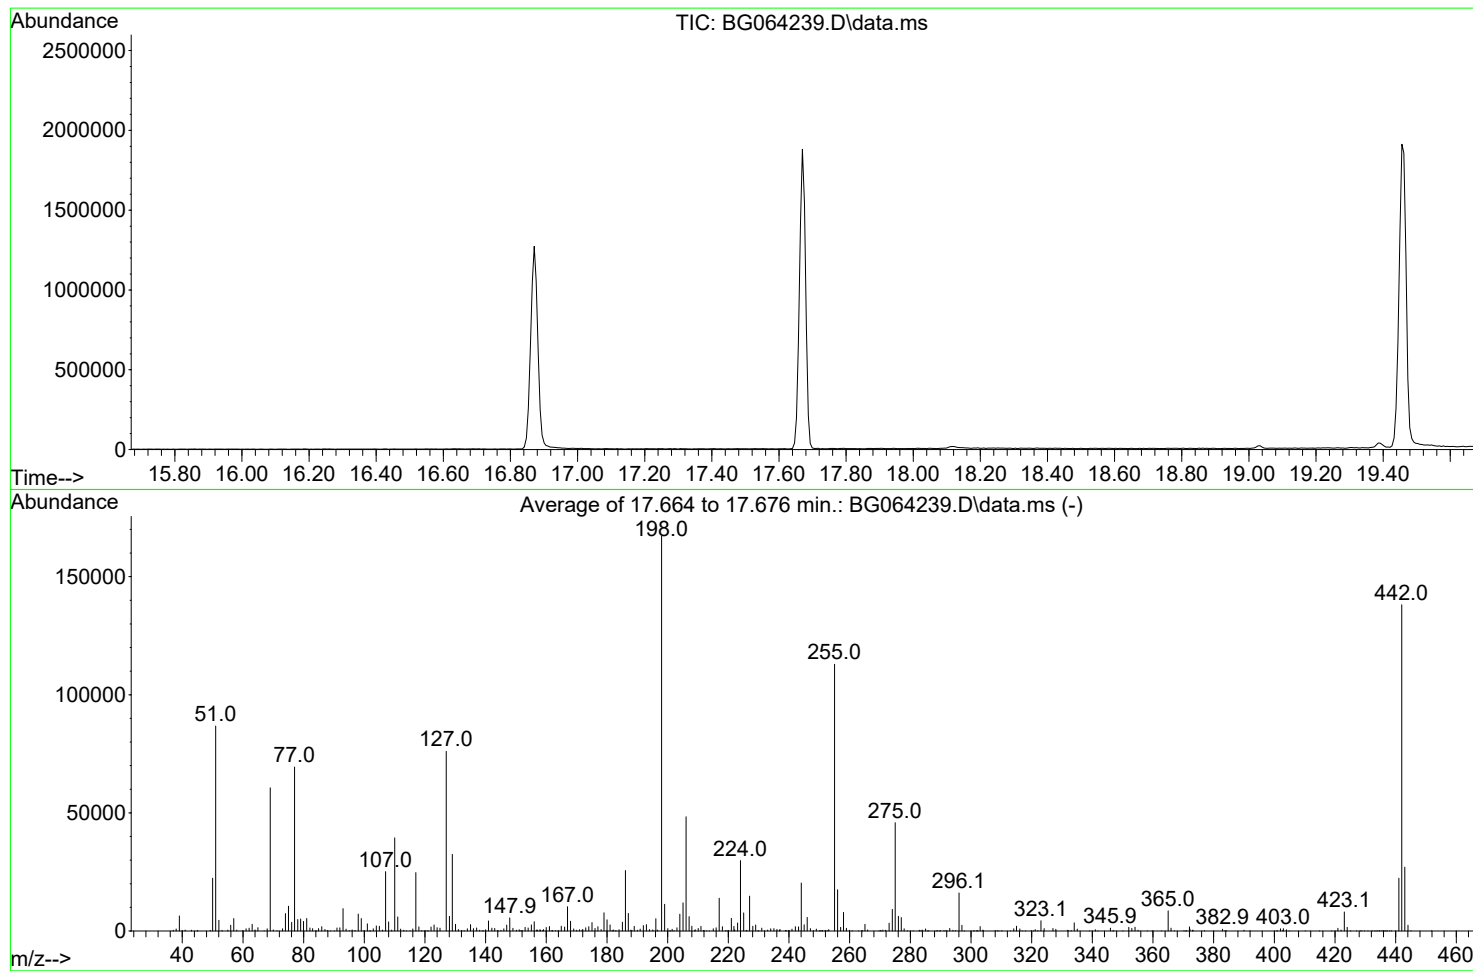

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	927	PASS
69	69	100	100	100.0	60645	PASS
70	69	0.00	2	0.8	507	PASS
197	198	0.00	2	0.2	414	PASS
198	198	100	100	100.0	167125	PASS
199	198	5	9	6.8	11307	PASS
365	198	1	100	5.1	8555	PASS
441	443	0.01	150	82.8	22382	PASS
442	442	100	100	100.0	138120	PASS
443	442	15	24	19.6	27024	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/2/2025	BNA_G	BG064239.D
Compound Name	Response	Retention Time
DDT	557554	20.69
DDD	12593	20.249
DDE	584	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13177	570731	2.31

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090225\
Data File : BG064239.D
Acq On : 2 Sep 2025 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 02 12:14:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

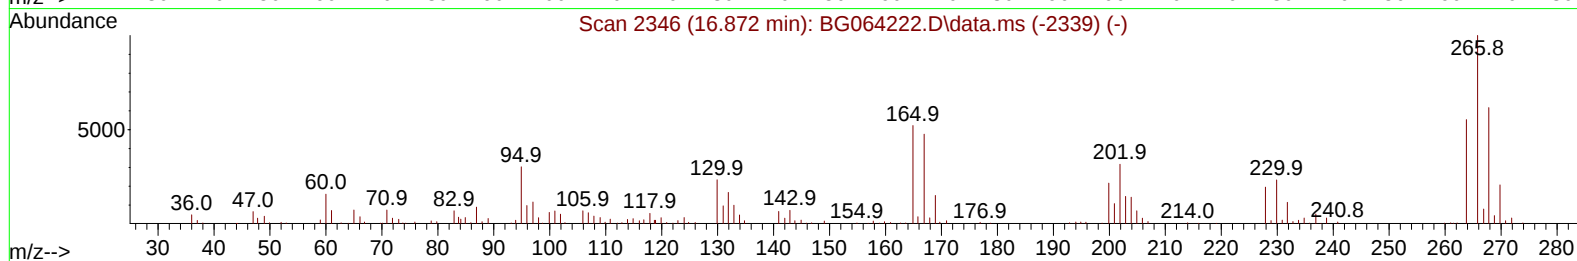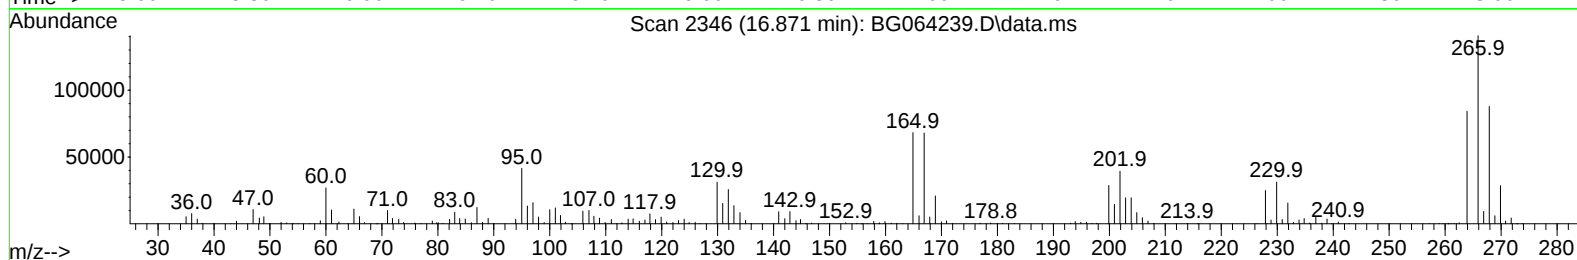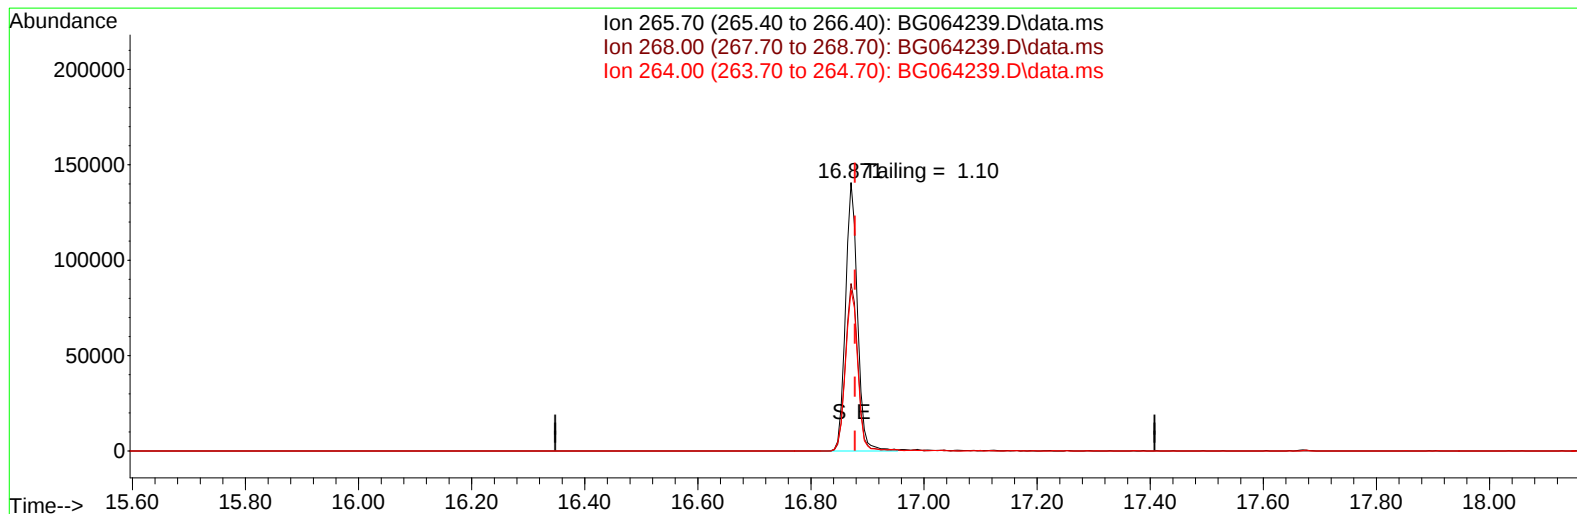

TIC: BG064239.D\data.ms

(70) Pentachlorophenol (C)

16.871min (-0.007) 208165.51 ng




response 206933

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.39
264.00	55.40	59.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090225\
Data File : BG064239.D
Acq On : 2 Sep 2025 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 02 12:14:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

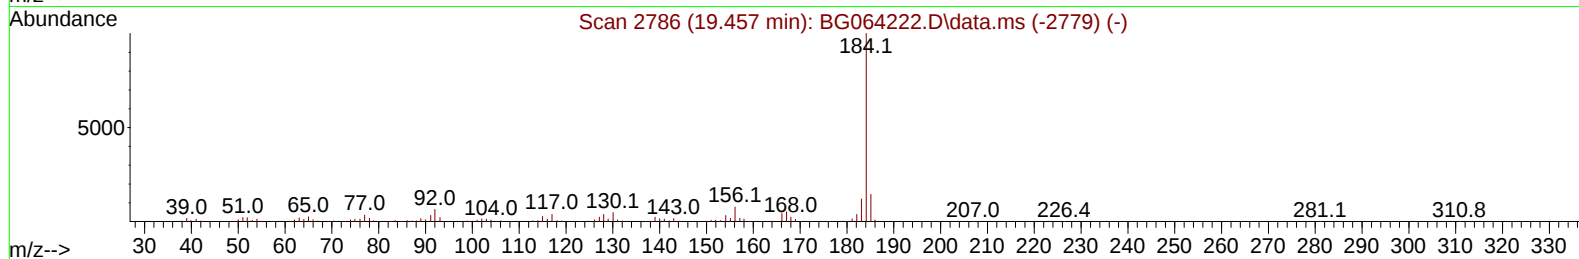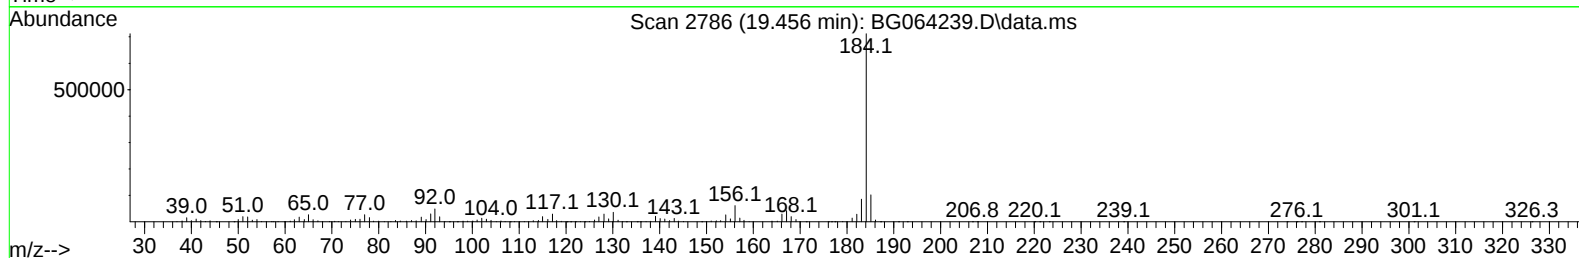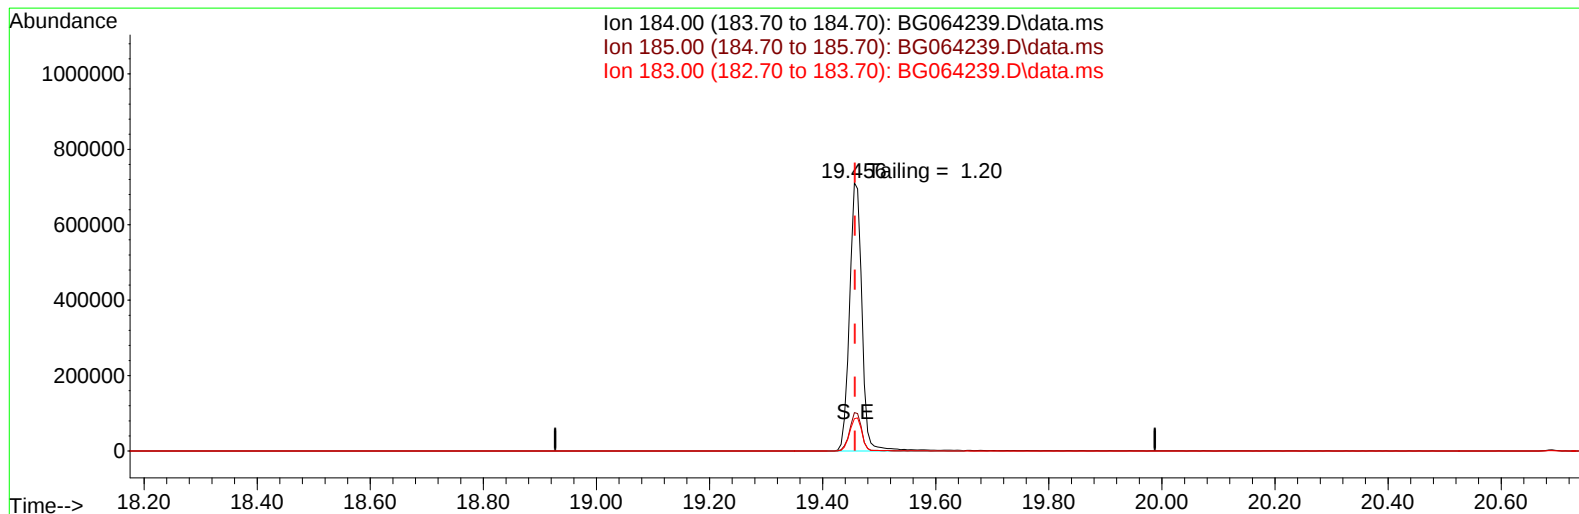

TIC: BG064239.D\data.ms

(77) Benzidine

19.456min (-0.001) 576729.23 ng

response 1079780

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	12.10	12.05
0.00	0.00	0.00