
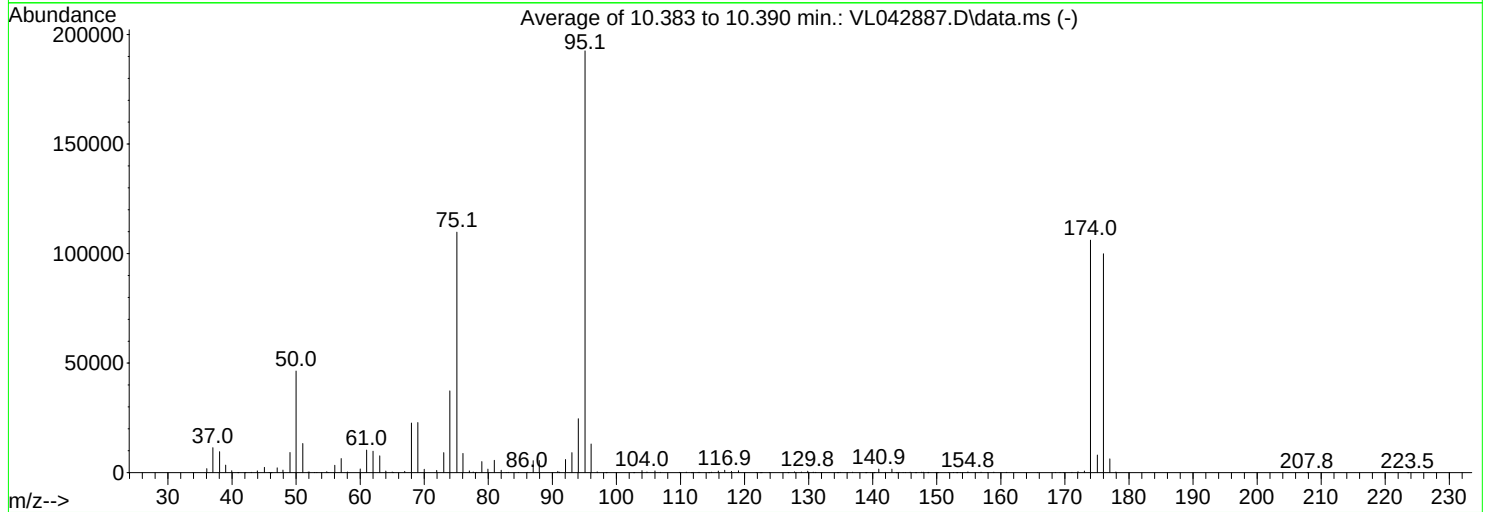


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090425\
Data File : VL042887.D
Acq On : 04 Sep 2025 09:58
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Aug 14 02:12:54 2025

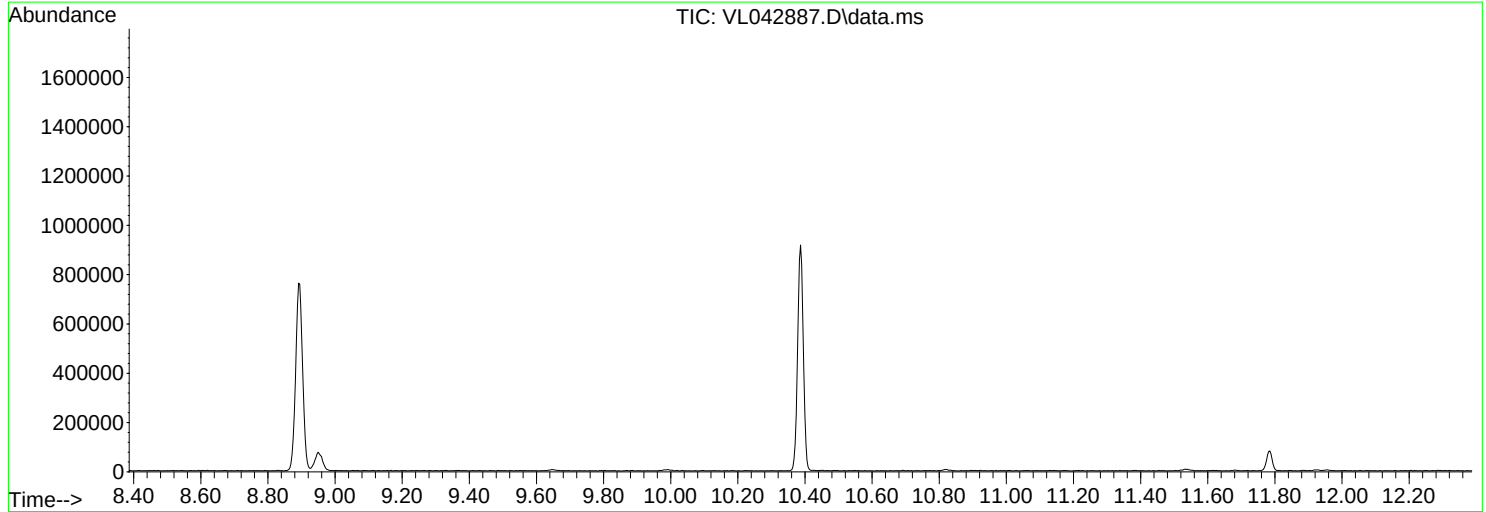

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	46379	PASS
75	95	30	66	57.0	109781	PASS
95	95	100	100	100.0	192555	PASS
96	95	5	9	6.8	13091	PASS
173	174	0.00	2	0.7	765	PASS
174	95	50	120	55.1	106109	PASS
175	174	4	9	7.6	8017	PASS
176	174	93	101	94.1	99893	PASS
177	176	5	9	6.3	6290	PASS

Average of 10.383 to 10.390 min.: VL042887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.95	106	45.80	85	54.00	59	65.00	27
36.05	1861	46.10	27	54.80	471	65.20	4
37.00	11413	47.05	2160	55.00	87	66.95	60
38.05	9586	47.95	1173	56.05	3345	68.00	2262
39.00	3439	49.05	9247	57.05	6461	69.00	22861
39.95	866	50.00	46379	58.05	302	70.00	1523
40.90	20	51.05	13297	60.00	1692	71.95	1000
42.00	25	51.90	266	61.00	10332	73.05	9133
43.00	177	52.05	304	62.00	9815	74.00	37360
43.95	793	52.90	70	63.05	7645	75.10	109781
45.05	2394	53.25	67	64.00	708	76.05	8778

Average of 10.383 to 10.390 min.: VL042887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	828	87.00	5476	102.70	19	114.40	19
77.65	276	87.95	5585	104.00	989	114.85	241
78.10	152	90.85	599	104.75	306	115.90	723
79.00	5032	91.10	194	106.00	807	116.90	1111
79.95	1601	92.05	5972	106.85	175	117.95	552
80.95	5648	93.05	9109	109.85	124	119.05	858
82.00	1075	94.05	24592	110.90	204	120.00	50
82.80	56	95.10	192555	111.70	28	121.85	47
83.10	116	96.05	13091	111.95	186	122.50	19
84.70	43	97.00	386	112.75	123	122.75	86
86.05	186	98.40	21	113.00	121	123.90	70

Average of 10.383 to 10.390 min.: VL042887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.80	24	136.85	260	145.10	44	153.10	31
127.80	393	138.90	22	145.85	216	153.70	54
128.00	171	139.10	44	146.70	26	154.85	354
128.85	333	139.70	89	147.65	250	156.00	70
129.85	624	140.20	25	147.90	196	156.90	251
130.70	211	140.95	1646	148.60	17	157.95	50
131.10	136	141.95	160	148.75	114	158.90	233
131.90	24	143.00	1615	149.90	161	160.90	184
134.50	33	143.70	26	150.10	17	165.75	42
134.90	154	144.10	143	151.80	101	168.55	86
136.05	74	144.75	96	152.60	49	169.25	73

Average of 10.383 to 10.390 min.: VL042887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.85	44						
171.10	130						
172.05	415						
173.05	765						
174.00	106109						
175.05	8017						
176.00	99893						
177.00	6290						
177.95	295						
207.80	19						
223.50	23						