

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081825\
 Data File : PD089963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 11:11
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:50:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081825.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 19 05:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	51436205	399.9E6	17.526	18.136
28)	SA Decachlor...	9.067	8.065	78486470	449.1E6	18.185	17.349
Target Compounds							
9)	A Endosulfan I	6.071	5.242	38316895	233.7E6	8.303	8.914
10)	B gamma-Chl...	5.942	5.120	41454854	284.6E6	8.476	9.610
12)	B 4,4'-DDE	6.192	5.369	76260501	533.3E6	17.378	18.503
13)	MA Dieldrin	6.343	5.507	83807641	528.6E6	17.118	18.049
19)	B Endosulfa...	7.146	6.477	69663640	444.5E6	17.778	18.232
20)	A Methoxychlor	7.490	6.748	170.7E6	1029.5E6	85.111	79.829
21)	B Endrin ke...	7.627	6.986	72376845	479.6E6	17.463	18.001



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081825\
Data File : PD089963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 11:11
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:50:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081825.M
Quant Title : GC Extractables
QLast Update : Tue Aug 19 05:46:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

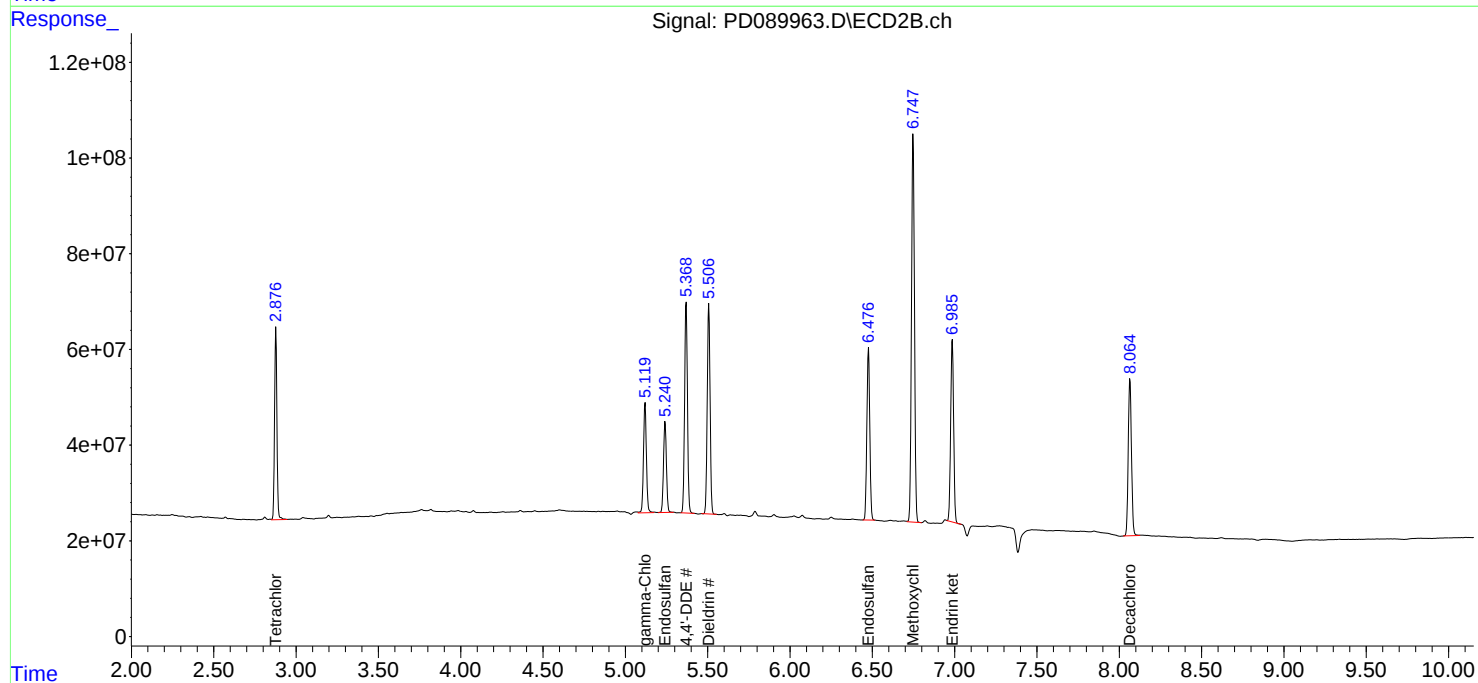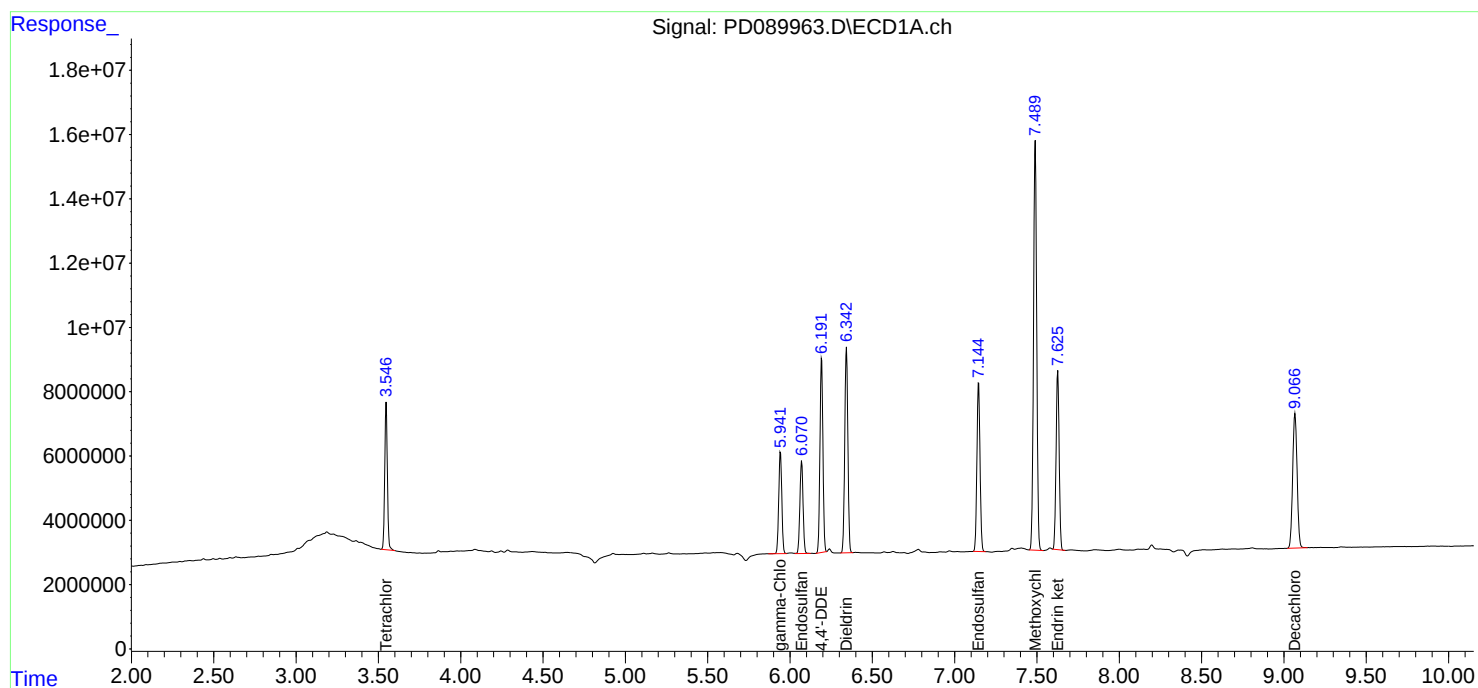


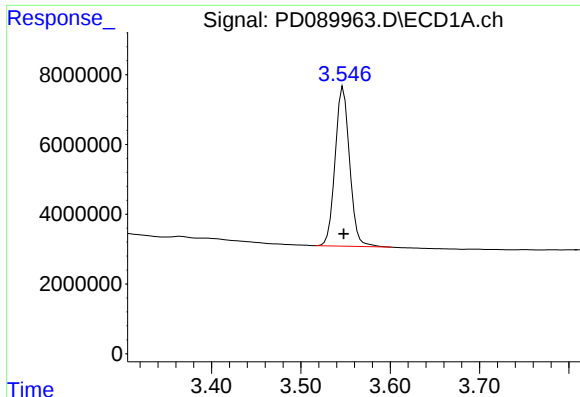

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 51436205
Conc: 17.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

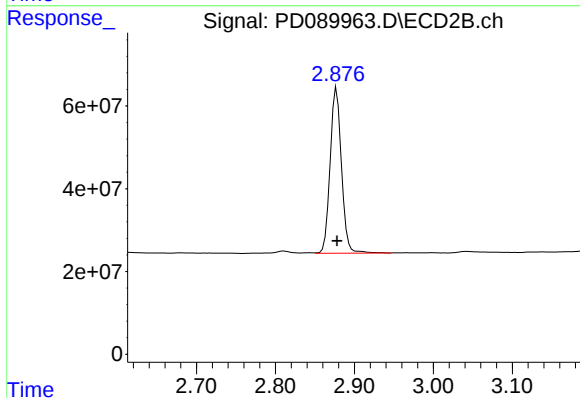


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 399914823
Conc: 18.14 ng/ml

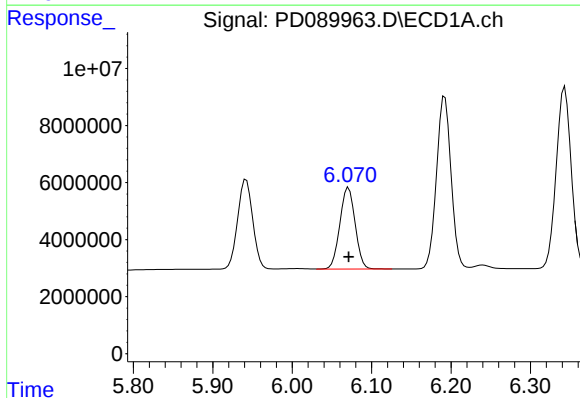


#9 Endosulfan I

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 38316895
Conc: 8.30 ng/ml

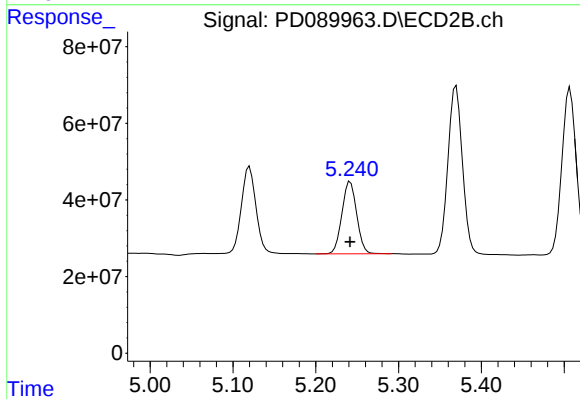

#9 Endosulfan I


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 233749878
Conc: 8.91 ng/ml

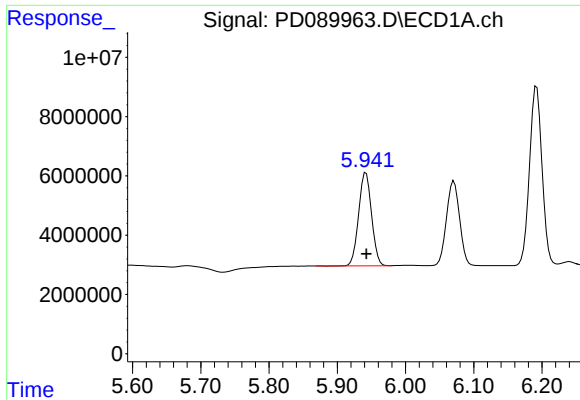

#10 gamma-Chlordane


R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 41454854
Conc: 8.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

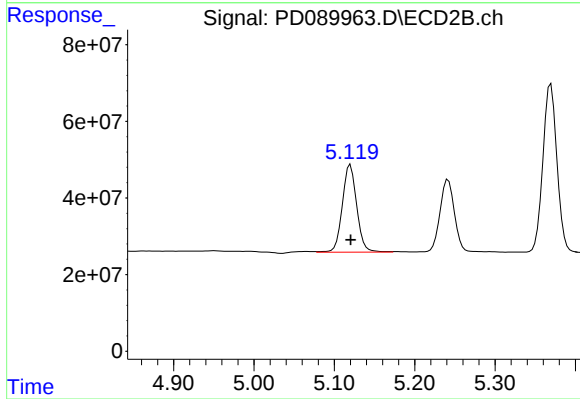


#10 gamma-Chlordane

R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 284563857
Conc: 9.61 ng/ml

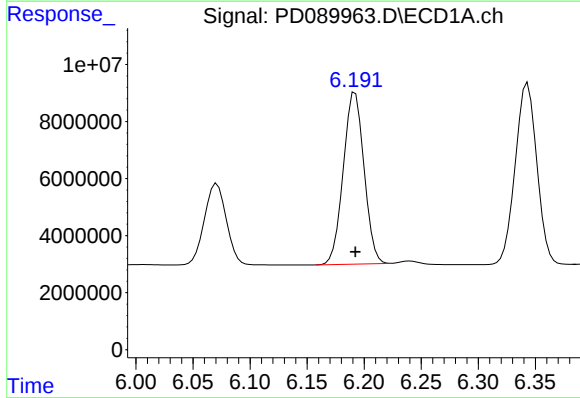


#12 4,4'-DDE

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 76260501
Conc: 17.38 ng/ml

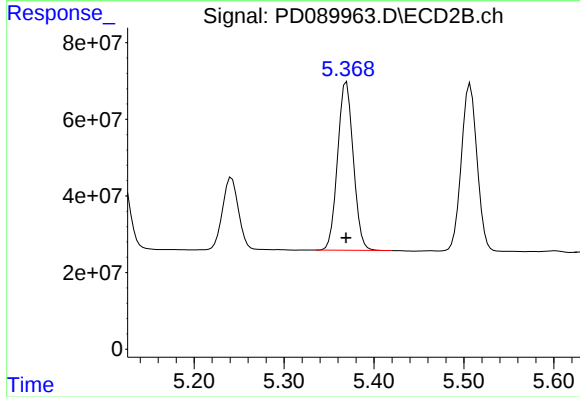

#12 4,4'-DDE


R.T.: 5.369 min
Delta R.T.: 0.000 min
Response: 533310087
Conc: 18.50 ng/ml

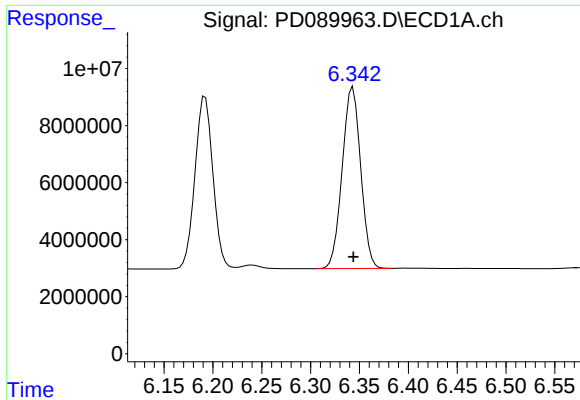

#13 Dieldrin


R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 83807641
Conc: 17.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

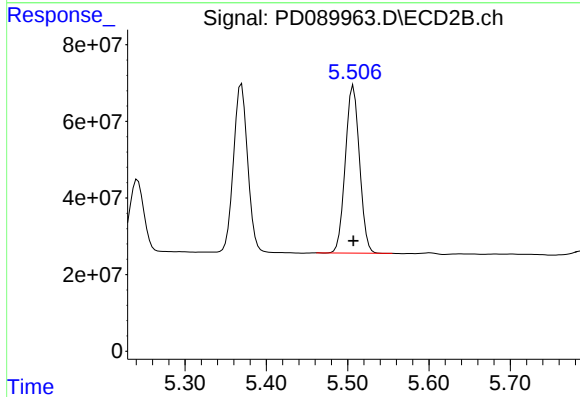


#13 Dieldrin

R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 528613395
Conc: 18.05 ng/ml

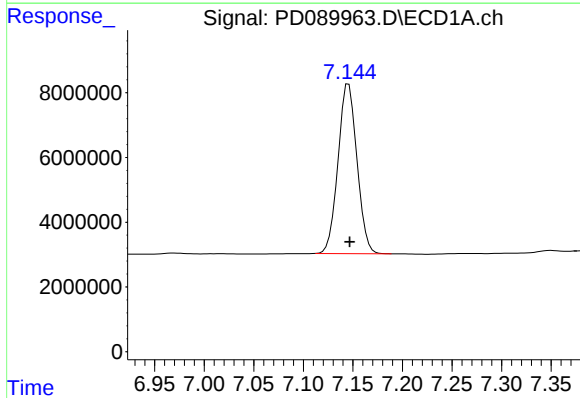


#19 Endosulfan Sulfate

R.T.: 7.146 min
Delta R.T.: -0.001 min
Response: 69663640
Conc: 17.78 ng/ml

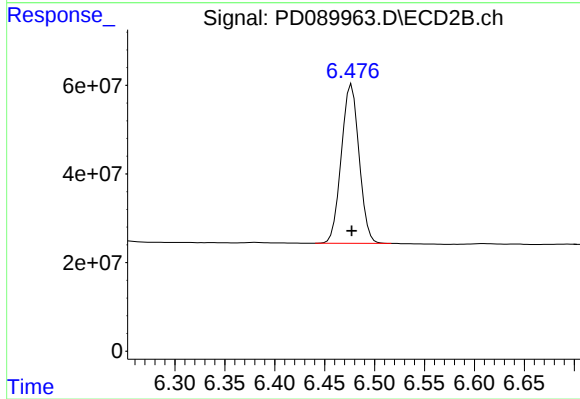

#19 Endosulfan Sulfate


R.T.: 6.477 min
Delta R.T.: 0.000 min
Response: 444483987
Conc: 18.23 ng/ml

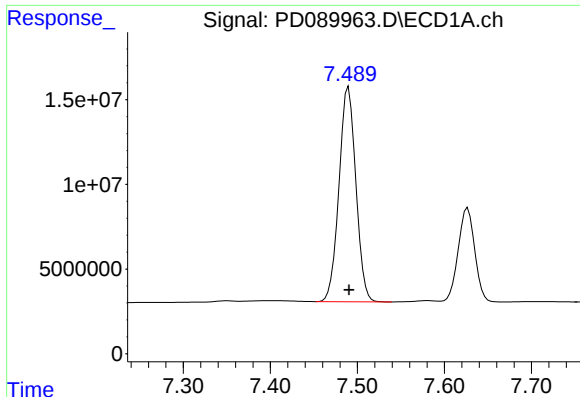

#20 Methoxychlor


R.T.: 7.490 min
Delta R.T.: 0.000 min
Response: 170700084
Conc: 85.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

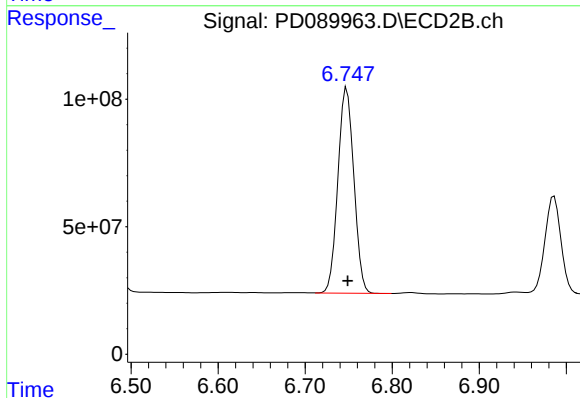


#20 Methoxychlor

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 1029459046
Conc: 79.83 ng/ml

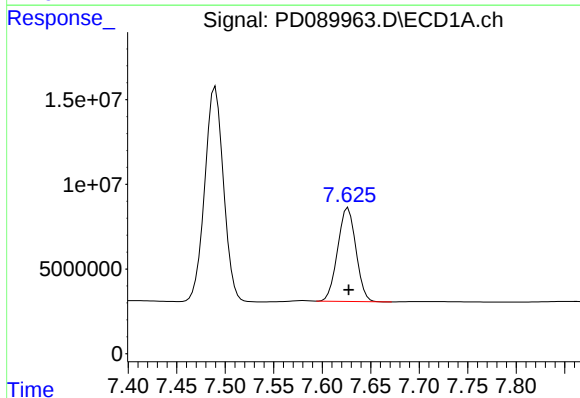


#21 Endrin ketone

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 72376845
Conc: 17.46 ng/ml

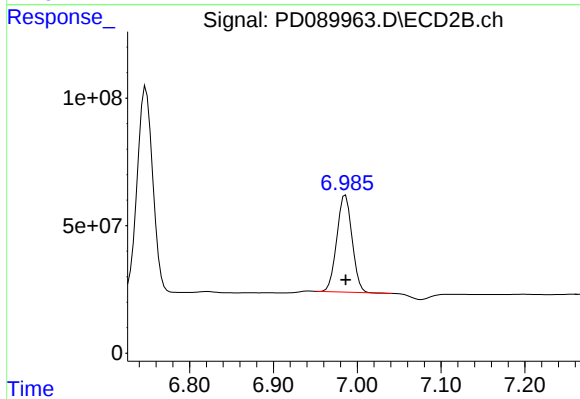

#21 Endrin ketone


R.T.: 6.986 min
Delta R.T.: 0.000 min
Response: 479625043
Conc: 18.00 ng/ml

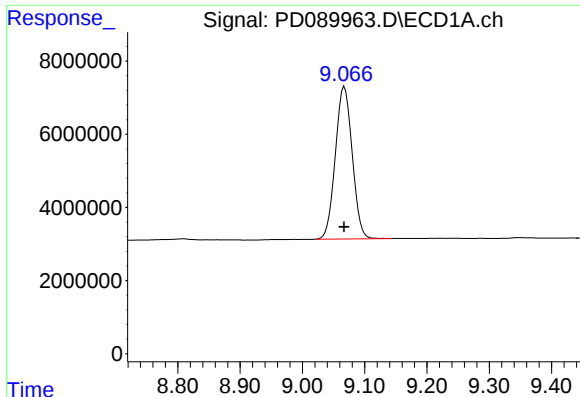

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 78486470
Conc: 18.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

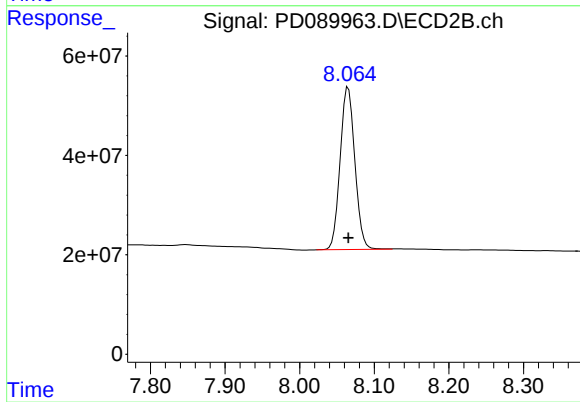

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 449091853
Conc: 17.35 ng/ml