


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025724.D
Acq On : 11 Sep 2025 08:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

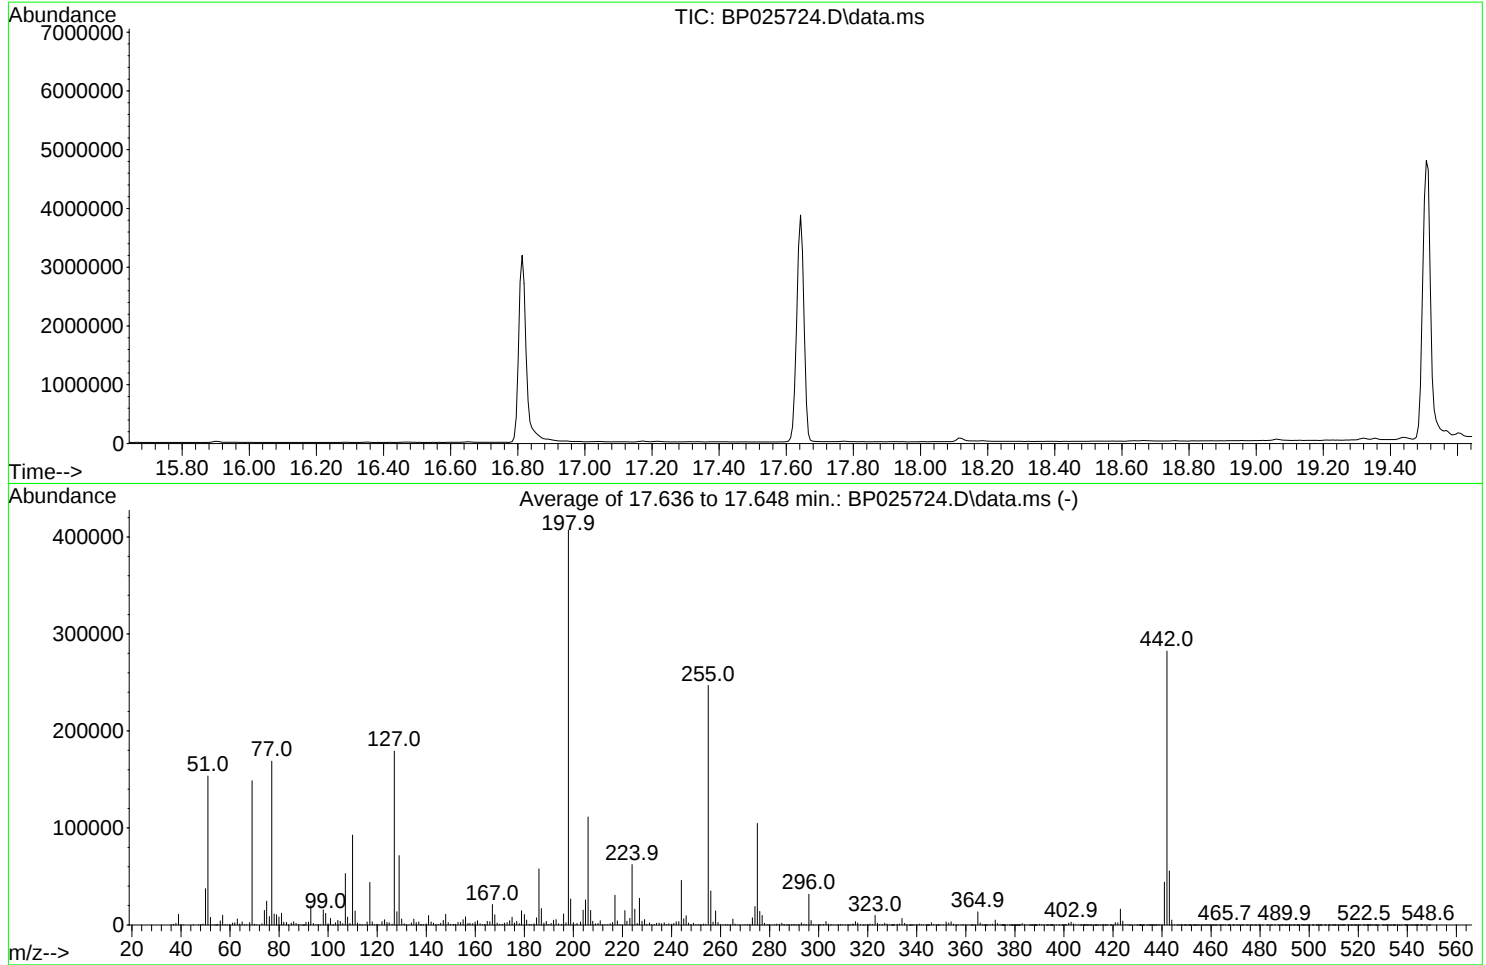




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2490

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2392	PASS
69	69	100	100	100.0	148681	PASS
70	69	0.00	2	0.5	775	PASS
197	198	0.00	2	0.6	2274	PASS
198	198	100	100	100.0	407104	PASS
199	198	5	9	6.6	26775	PASS
365	198	1	100	3.3	13409	PASS
441	443	0.01	150	79.1	44067	PASS
442	442	100	100	100.0	282368	PASS
443	442	15	24	19.7	55680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025724.D
Acq On : 11 Sep 2025 08:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 11 12:58:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 09:20:45 2025
Response via : Initial Calibration

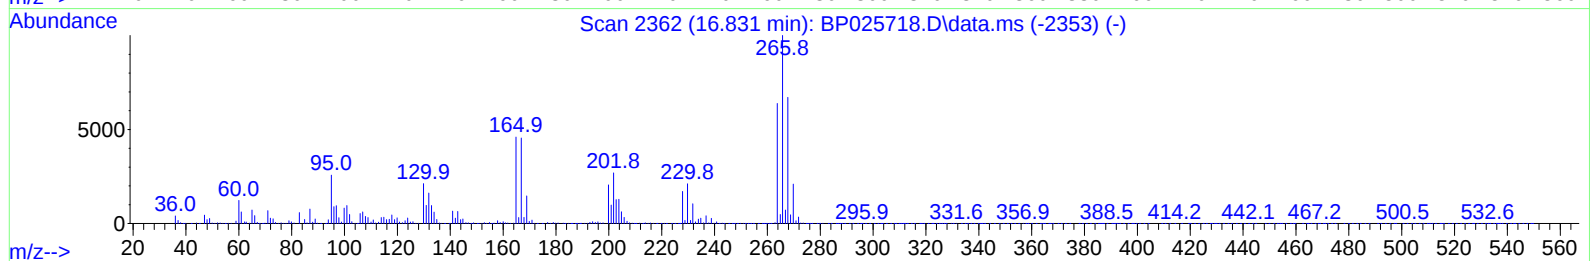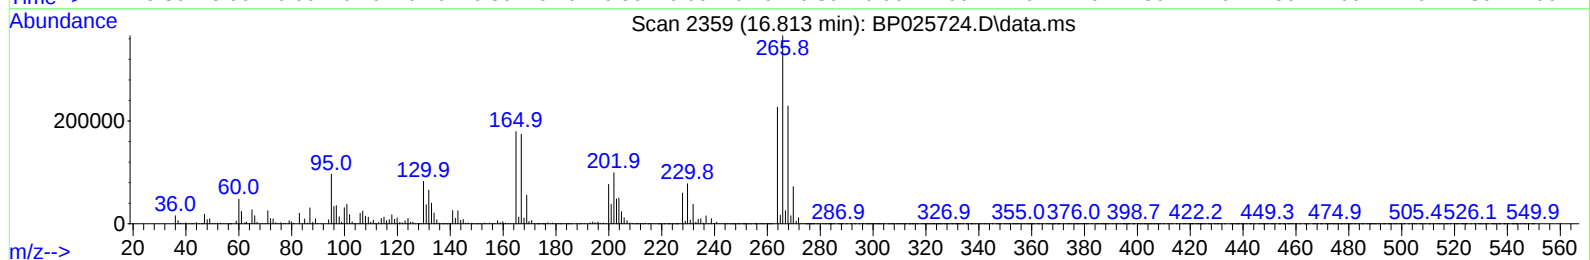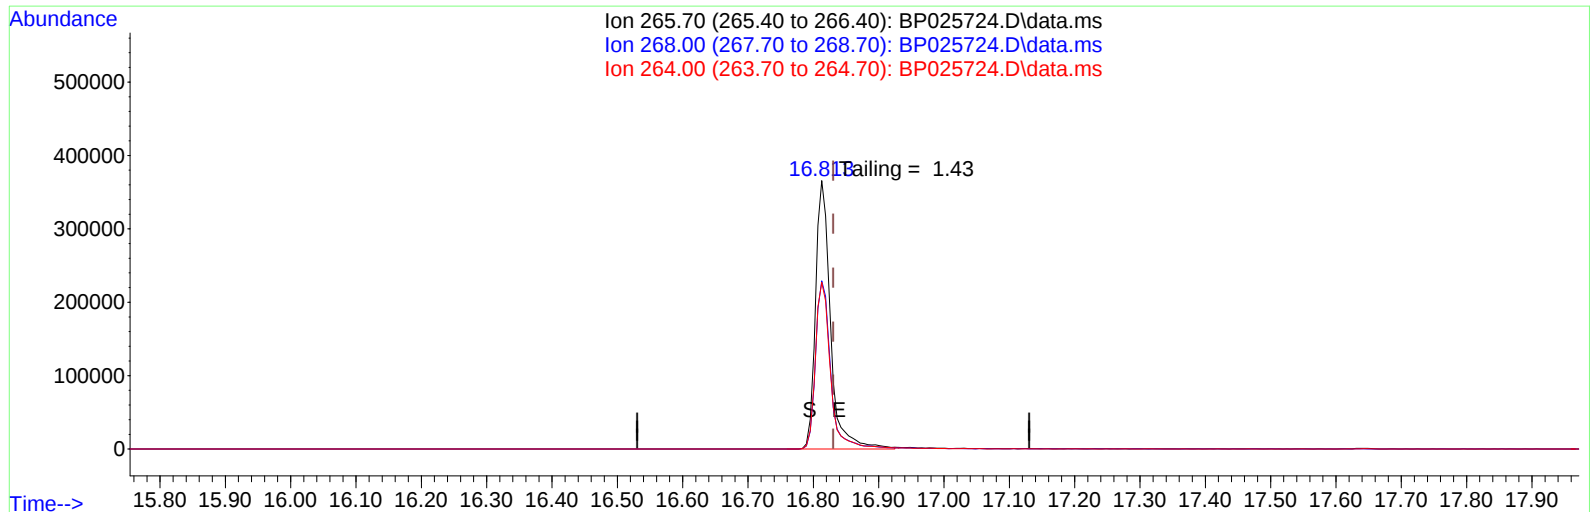

TIC: BP025724.D\data.ms

(70) Pentachlorophenol (C)

16.813min (-0.018) 7217.81 ng




response 589827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	62.64
264.00	63.80	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025724.D
Acq On : 11 Sep 2025 08:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 11 12:58:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 09:20:45 2025
Response via : Initial Calibration

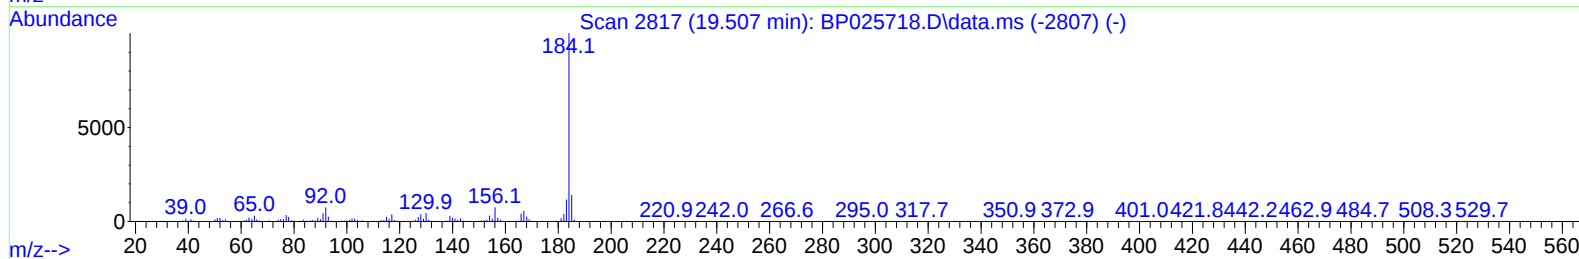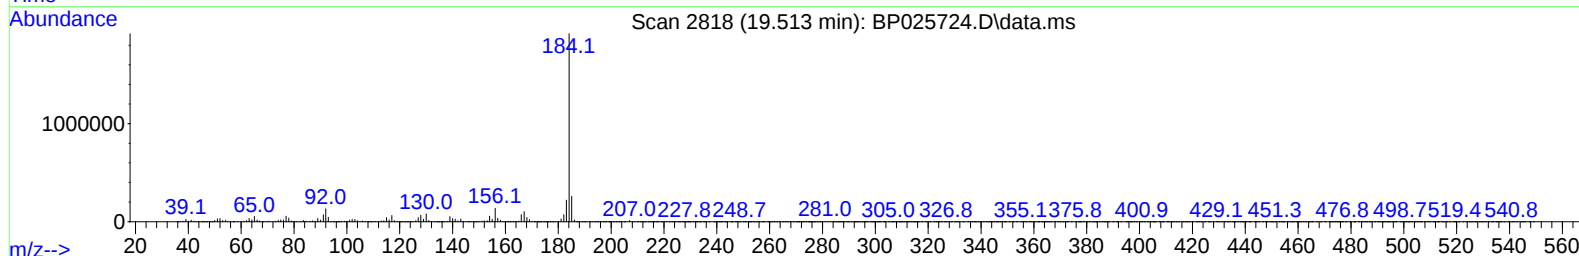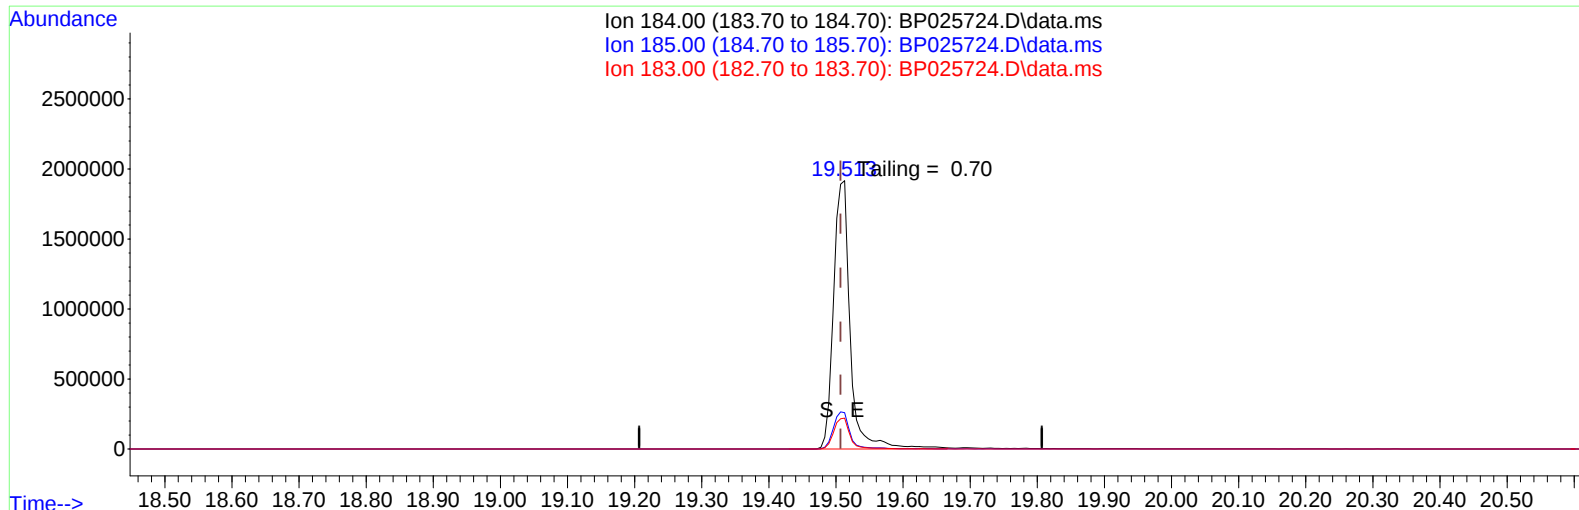

TIC: BP025724.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 4369.52 ng

response 3272403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.55
183.00	11.50	11.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2025	BNA_P	<u>BP025724.D</u>
Compound Name	Response	Retention Time
DDT	1712718	20.801
DDD	33235	20.342
DDE	3389	19.813
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36624	1749342	2.09

Instrument :
BNA_P
ClientSampleId :
DFTPP