


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091725\
Data File : BP025768.D
Acq On : 17 Sep 2025 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

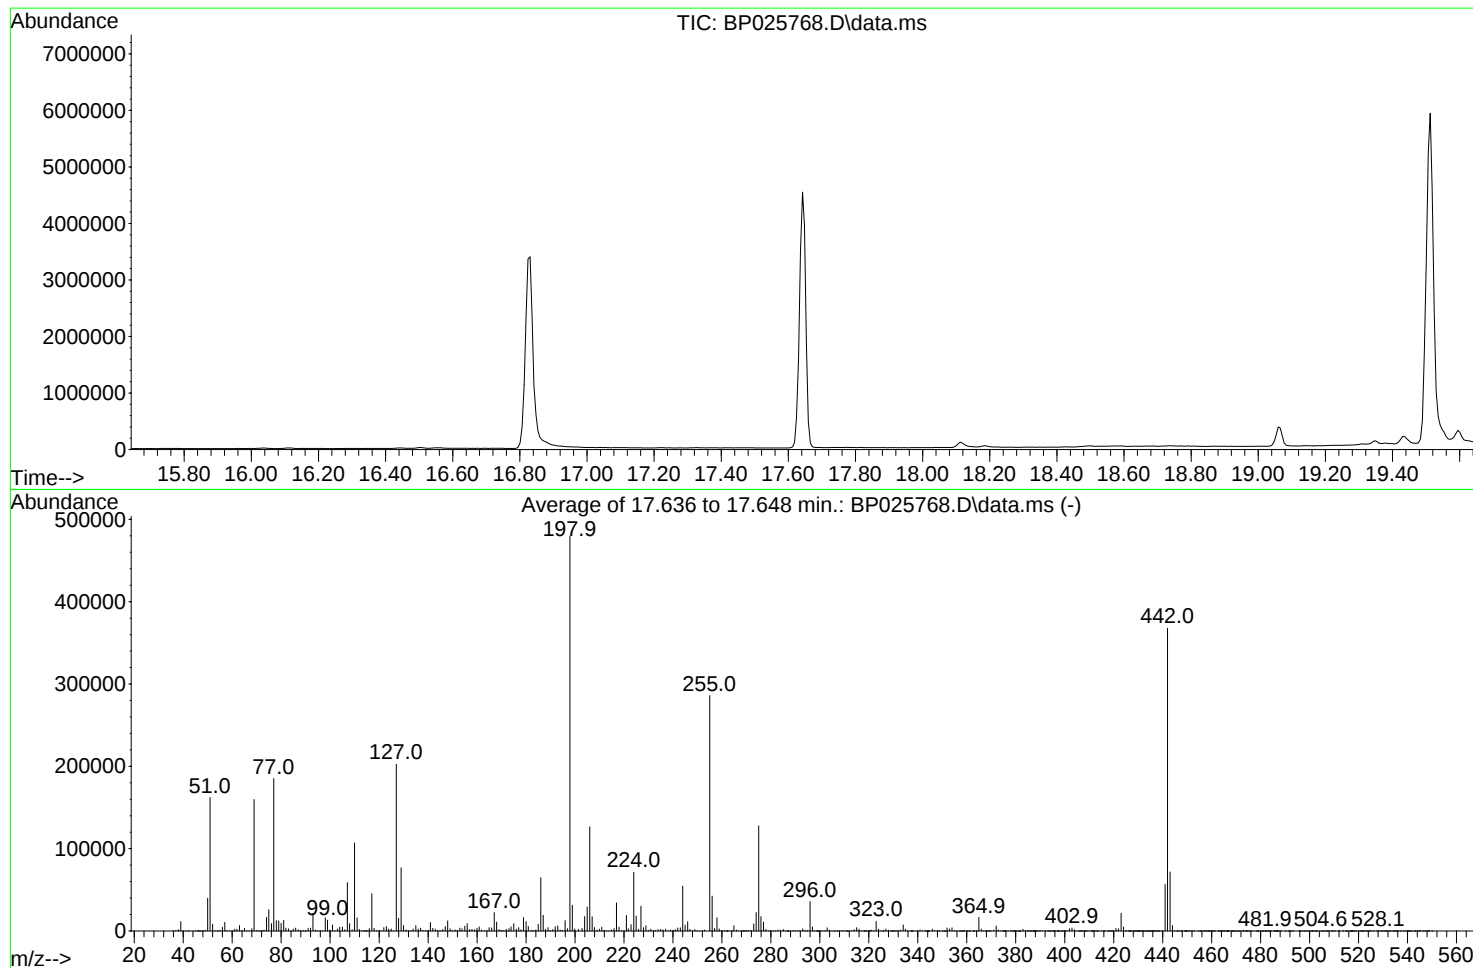




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2490

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2722	PASS
69	69	100	100	100.0	159833	PASS
70	69	0.00	2	0.5	762	PASS
197	198	0.00	2	0.6	2688	PASS
198	198	100	100	100.0	479553	PASS
199	198	5	9	6.5	31290	PASS
365	198	1	100	3.4	16511	PASS
441	443	0.01	150	78.8	56501	PASS
442	442	100	100	100.0	367637	PASS
443	442	15	24	19.5	71685	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091725\
Data File : BP025768.D
Acq On : 17 Sep 2025 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 17 13:24:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

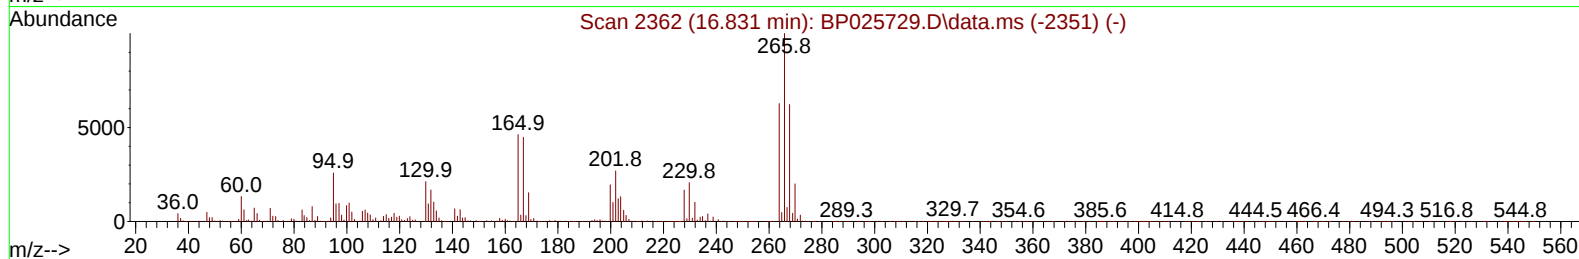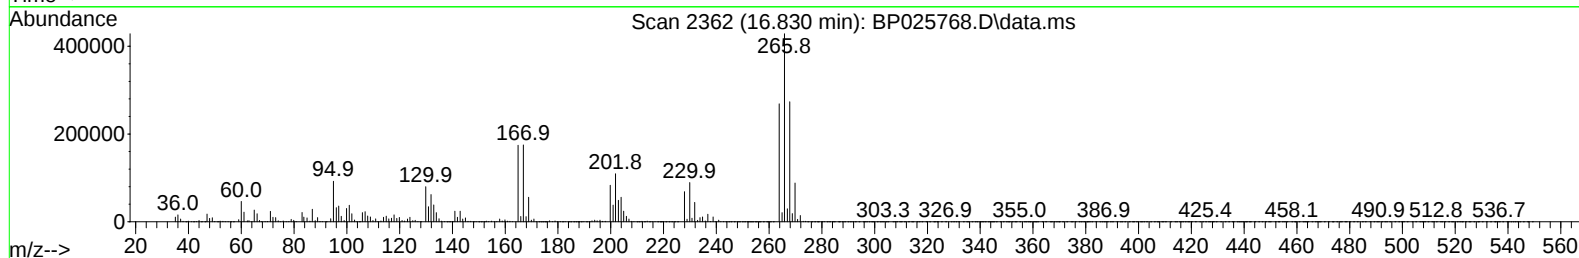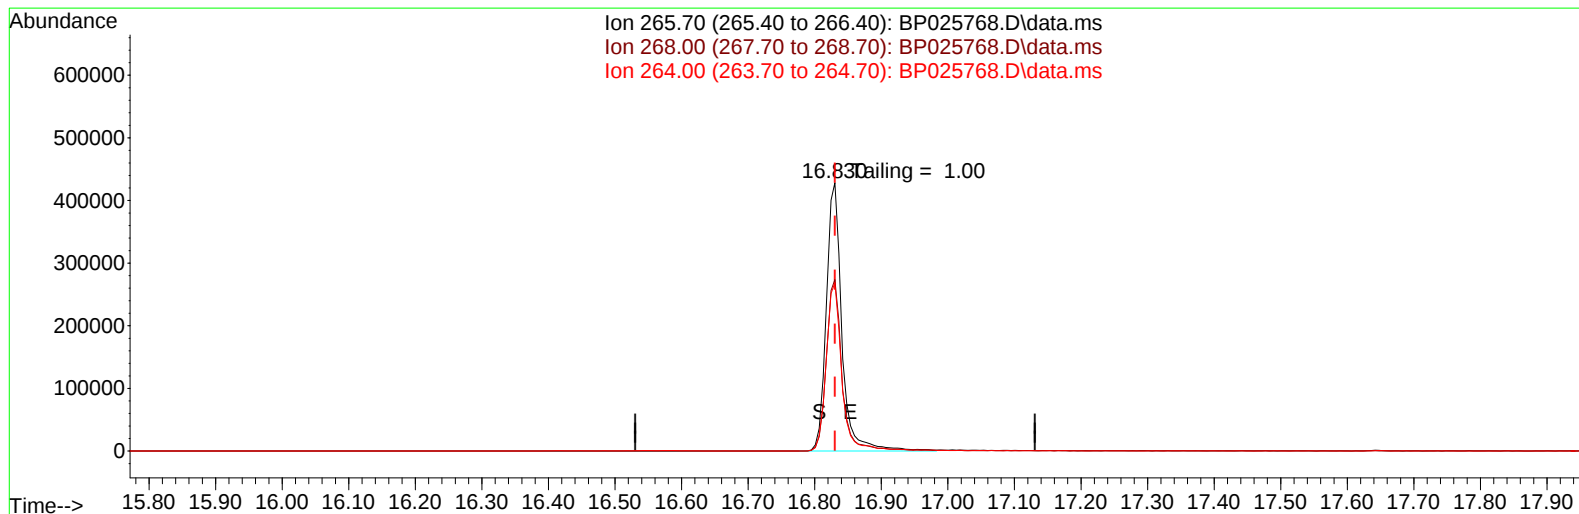

TIC: BP025768.D\data.ms

(70) Pentachlorophenol (C)

16.830min (-0.000) 1245628.62 ng




response 694952

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.86
264.00	62.70	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091725\
Data File : BP025768.D
Acq On : 17 Sep 2025 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 17 13:24:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

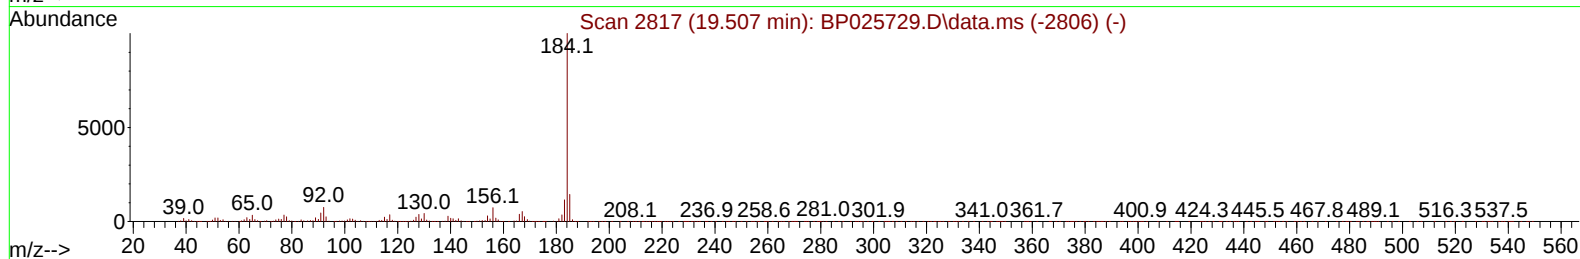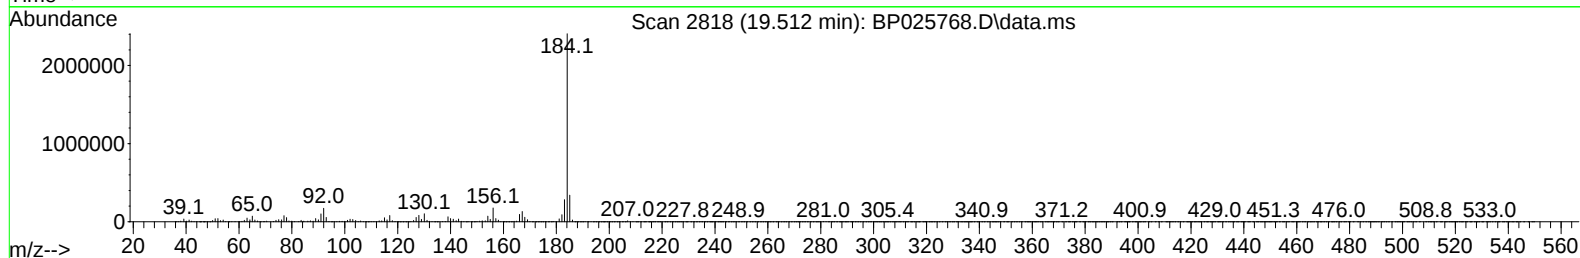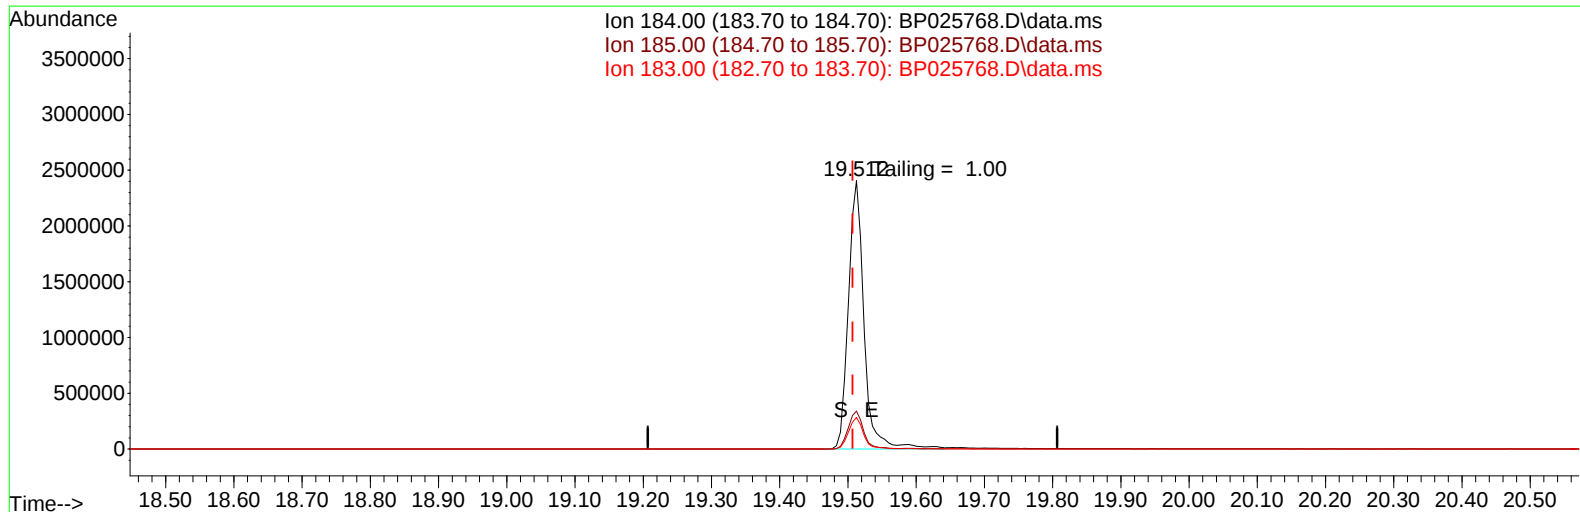

TIC: BP025768.D\data.ms

(77) Benzidine

19.512min (+ 0.006) 1057543.21 ng

response 3746937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.50	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2025	BNA_P	<u>BP025768.D</u>
Compound Name	Response	Retention Time
DDT	1963626	20.801
DDD	38286	20.336
DDE	5049	19.812
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43335	2006961	2.16

Instrument :
BNA_P
ClientSampleId :
DFTPP