


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092425\
Data File : BN037870.D
Acq On : 24 Sep 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

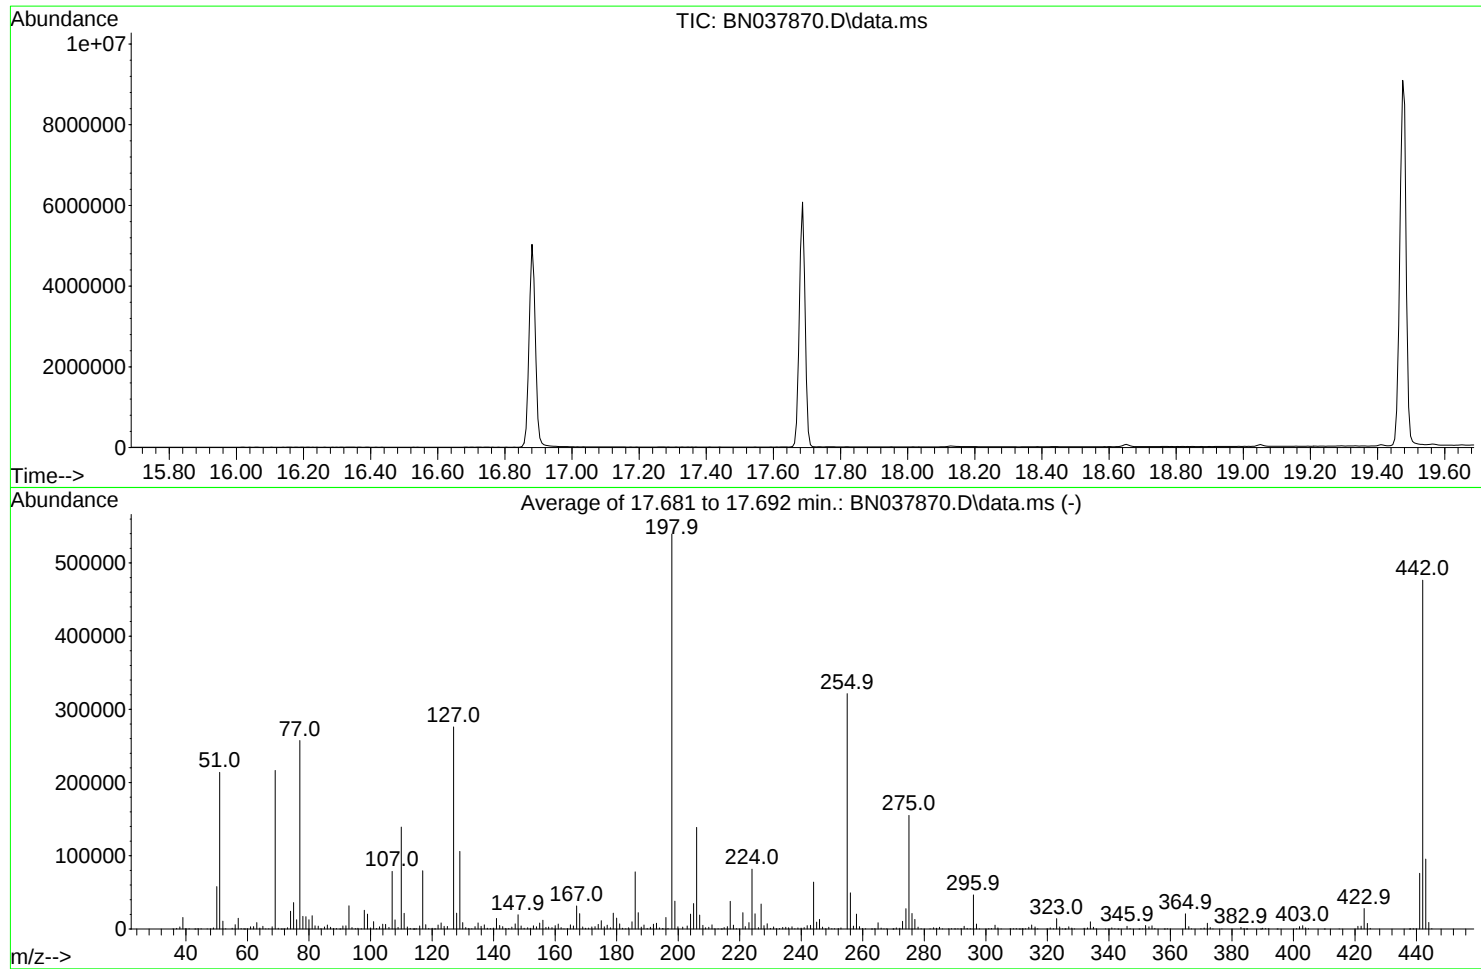




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	3143	PASS
69	69	100	100	100.0	216661	PASS
70	69	0.00	2	0.5	1168	PASS
197	198	0.00	2	0.2	839	PASS
198	198	100	100	100.0	539285	PASS
199	198	5	9	7.1	38096	PASS
365	198	1	100	3.8	20696	PASS
441	443	0.01	150	79.6	76072	PASS
442	442	100	100	100.0	476331	PASS
443	442	15	24	20.1	95557	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092425\
Data File : BN037870.D
Acq On : 24 Sep 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 24 11:37:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

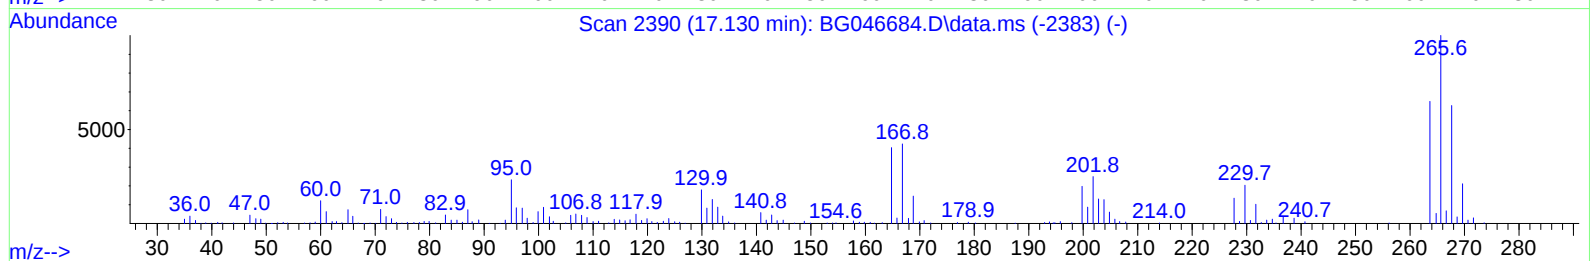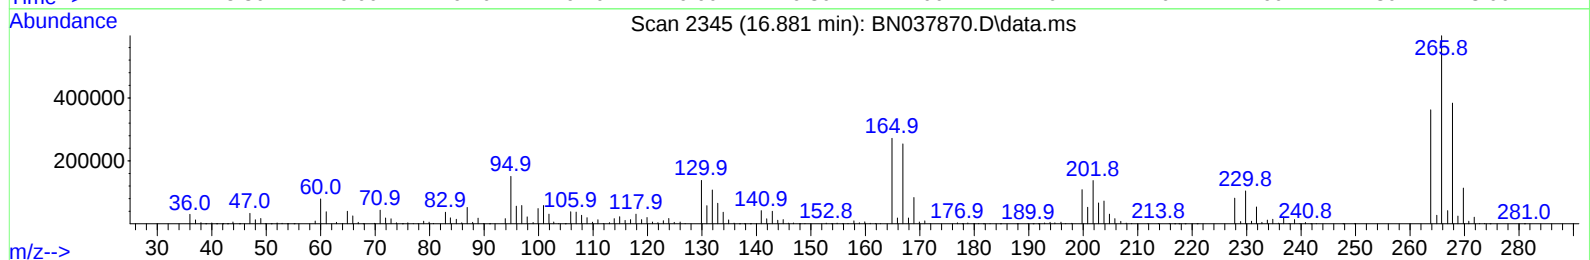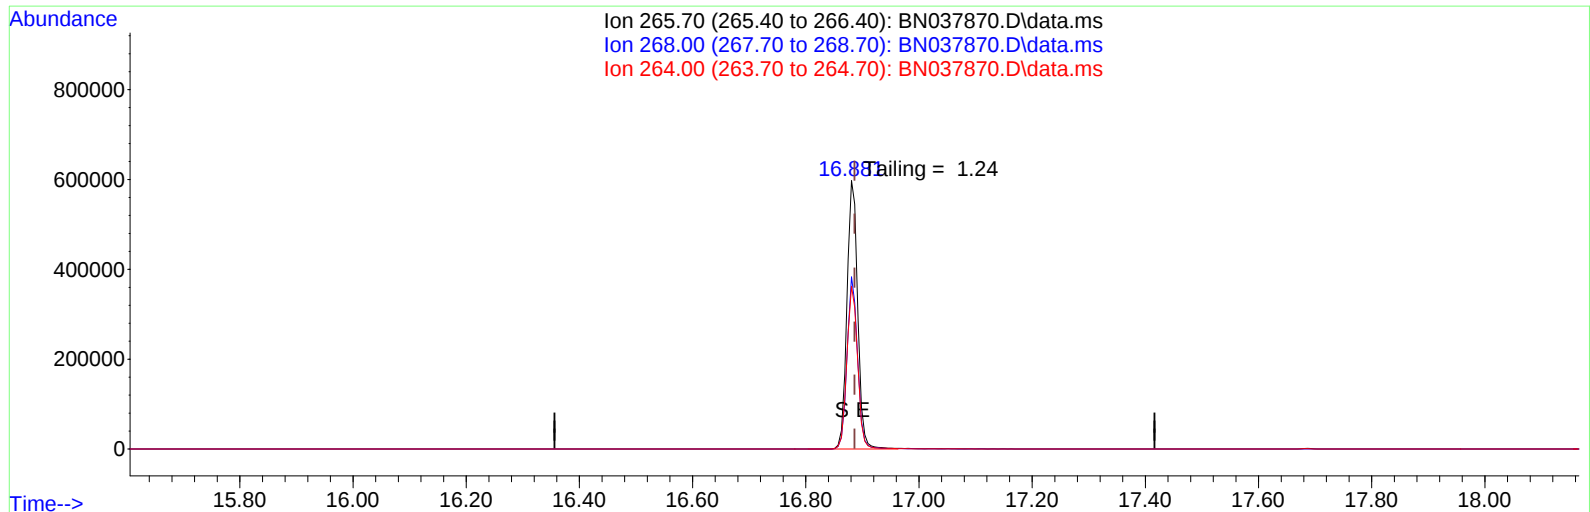

TIC: BN037870.D\data.ms

(70) Pentachlorophenol (C)

16.881min (-0.005) 29214.29 ng




response 795325

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.18
264.00	61.60	60.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092425\
Data File : BN037870.D
Acq On : 24 Sep 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 24 11:37:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

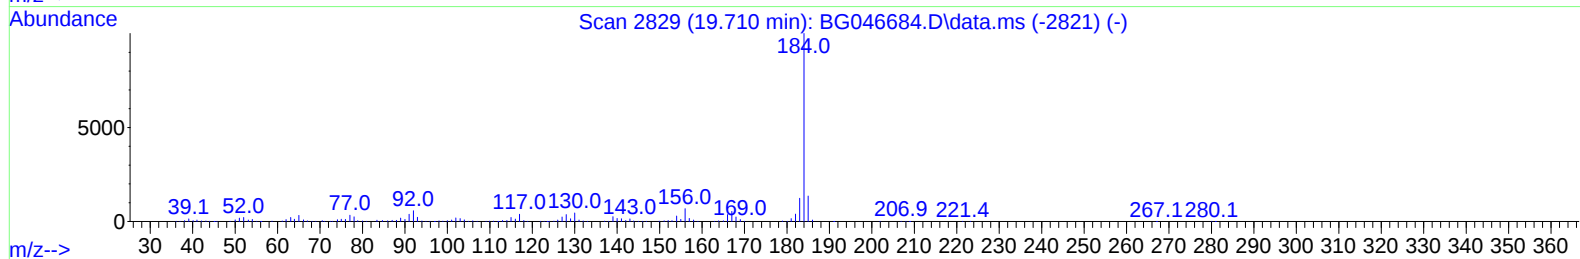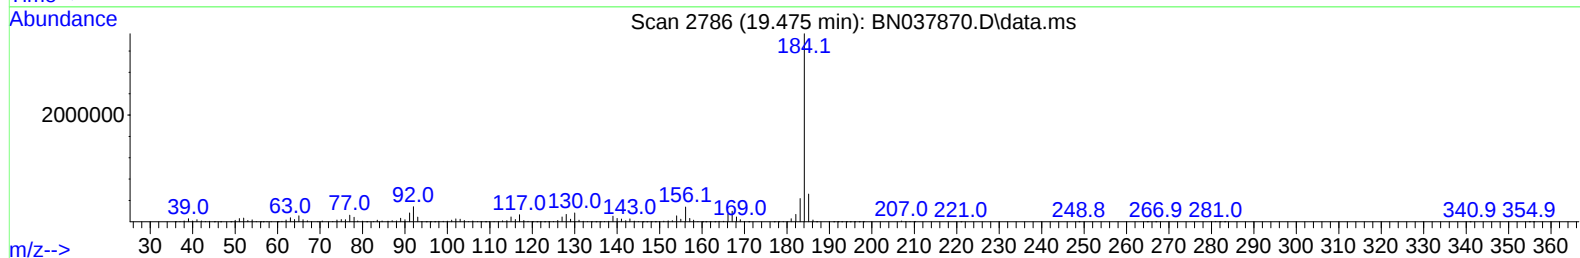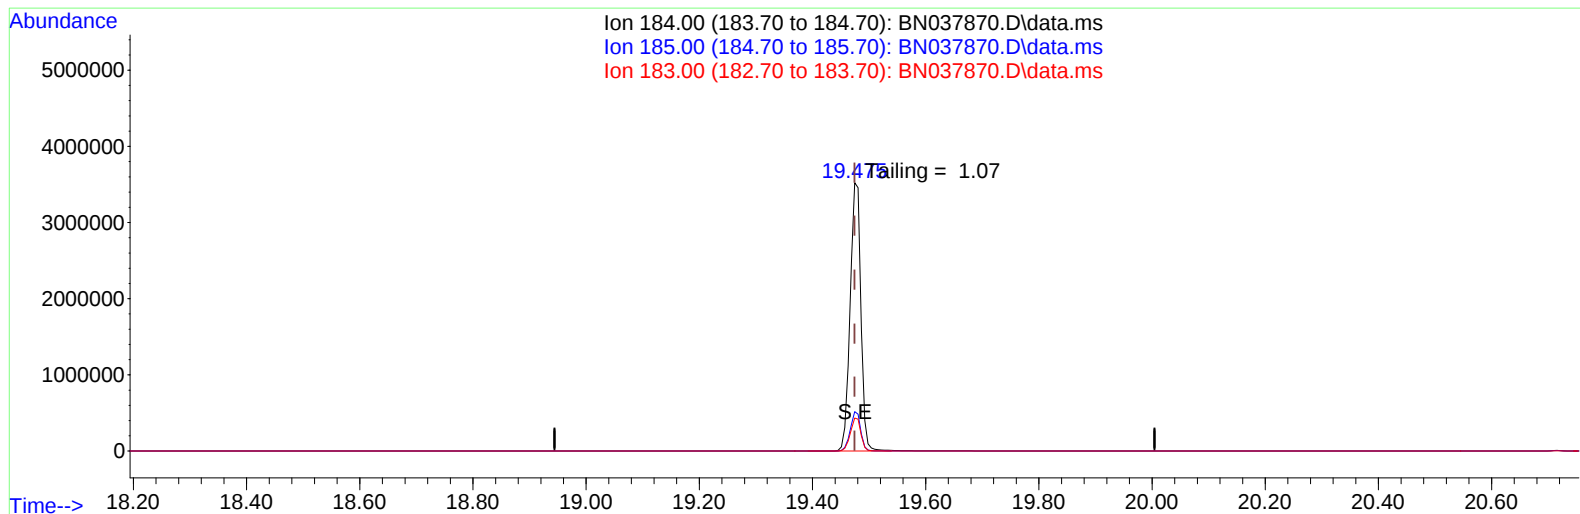

TIC: BN037870.D\data.ms

(77) Benzidine

19.475min (+ 0.001) 0.00 ng

response 4681423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.71
183.00	13.20	12.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/24/2025	BNA_N	<u>BN037870.D</u>
Compound Name	Response	Retention Time
DDT	2091319	20.716
DDD	5093	20.328
DDE	153	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5246	2096565	0.25

Instrument :
BNA_N
ClientSampleId :
DFTPP