


Ident	Instrument IC-1				Analyst: RM		Method: 300.0 / 9056A		Initial w Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name		date time	
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 10:21	10 RM/IZ
STD2	0.423	0.641	0.632	2.091	0.529	1.063	3.237	IC1-090925	9/9/2025 10:42	10 RM/IZ	
STD3	0.794	1.189	1.197	3.984	0.997	2.006	6.010	IC1-090925	9/9/2025 11:25	10 RM/IZ	
STD4	0.990	1.475	1.473	4.920	1.228	2.461	7.371	IC1-090925	9/9/2025 11:47	10 RM/IZ	
STD5	2.008	3.012	3.027	10.105	2.514	4.978	15.047	IC1-090925	9/9/2025 13:36	10 RM/IZ	
STD6	3.935	5.921	5.894	19.658	4.924	9.905	29.203	IC1-090925	9/9/2025 13:58	10 RM/IZ	
STD7	5.050	7.561	7.577	25.243	6.308	12.587	37.633	IC1-090925	9/9/2025 14:41	10 RM/IZ	
ICV	2.001	2.995	2.988	9.985	2.483	5.041	14.797	IC1-090925	9/9/2025 15:02	10 RM/IZ	
ICB	0.000	0.063	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 15:45	10 RM/IZ	
CCV	2.004	2.970	2.981	10.060	2.440	5.083	14.890	IC1-090925	9/11/2025 10:23	10 RM/IZ	
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/11/2025 10:45	10 RM/IZ	
LB137171BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/11/2025 11:06	10 RM/IZ	
LB137171BSW	2.016	2.955	2.970	10.004	2.432	5.036	14.786	IC1-090925	9/11/2025 11:28	10 RM/IZ	
Q3019-05	3.367	259.814	0.000	5.201	0.000	0.000	111.521	IC1-090925	9/11/2025 11:49	10 RM/IZ	
Q3019-11	0.000	47.723	0.000	0.000	8.087	3.837	0.000	IC1-090925	9/11/2025 12:33	10 RM/IZ	
Q3019-15	0.000	0.074	1.531	0.000	0.000	0.000	0.000	IC1-090925	9/11/2025 12:54	10 RM/IZ	
Q3019-05DLX10	0.354	19.027	0.000	0.635	0.000	0.000	10.024	IC1-090925	9/11/2025 13:16	10 RM/IZ	
Q3019-05DL2X50	0.096	3.521	0.000	0.241	0.000	0.000	2.301	IC1-090925	9/11/2025 13:37	10 RM/IZ	
Q3019-11DLX2	0.000	21.812	0.000	0.000	3.908	1.755	0.000	IC1-090925	9/11/2025 13:59	10 RM/IZ	
CCV	2.017	2.948	2.964	10.001	2.429	5.049	14.851	IC1-090925	9/11/2025 14:20	10 RM/IZ	
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/11/2025 14:42	10 RM/IZ	

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentratio n HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-090925	10 RM/IZ
STD2	0.4230	0.6410	0.6320	2.0910	0.5290	1.0630	3.2370	IC1-090925	10 RM/IZ
STD3	0.7940	1.1890	1.1970	3.9840	0.9970	2.0060	6.0100	IC1-090925	10 RM/IZ
STD4	0.9900	1.4750	1.4730	4.9200	1.2280	2.4610	7.3710	IC1-090925	10 RM/IZ
STD5	2.0080	3.0120	3.0270	10.1050	2.5140	4.9780	15.0470	IC1-090925	10 RM/IZ
STD6	3.9350	5.9210	5.8940	19.6580	4.9240	9.9050	29.2030	IC1-090925	10 RM/IZ
STD7	5.0500	7.5610	7.5770	25.2430	6.3080	12.5870	37.6330	IC1-090925	10 RM/IZ
date time	9/9/2025 10:21	9/9/2025 10:42	9/9/2025 10:42	9/9/2025 11:25	9/9/2025 11:47	9/9/2025 13:36	9/9/2025 13:58	9/9/2025 14:41	
Analyst									
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	5.7500	6.8333	5.3333	4.5500	5.8000	6.3000	7.9000		
STD3	-0.7500	-0.9167	-0.2500	-0.4000	-0.3000	0.3000	0.1667		
STD4	-1.0000	-1.6667	-1.8000	-1.6000	-1.7600	-1.5600	-1.7200		
STD5	0.4000	0.4000	0.9000	1.0500	0.5600	-0.4400	0.3133		
STD6	-1.6250	-1.3167	-1.7667	-1.7100	-1.5200	-0.9500	-2.6567		
STD7	1.0000	0.8133	1.0267	0.9720	0.9280	0.6960	1.7108		

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

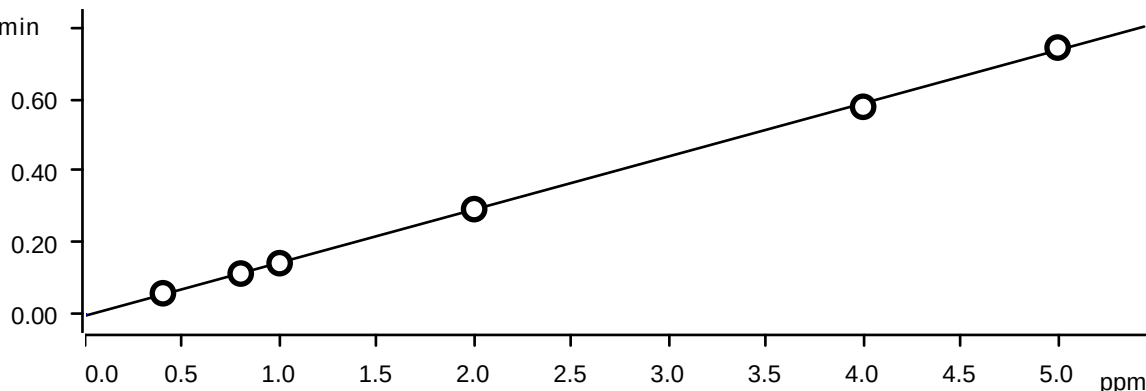

Function: $A = -3.91674\text{E-}3 + 0.0148053 \times Q$


Relative standard deviation 1.985504 %

Correlation coefficient 0.999790

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.059	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.114	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.579	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.744	STD7	2025-09-09 14:41:06 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

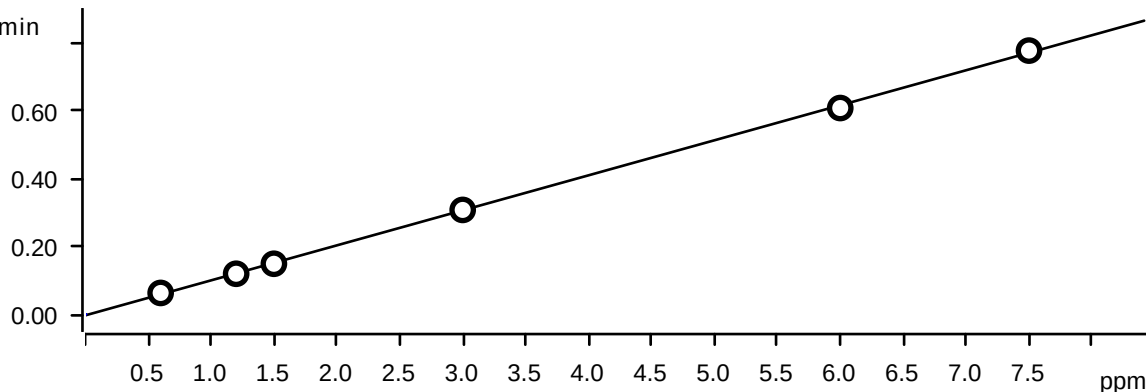


Function: $A = -2.97735\text{E-}3 + 0.0103068 \times Q$

Relative standard deviation 1.712968 %

Correlation coefficient 0.999843

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.063	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.120	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.149	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.307	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.607	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.776	STD7	2025-09-09 14:41:06 UTC-4	used

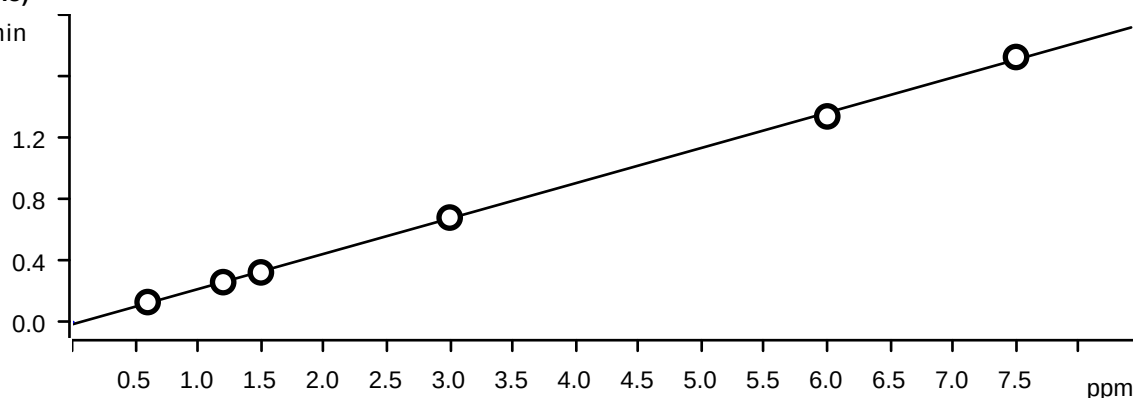Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0143669 + 0.0229543 \times Q$


Relative standard deviation 2.170764 %

Correlation coefficient 0.999753

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.131	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.260	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.324	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.681	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.339	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.725	STD7	2025-09-09 14:41:06 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

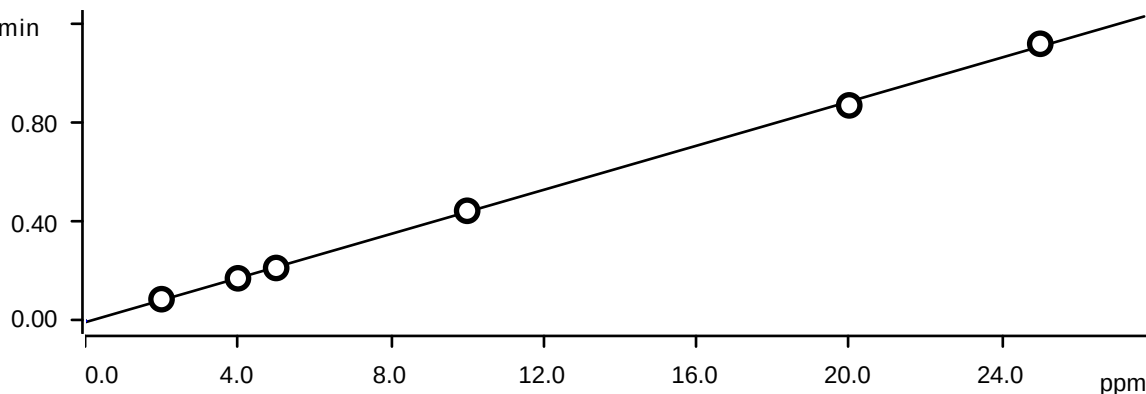

Function: $A = -5.68247E-3 + 4.44287E-3 \times Q$


Relative standard deviation: 2.066849 %

Correlation coefficient: 0.999773

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.171	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.443	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.868	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.116	STD7	2025-09-09 14:41:06 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

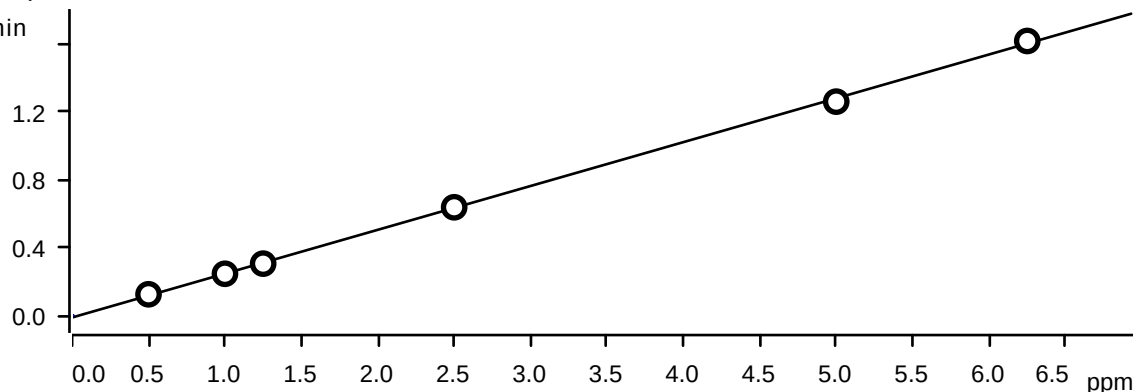


Function: $A = -0.0122982 + 0.0258010 \times Q$

Relative standard deviation: 1.914251 %

Correlation coefficient 0.999807

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.245	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.305	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.636	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.258	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.615	STD7	2025-09-09 14:41:06 UTC-4	used

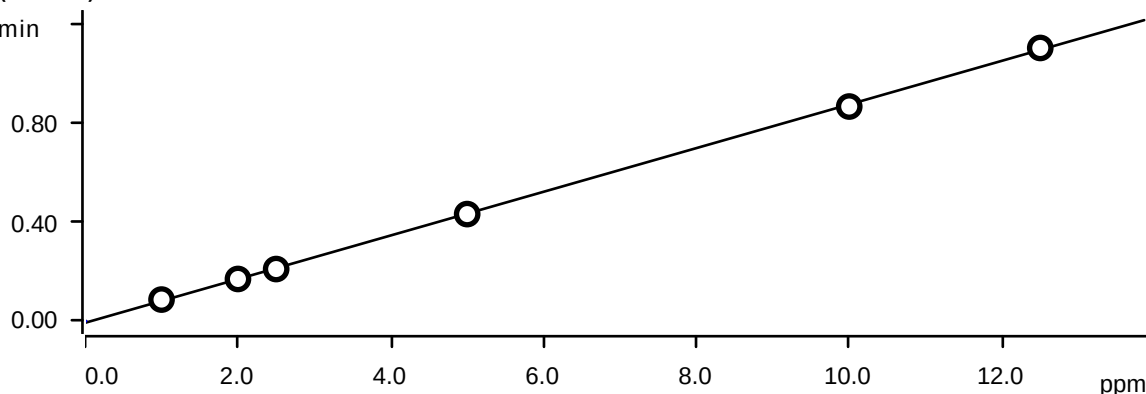
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -6.72192E-3 + 8.79335E-3 \times Q$

Relative standard deviation 1.384046 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.170	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.210	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.431	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.100	STD7	2025-09-09 14:41:06 UTC-4	used

Sulfate (Anions)

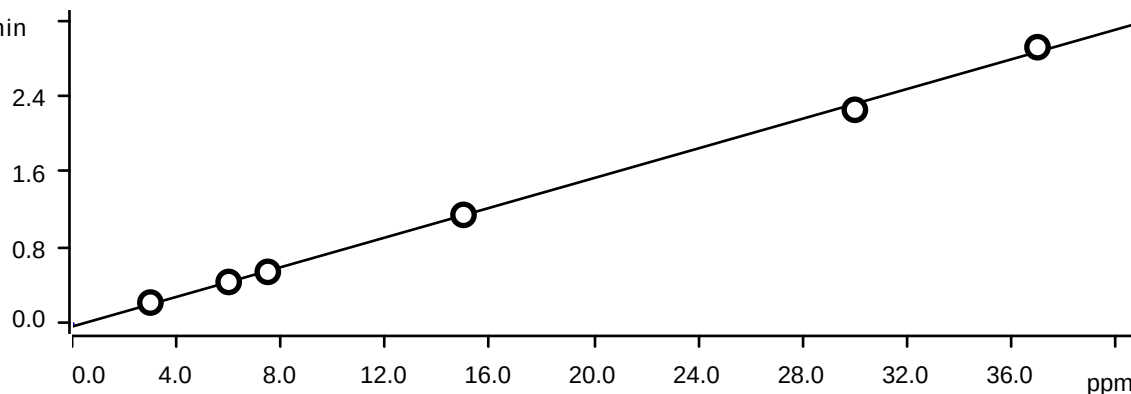 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0295615 + 7.81954E-3 \times Q$

Relative standard deviation 3.285067 %

Correlation coefficient 0.999433


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.224	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.440	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.547	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.147	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.254	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.913	STD7	2025-09-09 14:41:06 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-09-09 10:21:26 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

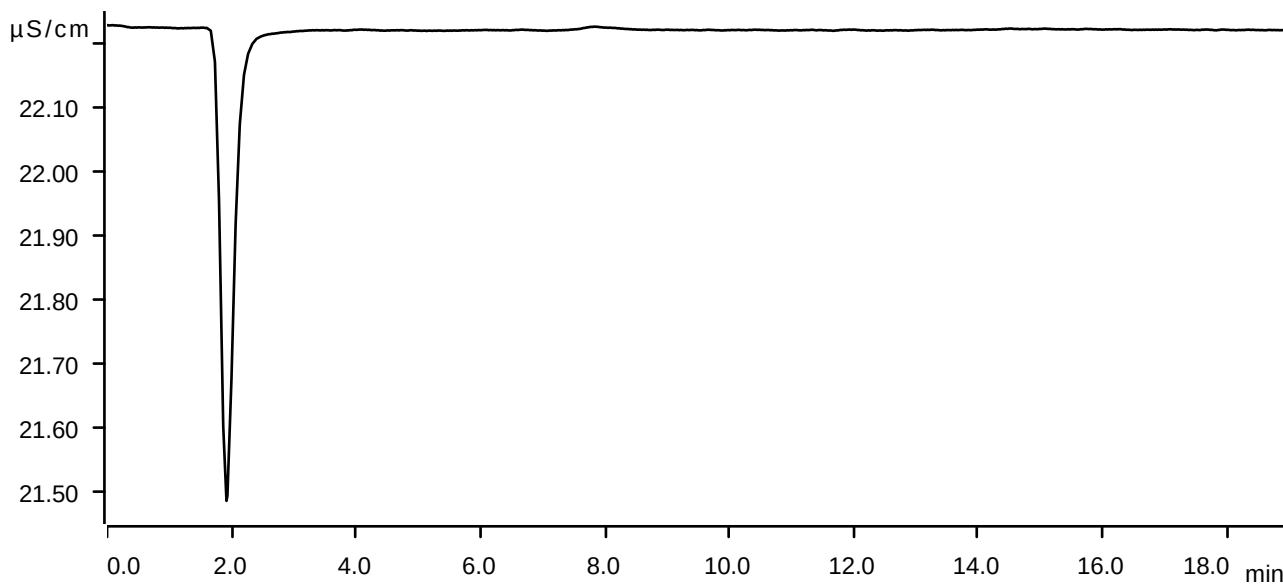Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-09-09 10:42:49 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

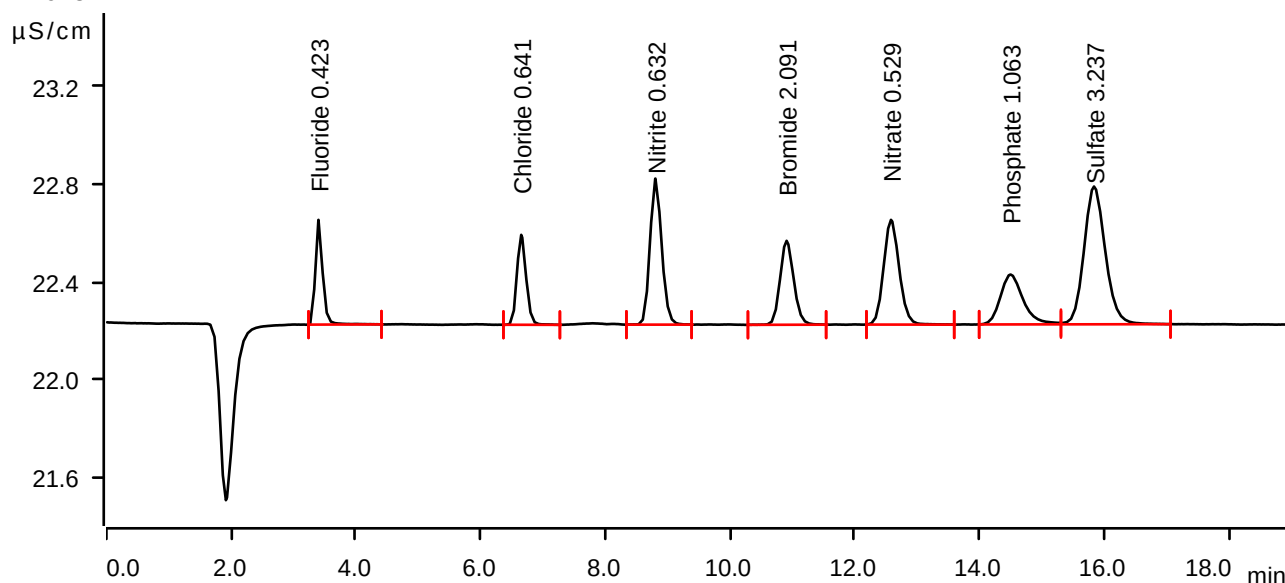

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.0587	0.429	0.423	Fluoride
2	6.652	0.0631	0.369	0.641	Chloride
3	8.803	0.1306	0.599	0.632	Nitrite
4	10.907	0.0872	0.344	2.091	Bromide
5	12.580	0.1242	0.430	0.529	Nitrate
6	14.497	0.0867	0.205	1.063	Phosphate
7	15.835	0.2236	0.565	3.237	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-09-09 11:25:44 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

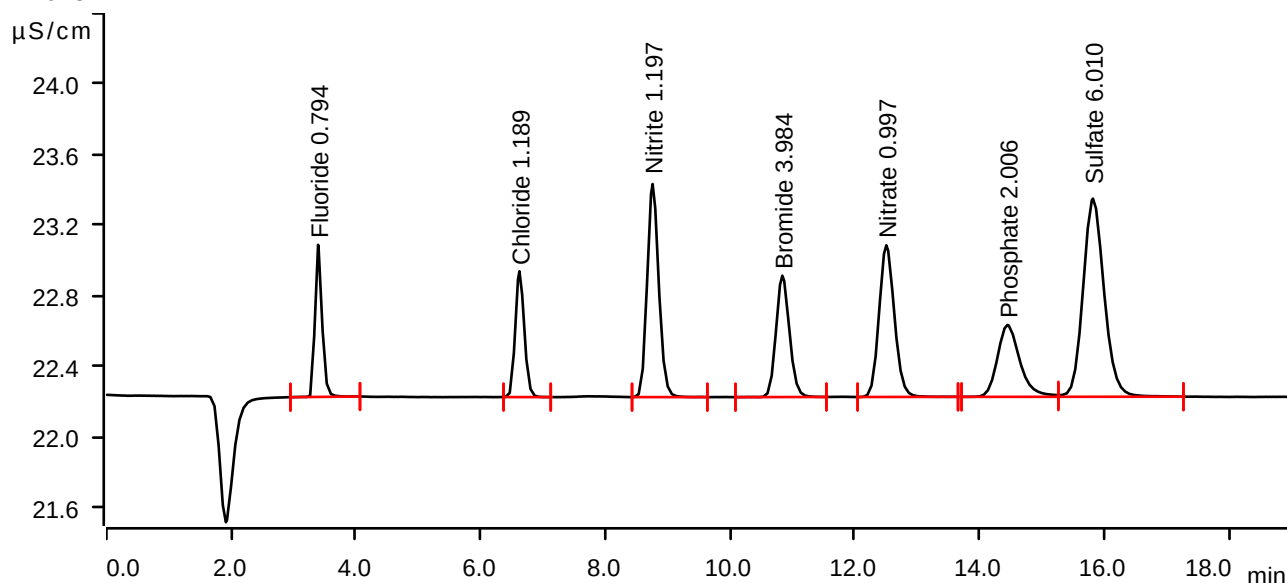

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.1137	0.861	0.794	Fluoride
2	6.623	0.1196	0.712	1.189	Chloride
3	8.758	0.2603	1.206	1.197	Nitrite
4	10.838	0.1713	0.687	3.984	Bromide
5	12.505	0.2450	0.859	0.997	Nitrate
6	14.448	0.1697	0.407	2.006	Phosphate
7	15.818	0.4404	1.122	6.010	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-09-09 11:47:10 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

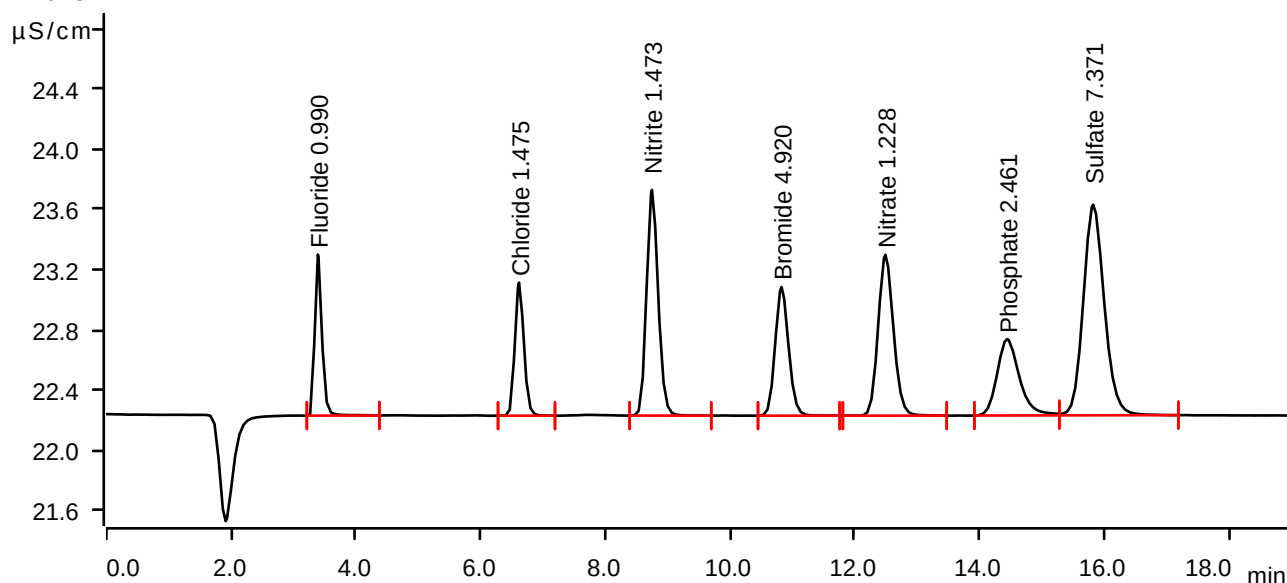

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.392	0.1426	1.068	0.990	Fluoride
2	6.617	0.1490	0.884	1.475	Chloride
3	8.748	0.3238	1.499	1.473	Nitrite
4	10.825	0.2129	0.854	4.920	Bromide
5	12.490	0.3046	1.068	1.228	Nitrate
6	14.443	0.2097	0.507	2.461	Phosphate
7	15.822	0.5468	1.398	7.371	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-09-09 13:36:36 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

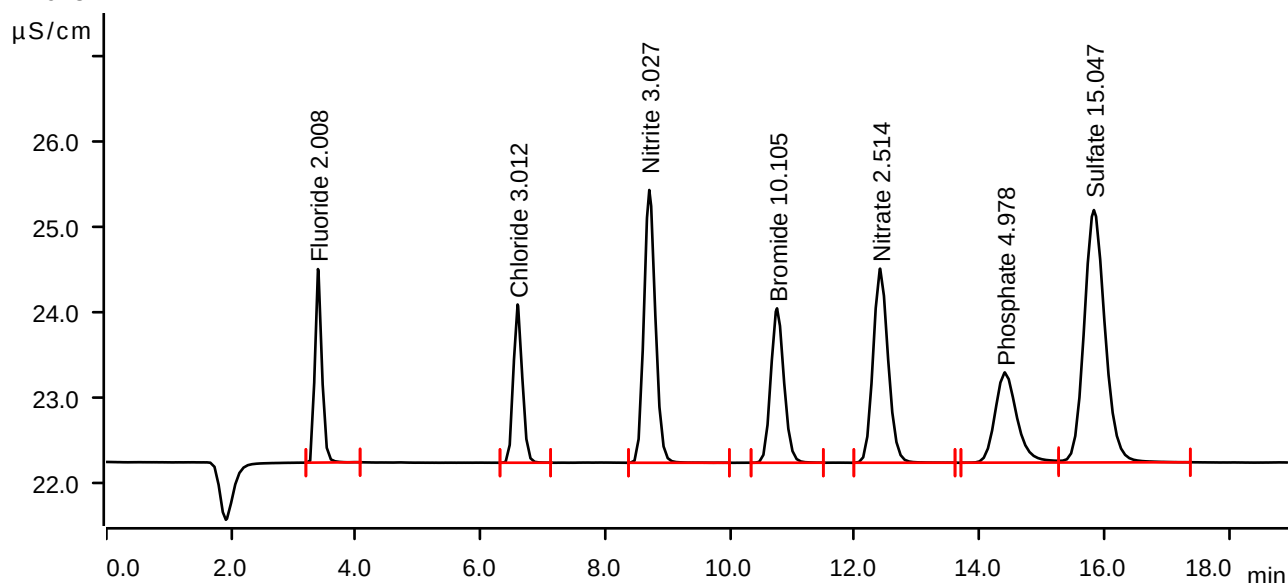

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2933	2.266	2.008	Fluoride
2	6.593	0.3075	1.854	3.012	Chloride
3	8.705	0.6805	3.195	3.027	Nitrite
4	10.753	0.4432	1.809	10.105	Bromide
5	12.407	0.6363	2.273	2.514	Nitrate
6	14.405	0.4310	1.057	4.978	Phosphate
7	15.833	1.1470	2.956	15.047	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-09-09 13:58:07 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

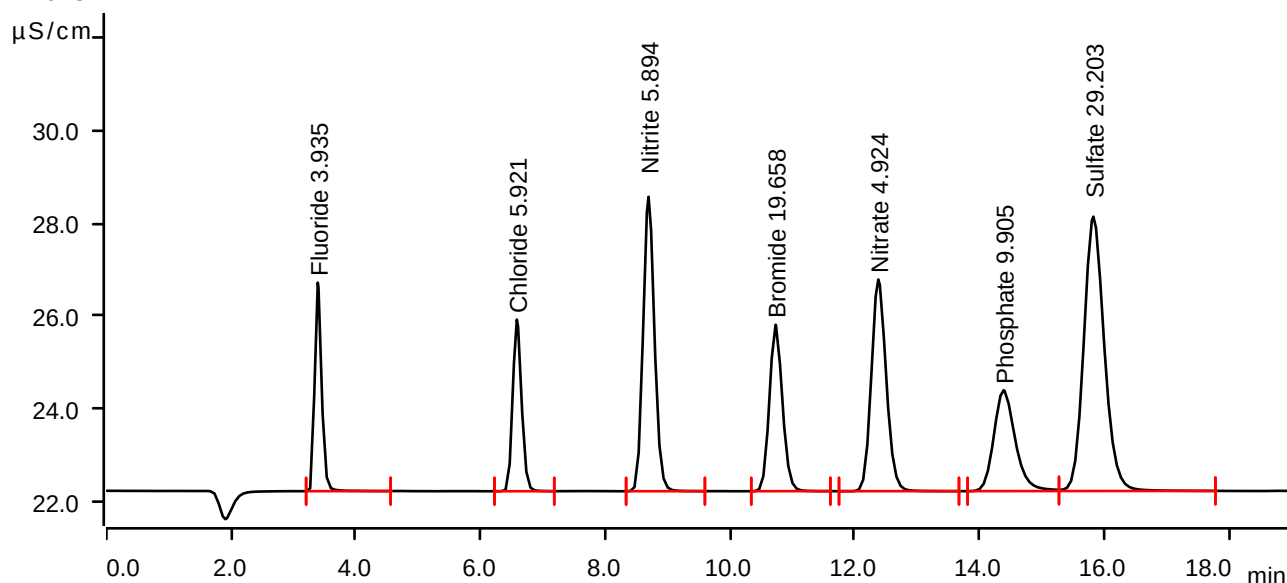

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.5787	4.477	3.935	Fluoride
2	6.582	0.6073	3.687	5.921	Chloride
3	8.693	1.3385	6.323	5.894	Nitrite
4	10.730	0.8677	3.574	19.658	Bromide
5	12.377	1.2581	4.546	4.924	Nitrate
6	14.385	0.8642	2.167	9.905	Phosphate
7	15.825	2.2540	5.893	29.203	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-09-09 14:41:06 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

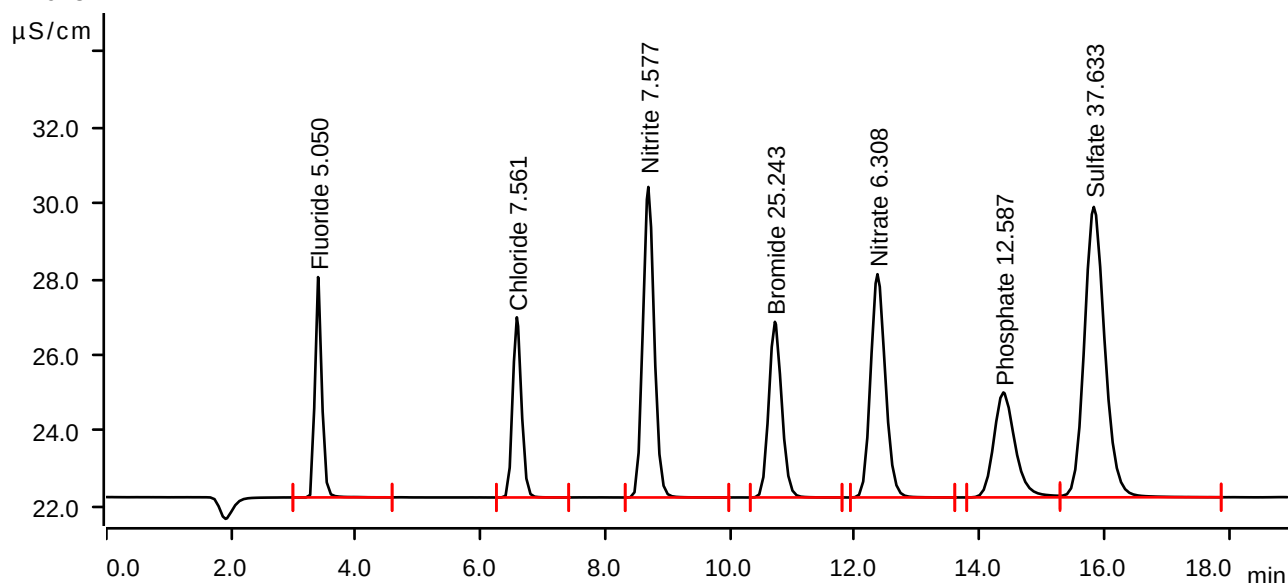

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.7438	5.806	5.050	Fluoride
2	6.582	0.7764	4.748	7.561	Chloride
3	8.690	1.7250	8.184	7.577	Nitrite
4	10.718	1.1158	4.629	25.243	Bromide
5	12.363	1.6152	5.884	6.308	Nitrate
6	14.382	1.1001	2.766	12.587	Phosphate
7	15.832	2.9131	7.654	37.633	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-09-09 15:02:34 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

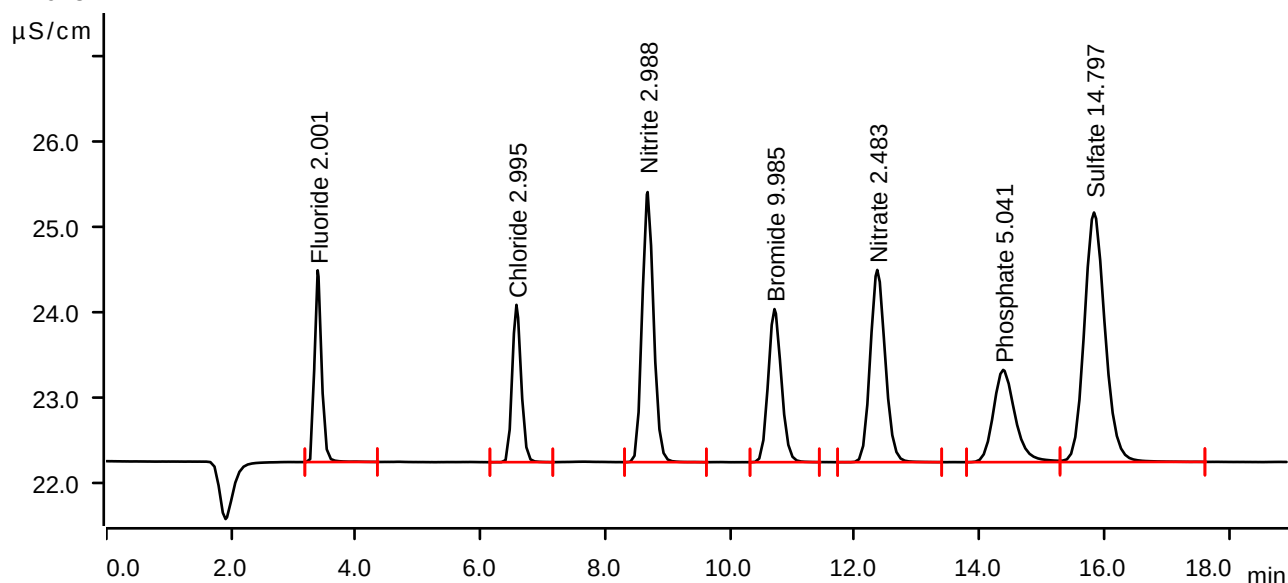

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.2923	2.246	2.001	Fluoride
2	6.575	0.3057	1.843	2.995	Chloride
3	8.678	0.6715	3.164	2.988	Nitrite
4	10.712	0.4379	1.793	9.985	Bromide
5	12.360	0.6282	2.252	2.483	Nitrate
6	14.378	0.4365	1.080	5.041	Phosphate
7	15.835	1.1275	2.923	14.797	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-09-09 15:45:30 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

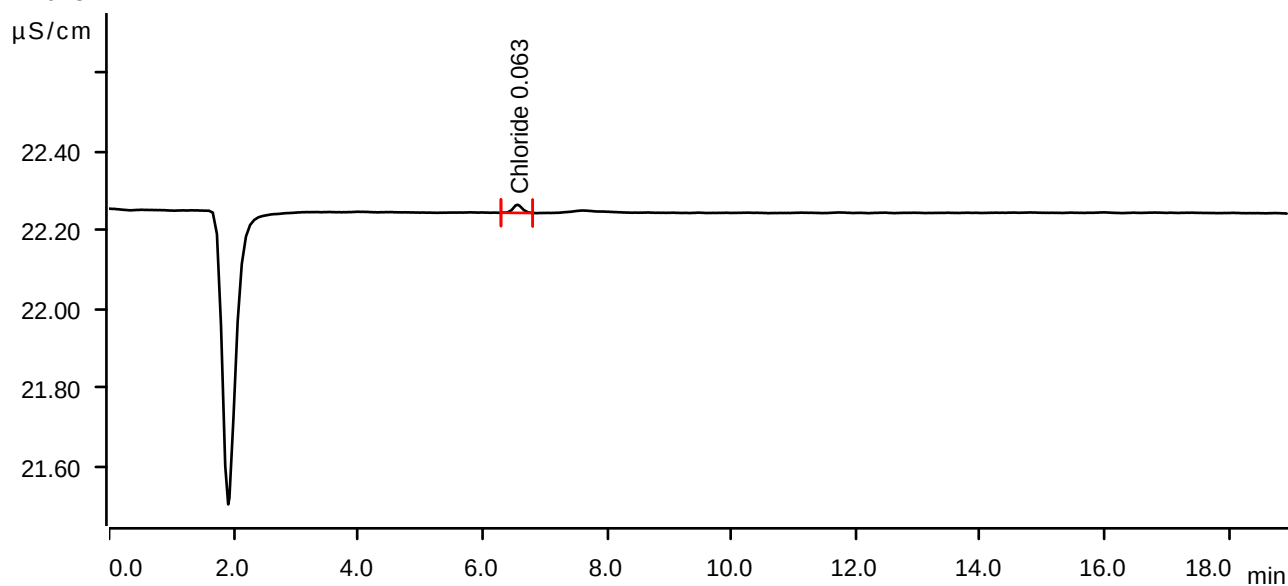

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.568	0.0036	0.021	0.063	Chloride


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-09-11 10:23:51 UTC-4
 Method IC1-090925
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.84 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

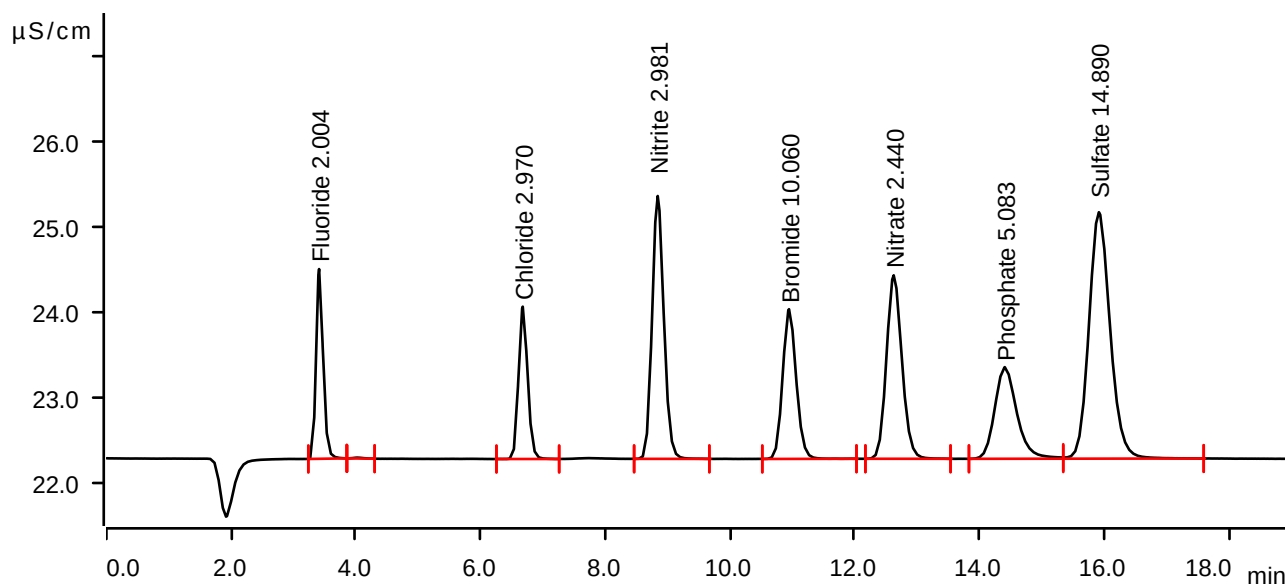

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.412	0.2928	2.222	2.004	Fluoride
2	4.022	0.0019	0.010	invalid	
3	6.677	0.3031	1.784	2.970	Chloride
4	8.840	0.6700	3.079	2.981	Nitrite
5	10.945	0.4413	1.754	10.060	Bromide
6	12.623	0.6173	2.149	2.440	Nitrate
7	14.405	0.4403	1.073	5.083	Phosphate
8	15.913	1.1347	2.887	14.890	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-11 10:45:22 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.78 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

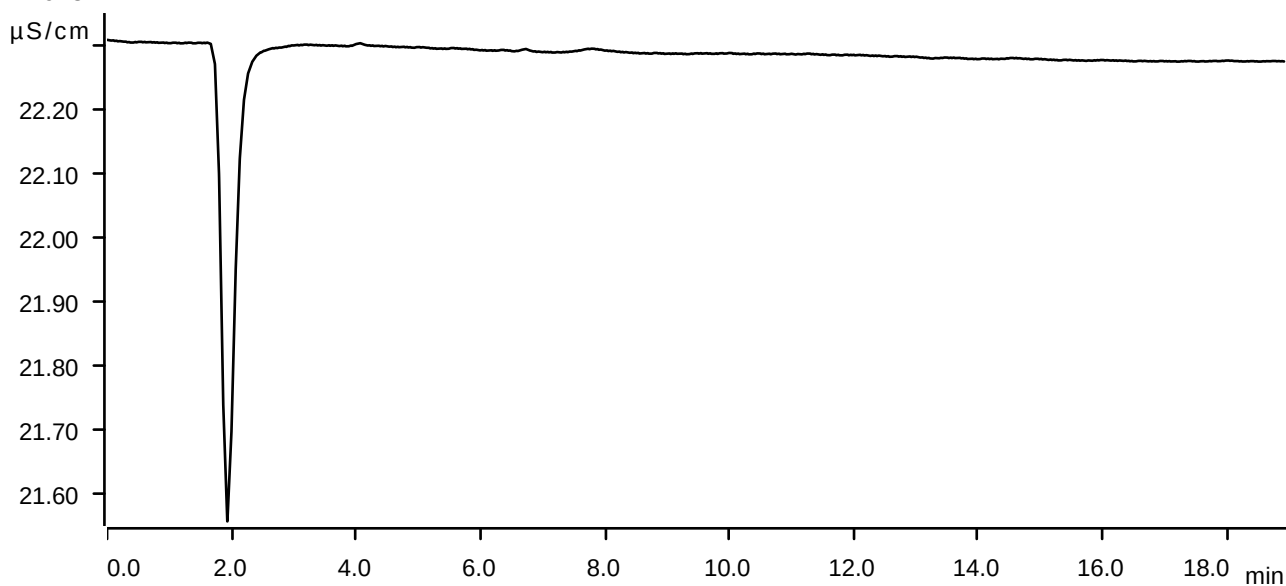


Sample data

Ident LB137171BLW
Sample type Sample
Determination start 2025-09-11 11:06:53 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.78 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

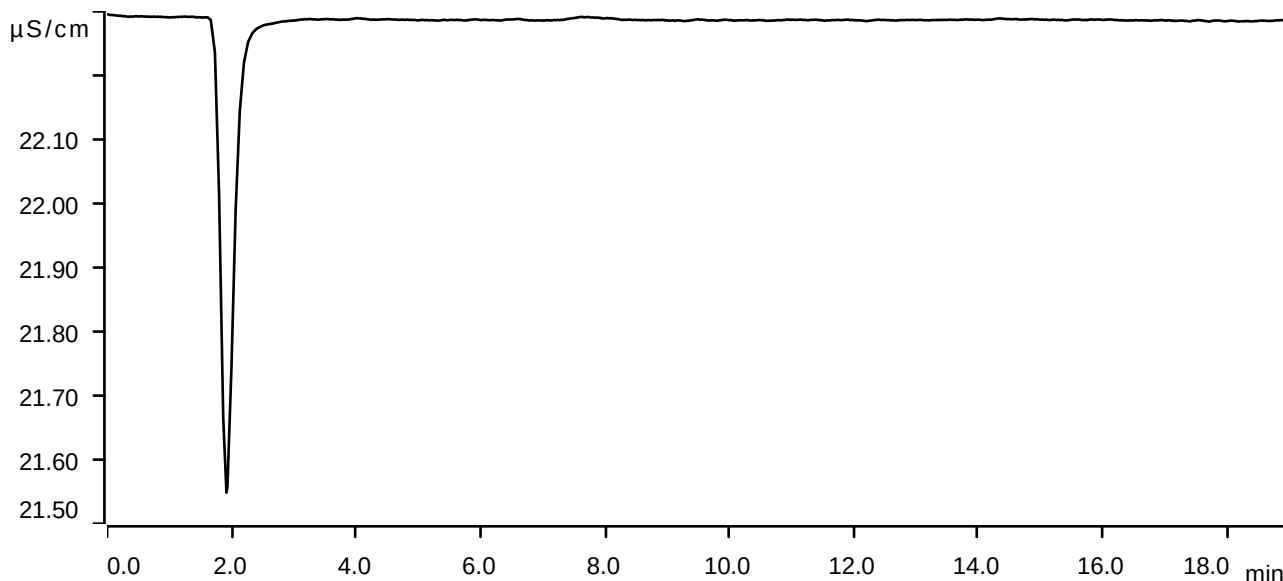


Sample data

Ident LB137171BSW
Sample type Check standard 1
Determination start 2025-09-11 11:28:24 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

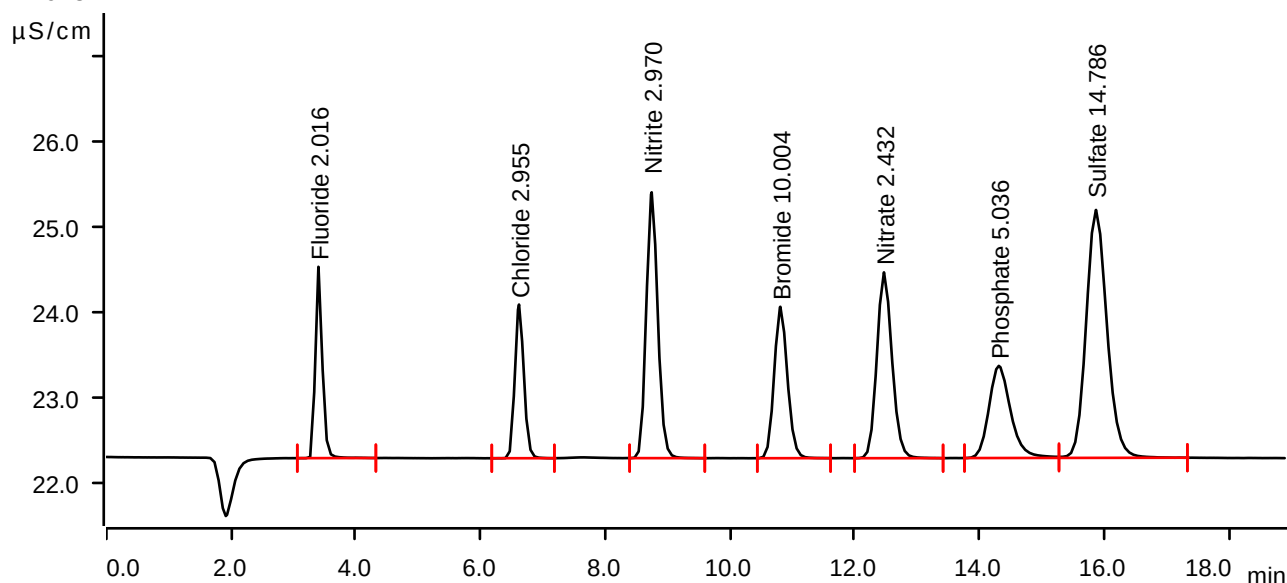

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.2946	2.241	2.016	Fluoride
2	6.617	0.3016	1.800	2.955	Chloride
3	8.743	0.6674	3.114	2.970	Nitrite
4	10.807	0.4388	1.774	10.004	Bromide
5	12.468	0.6152	2.177	2.432	Nitrate
6	14.308	0.4362	1.079	5.036	Phosphate
7	15.865	1.1267	2.904	14.786	Sulfate


Sample data

Ident Q3019-05
Sample type Sample
Determination start 2025-09-11 11:49:57 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

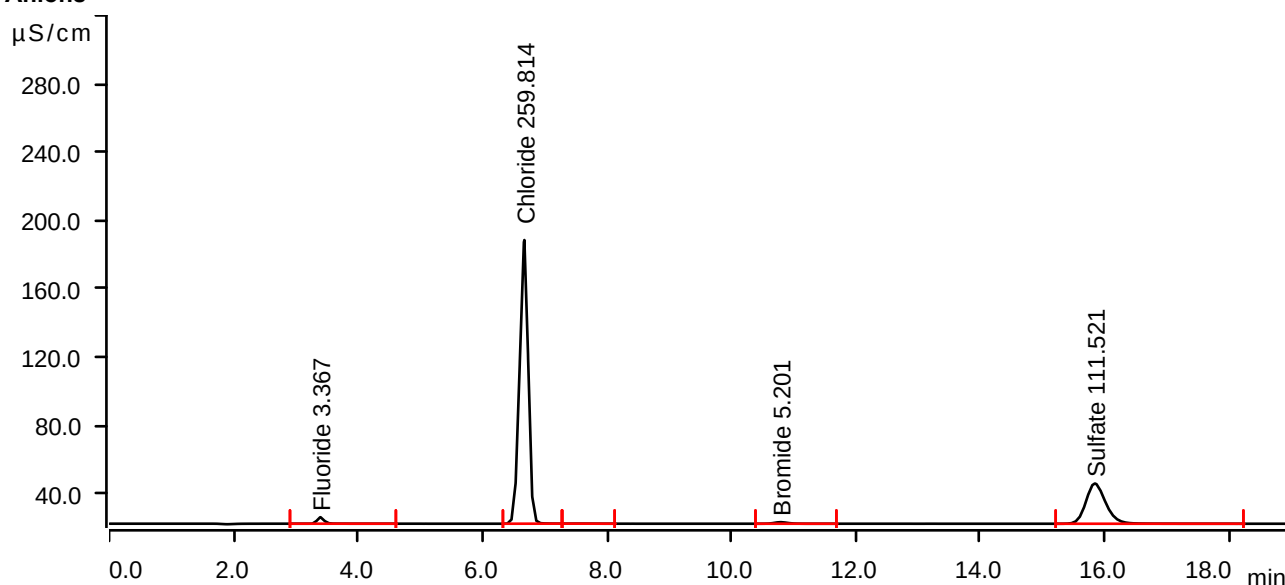

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.4946	3.799	3.367	Fluoride
2	6.675	26.7754	166.117	259.814	Chloride
3	7.502	0.0096	0.025	invalid	
4	10.792	0.2254	0.914	5.201	Bromide
5	15.842	8.6908	23.582	111.521	Sulfate


Sample data

Ident Q3019-11
Sample type Sample
Determination start 2025-09-11 12:33:04 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

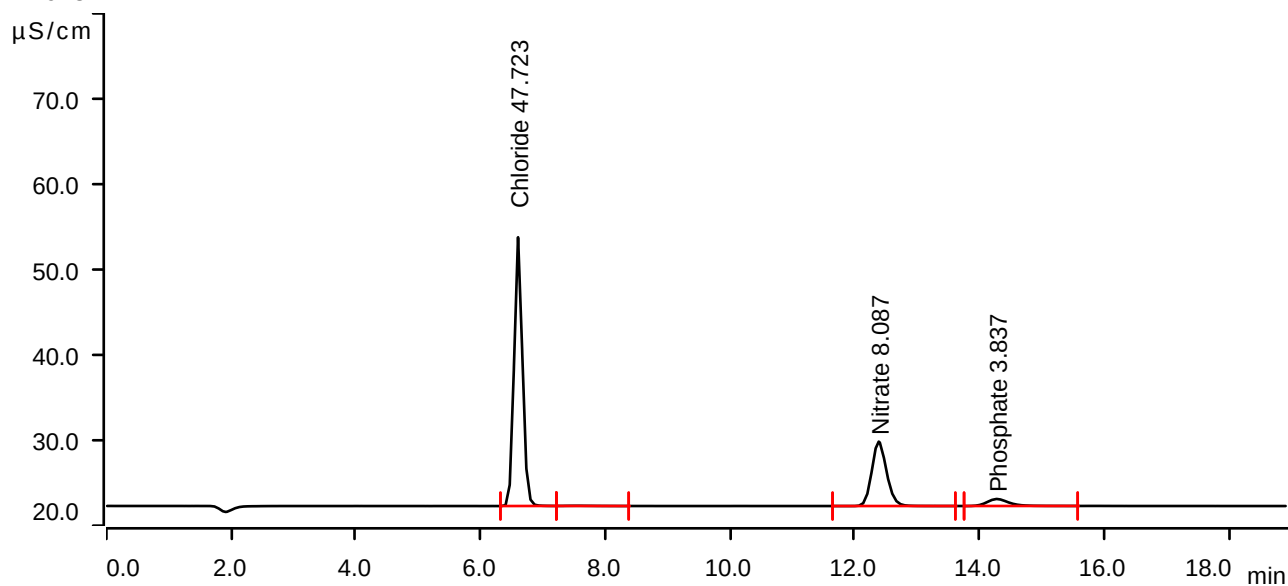

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.602	4.9157	31.480	47.723	Chloride
2	7.552	0.0102	0.023	invalid	
3	12.383	2.0742	7.546	8.087	Nitrate
4	14.278	0.3307	0.820	3.837	Phosphate


Sample data

Ident Q3019-15
Sample type Sample
Determination start 2025-09-11 12:54:38 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

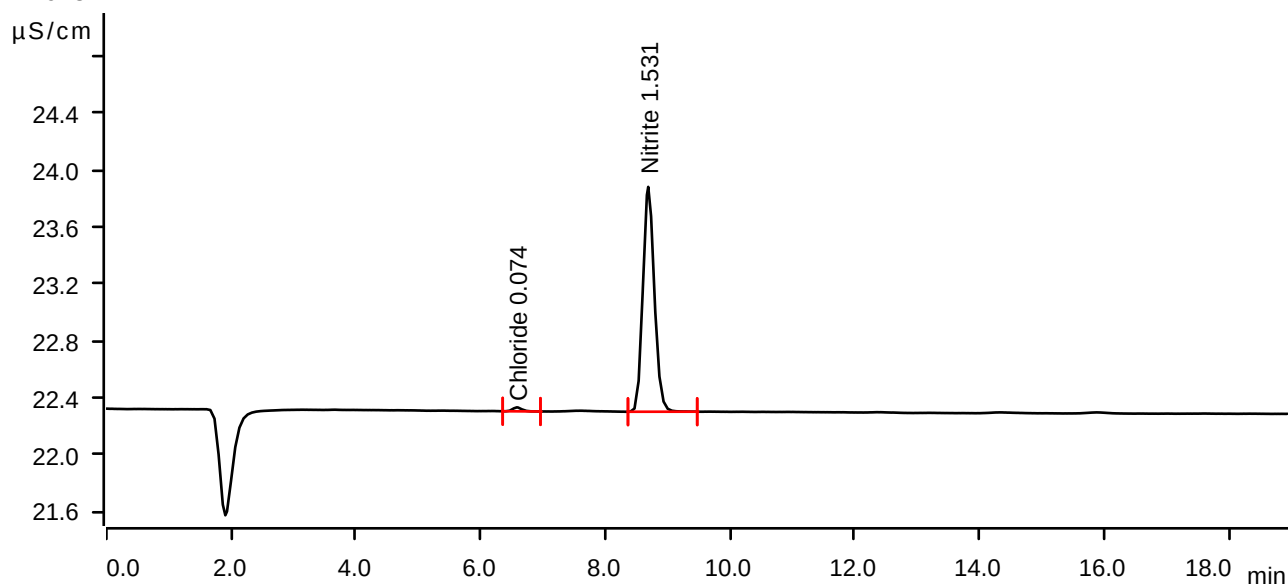

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	6.582	0.0047	0.028	0.074	Chloride
2	8.688	0.3371	1.580	1.531	Nitrite


Sample data

Ident Q3019-05DLX10
Sample type Sample
Determination start 2025-09-11 13:16:12 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

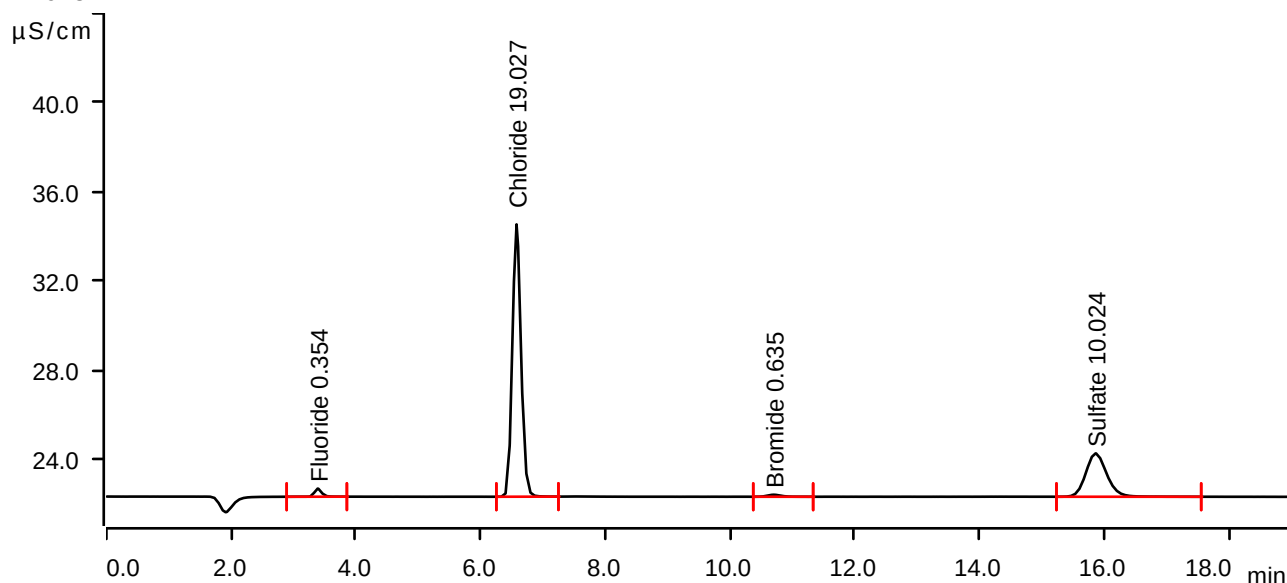

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.0485	0.366	0.354	Fluoride
2	6.577	1.9581	12.227	19.027	Chloride
3	10.698	0.0225	0.090	0.635	Bromide
4	15.860	0.7543	1.948	10.024	Sulfate


Sample data

Ident Q3019-05DL2X50
Sample type Sample
Determination start 2025-09-11 13:37:47 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

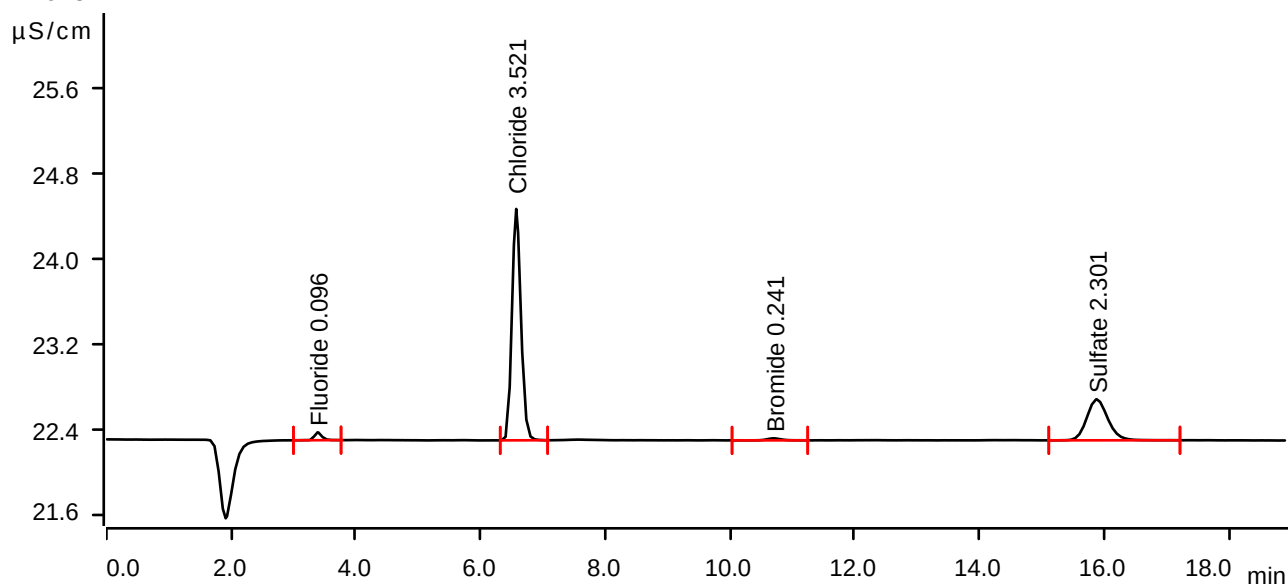

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.0102	0.074	0.096	Fluoride
2	6.572	0.3599	2.168	3.521	Chloride
3	10.708	0.0050	0.019	0.241	Bromide
4	15.878	0.1503	0.385	2.301	Sulfate


Sample data

Ident Q3019-11DLX2
Sample type Sample
Determination start 2025-09-11 13:59:22 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.63 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

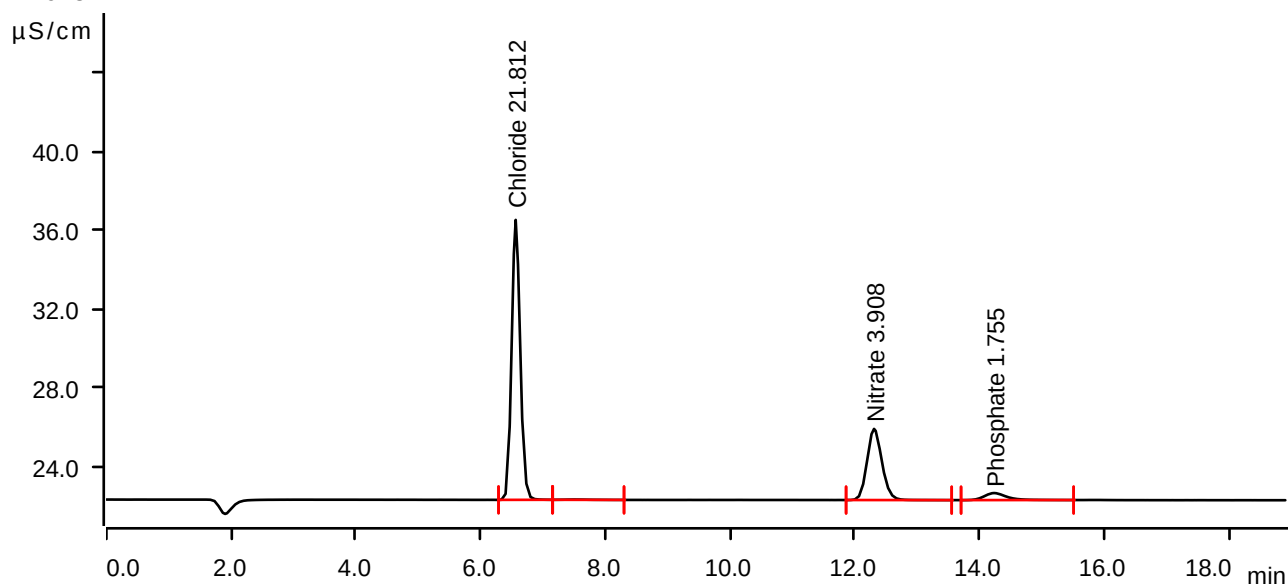

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.563	2.2451	14.208	21.812	Chloride
2	7.515	0.0068	0.015	invalid	
3	12.308	0.9960	3.613	3.908	Nitrate
4	14.233	0.1476	0.357	1.755	Phosphate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-11 14:20:56 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

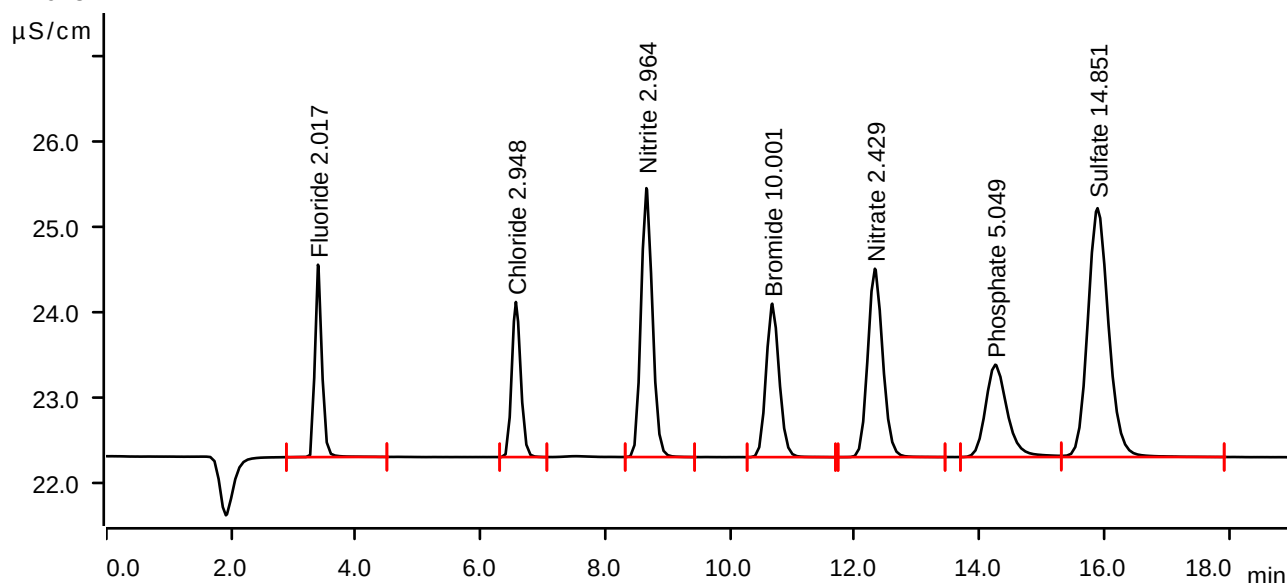


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2948	2.253	2.017	Fluoride
2	6.567	0.3009	1.817	2.948	Chloride
3	8.658	0.6660	3.150	2.964	Nitrite
4	10.677	0.4387	1.798	10.001	Bromide
5	12.322	0.6143	2.207	2.429	Nitrate
6	14.252	0.4372	1.081	5.049	Phosphate
7	15.892	1.1317	2.915	14.851	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-11 14:42:15 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

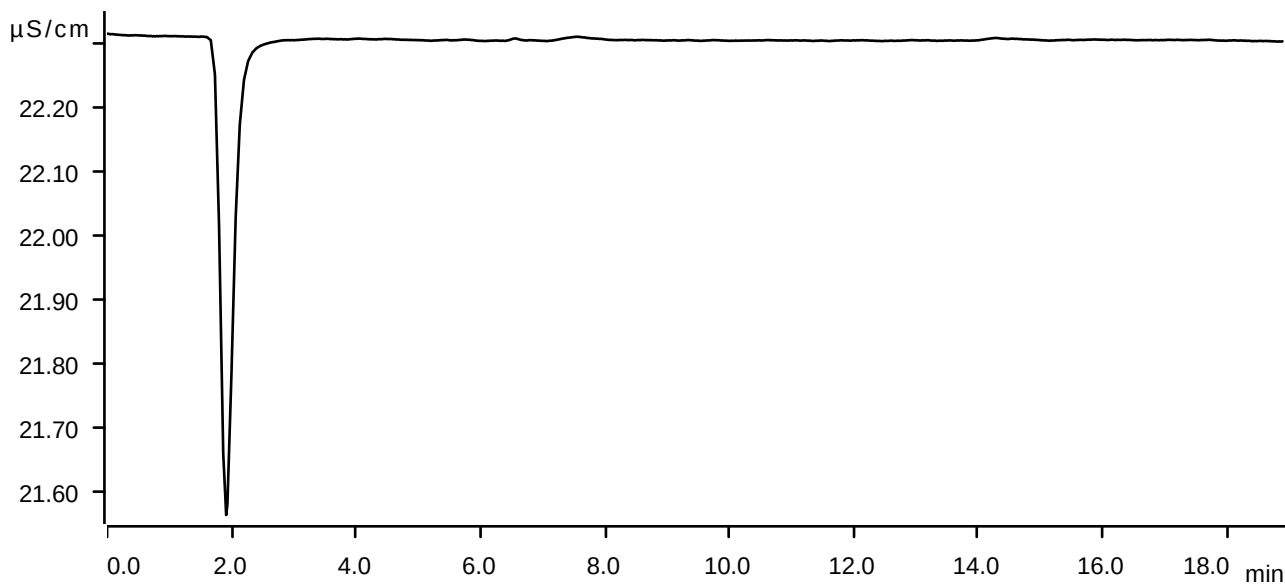Anions

LB137171
LB137172

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Anions-091125

WorkList ID : 191821

Department : Wet-Chemistry

Date : 09-11-2025 10:21:26

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3019-05	WP0925-PT-MIN1-WP	Water	Anions Group1	Cool 4 deg C	ALLI03	QA Of	09/02/2025	300.0
Q3019-06	WP0925-PT-MIN1-WP	Water	Anions Group1	Cool 4 deg C	ALLI03	QA Of	09/02/2025	9056A
Q3019-11	WP0925-PT-NUT1-WP	Water	Anions Group2	Cool 4 deg C	ALLI03	QA Of	09/02/2025	300.0
Q3019-12	WP0925-PT-NUT1-WP	Water	Anions Group2	Cool 4 deg C	ALLI03	QA Of	09/02/2025	9056A
Q3019-15	WP0925-PT-NUT3-WP	Water	Anions Group4	Cool 4 deg C	ALLI03	QA Of	09/02/2025	300.0
Q3019-16	WP0925-PT-NUT3-WP	Water	Anions Group5	Cool 4 deg C	ALLI03	QA Of	09/02/2025	9056A

Date/Time 09/11/25 10:30
Raw Sample Received by: 12 (WC)
Raw Sample Relinquished by: ST (QA)

Date/Time NA
Raw Sample Received by: 11
Raw Sample Relinquished by: 11