


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090525\
Data File : VN087732.D
Acq On : 05 Sep 2025 09:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

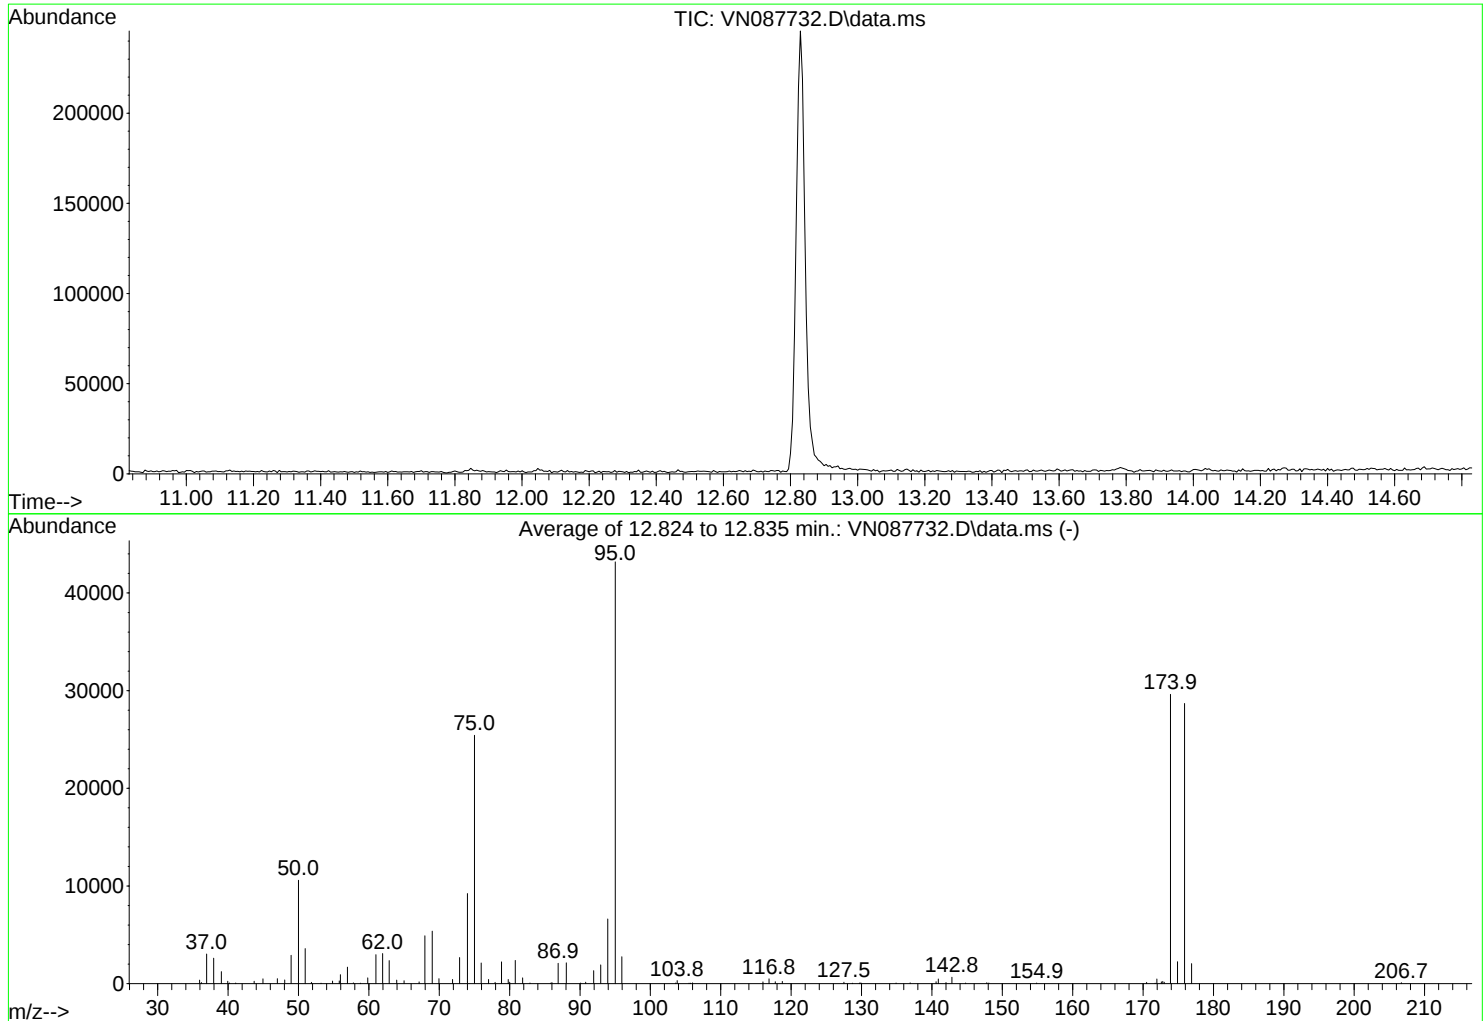

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.5	10582	PASS
75	95	30	60	58.9	25432	PASS
95	95	100	100	100.0	43189	PASS
96	95	5	9	6.4	2749	PASS
173	174	0.00	2	0.8	232	PASS
174	95	50	100	68.6	29629	PASS
175	174	5	9	7.6	2241	PASS
176	174	95	101	96.8	28683	PASS
177	176	5	9	7.2	2057	PASS

Average of 12.824 to 12.835 min.: VN087732.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	368	48.05	371	58.80	51	71.90	431
36.20	120	48.95	2901	59.85	588	72.90	267
36.95	3026	50.00	10582	61.00	2974	74.00	922
37.95	2613	50.95	3588	61.95	3087	75.00	2543
39.05	1232	51.85	134	62.90	2357	75.95	2115
39.95	240	53.20	55	63.95	360	77.00	433
40.20	66	54.85	261	65.00	289	77.95	138
41.10	69	55.80	277	67.15	178	78.85	2234
43.70	245	55.95	915	67.95	4907	79.80	430
44.95	497	56.95	1692	69.00	5378	80.00	148
47.00	516	57.80	76	69.95	510	80.80	2382

Average of 12.824 to 12.835 min.: VN087732.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	589	95.00	43189	127.50	146	147.80	98
82.90	70	95.95	2749	128.70	55	148.10	60
85.80	51	103.60	74	129.70	75	154.90	65
86.00	121	103.80	307	129.90	89	170.50	138
86.90	2083	105.50	57	134.90	60	171.70	53
88.05	2134	105.70	56	136.90	77	171.95	468
90.10	74	106.00	84	140.60	197	172.60	182
90.80	144	116.00	179	140.90	472	172.80	232
91.95	1324	116.85	491	142.00	116	173.00	150
92.95	1916	117.75	190	142.85	658	173.90	29629
93.95	6627	118.75	223	144.80	62	174.90	2241

Average of 12.824 to 12.835 min.: VN087732.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.90	28683						
176.90	2057						
206.70	96						

Instrument :

MSVOA_N

ClientSampleId :

BFB