


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091025\
Data File : BG064328.D
Acq On : 10 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

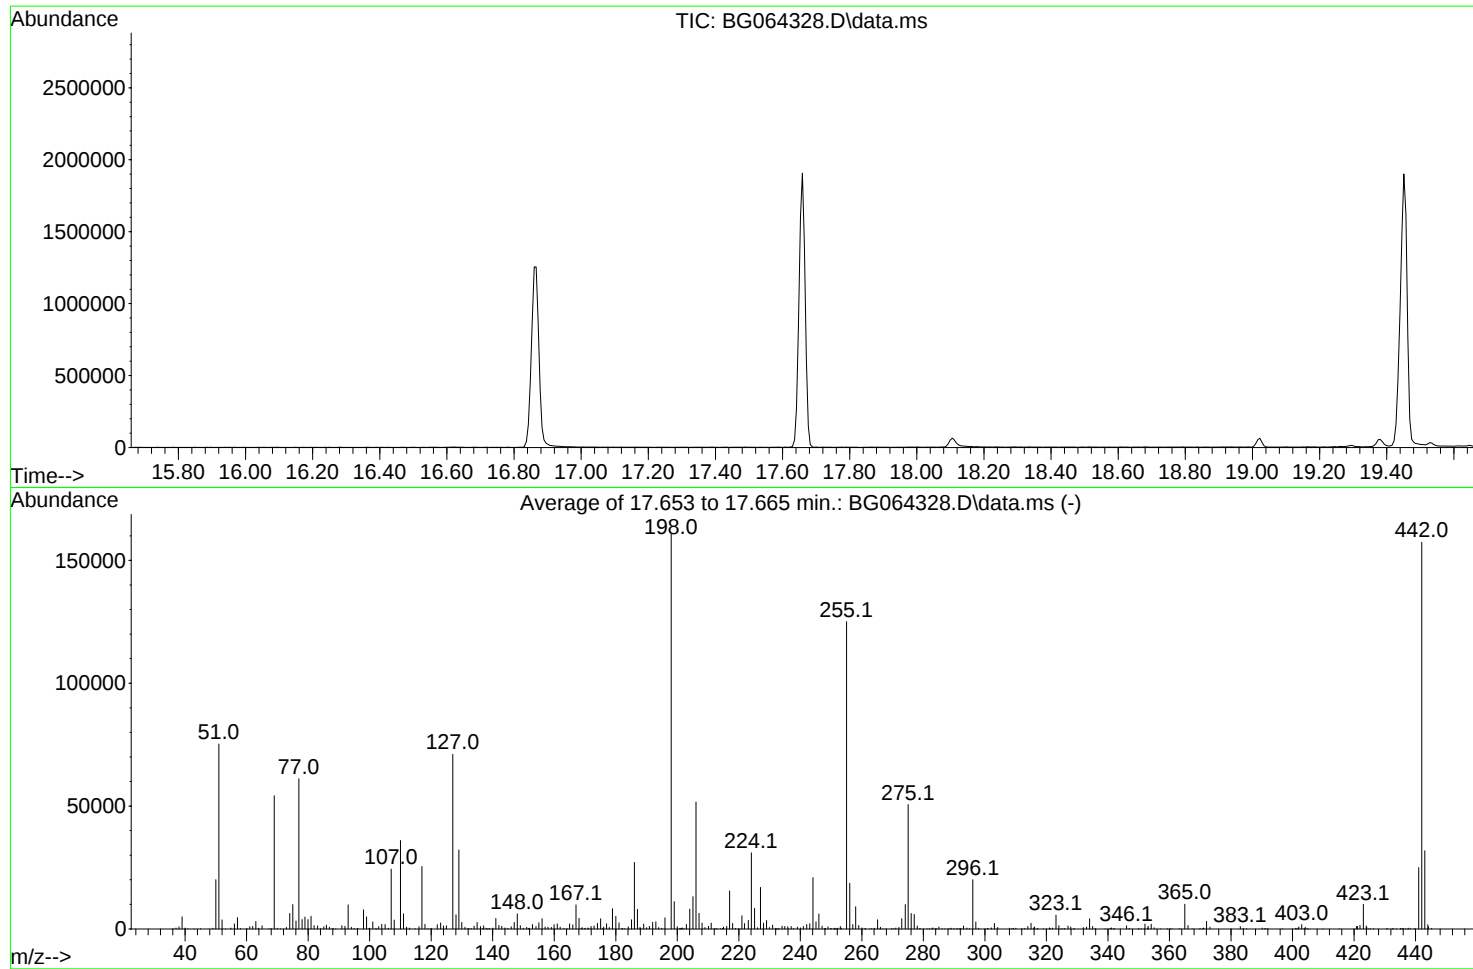




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.3	140	PASS
69	69	100	100	100.0	54224	PASS
70	69	0.00	2	0.6	321	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	160704	PASS
199	198	5	9	6.9	11109	PASS
365	198	1	100	6.3	10071	PASS
441	443	0.01	150	78.5	24955	PASS
442	442	100	100	100.0	157347	PASS
443	442	15	24	20.2	31784	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091025\
Data File : BG064328.D
Acq On : 10 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 10 12:18:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

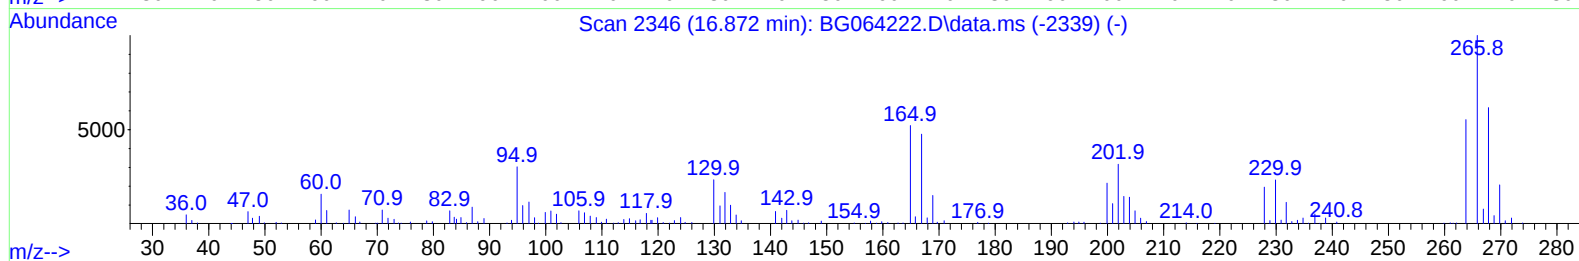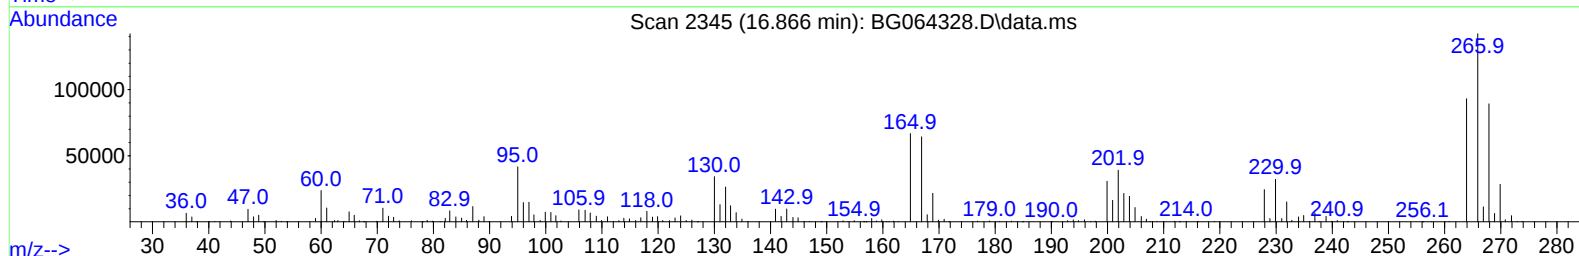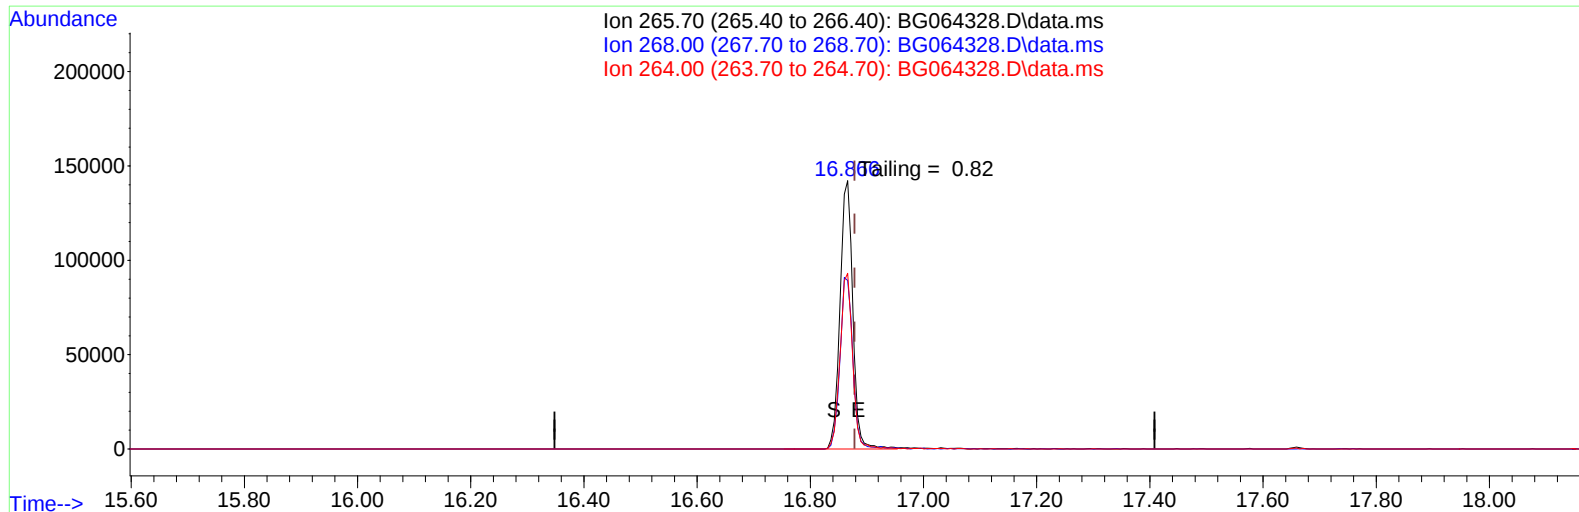

TIC: BG064328.D\data.ms

(70) Pentachlorophenol (C)

16.866min (-0.012) 579514.13 ng




response 223802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.79
264.00	55.40	65.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091025\
Data File : BG064328.D
Acq On : 10 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 10 12:18:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

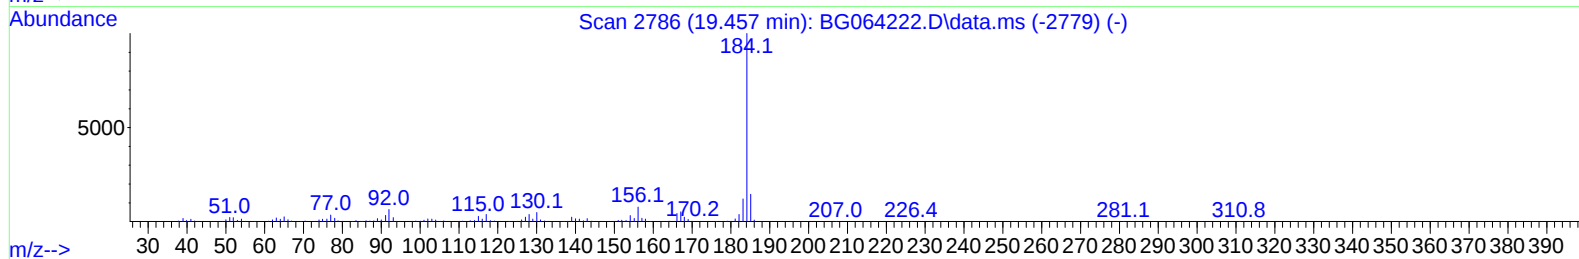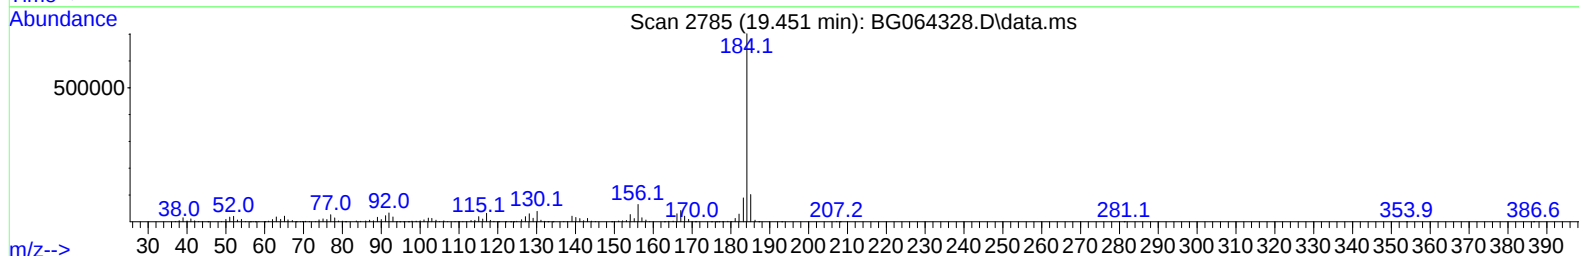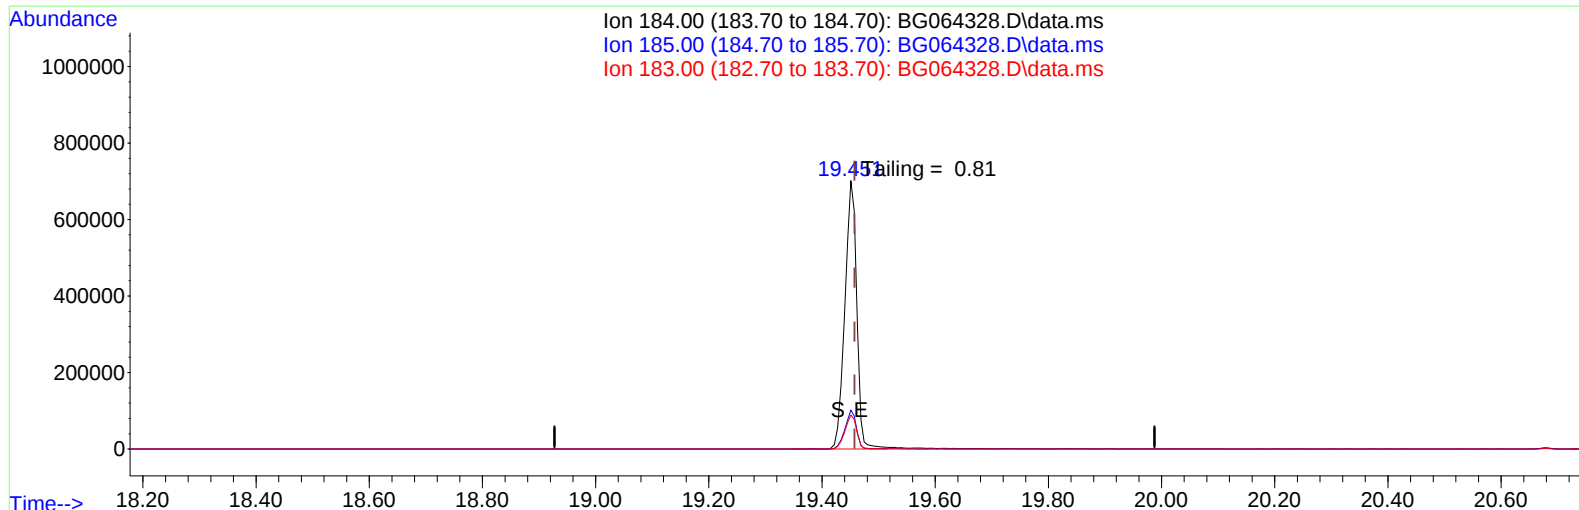

TIC: BG064328.D\data.ms

(77) Benzidine

19.451min (-0.006) 234970.81 ng

response 1028136

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.53
183.00	12.10	12.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2025	BNA_G	<u>BG064328.D</u>
Compound Name	Response	Retention Time
DDT	615490	20.679
DDD	10486	20.238
DDE	729	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11215	626705	1.79

Instrument :
BNA_G
ClientSampleId :
DFTPP