
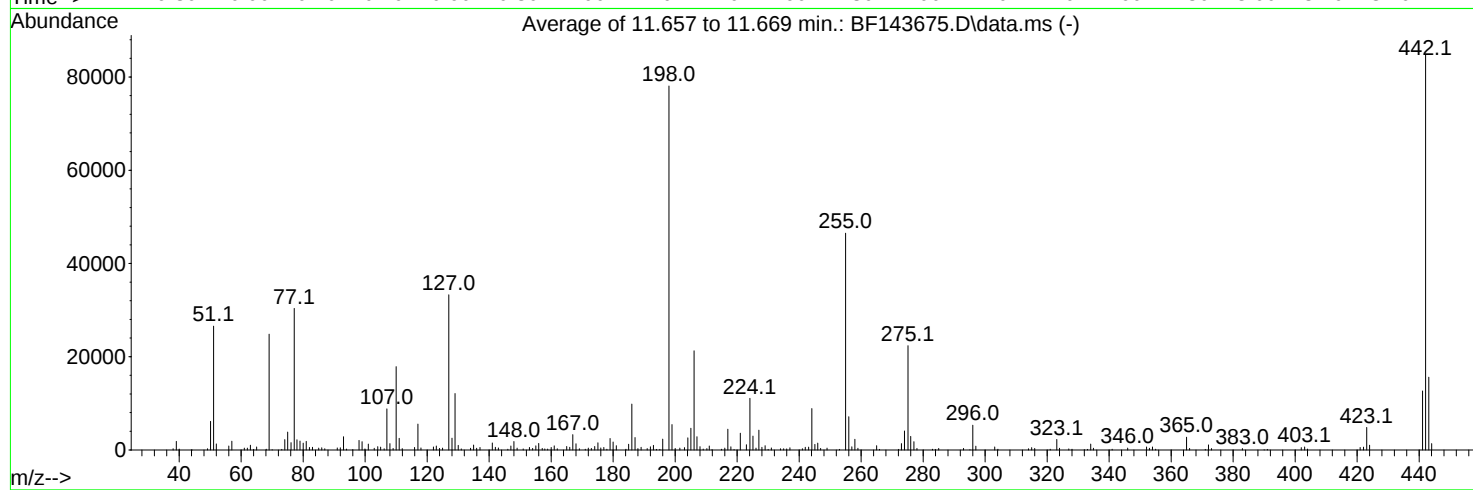


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091025\
Data File : BF143675.D
Acq On : 09 Sep 2025 08:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 09 15:20:16 2025

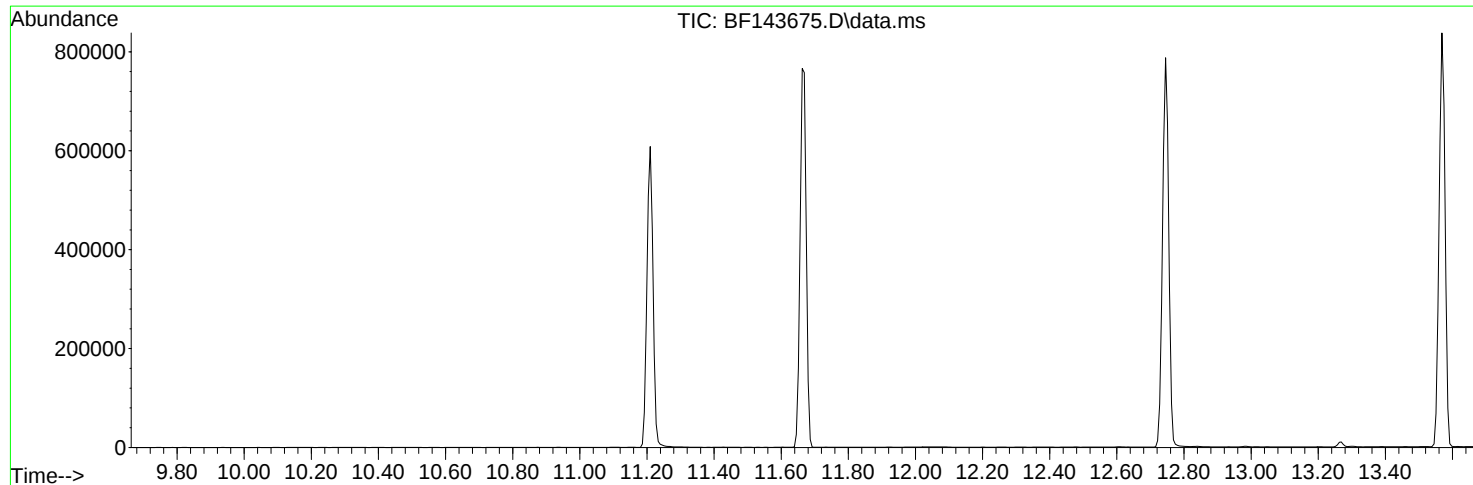




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.6	144	PASS
69	69	100	100	100.0	24837	PASS
70	69	0.00	2	0.2	62	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78083	PASS
199	198	5	9	7.0	5451	PASS
365	198	1	100	3.5	2728	PASS
441	443	0.01	150	81.0	12639	PASS
442	442	100	100	100.0	84704	PASS
443	442	15	24	18.4	15606	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091025\
Data File : BF143675.D
Acq On : 09 Sep 2025 08:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 09 11:56:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 11:54:23 2025
Response via : Initial Calibration

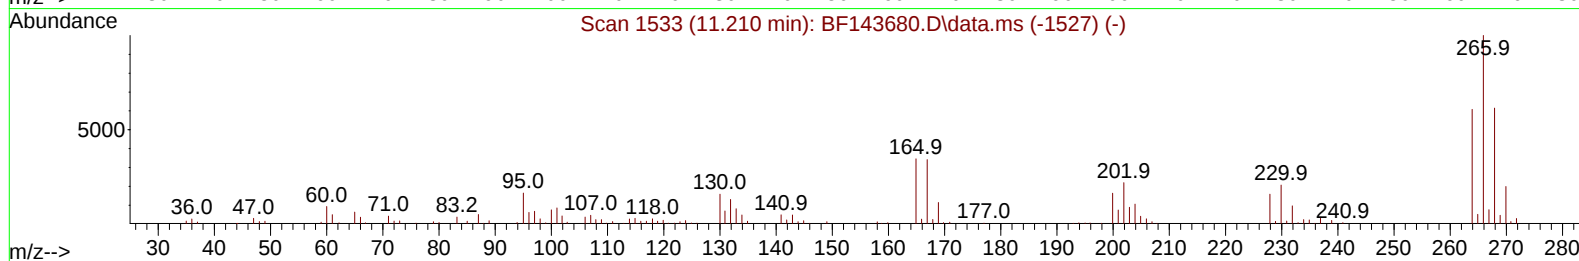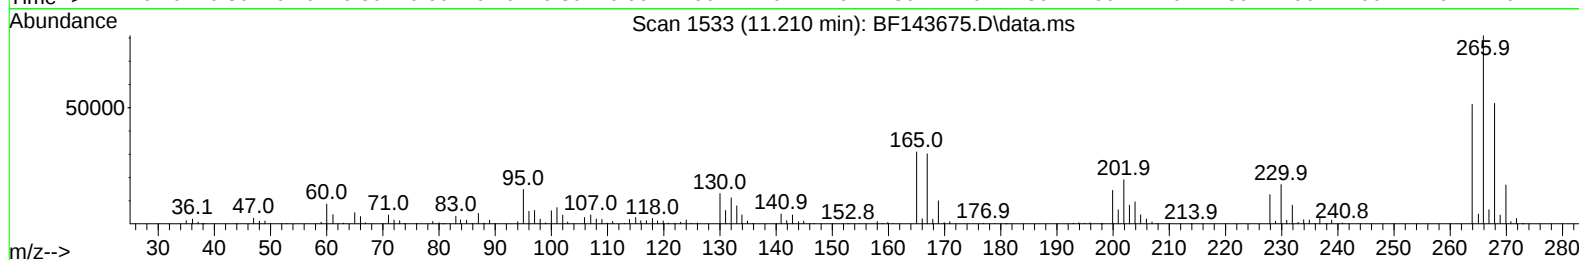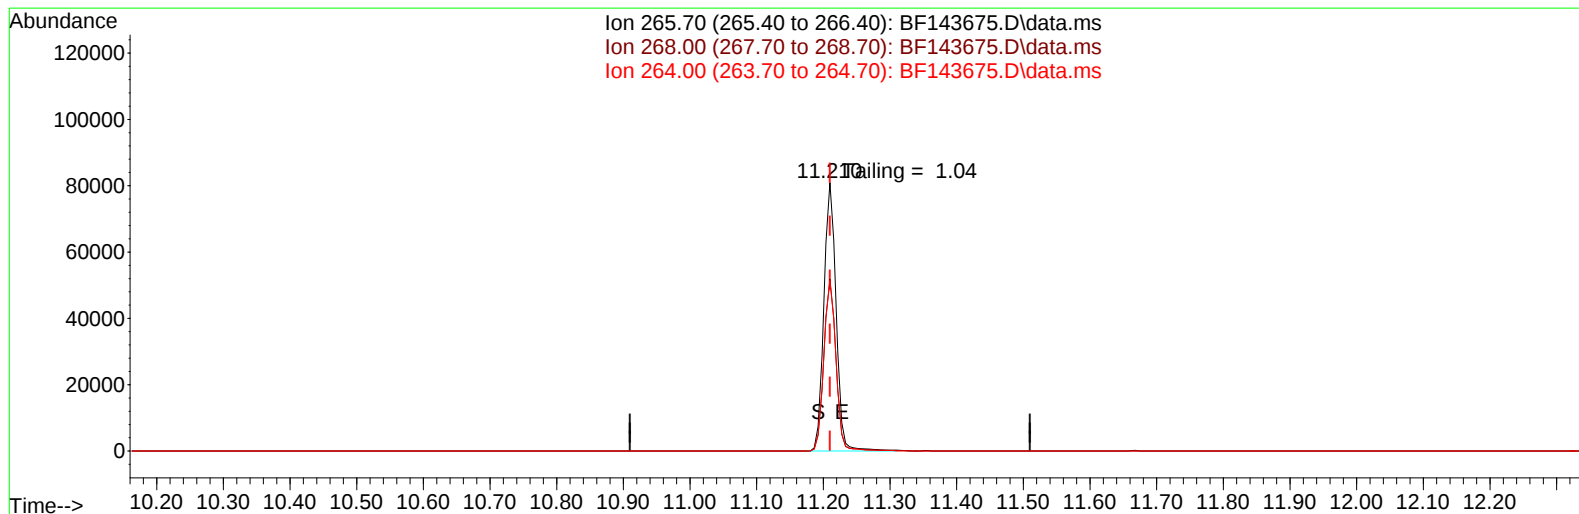

TIC: BF143675.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 33993.77 ng




response 103355

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	64.05
264.00	60.80	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091025\
Data File : BF143675.D
Acq On : 09 Sep 2025 08:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 09 11:56:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 11:54:23 2025
Response via : Initial Calibration

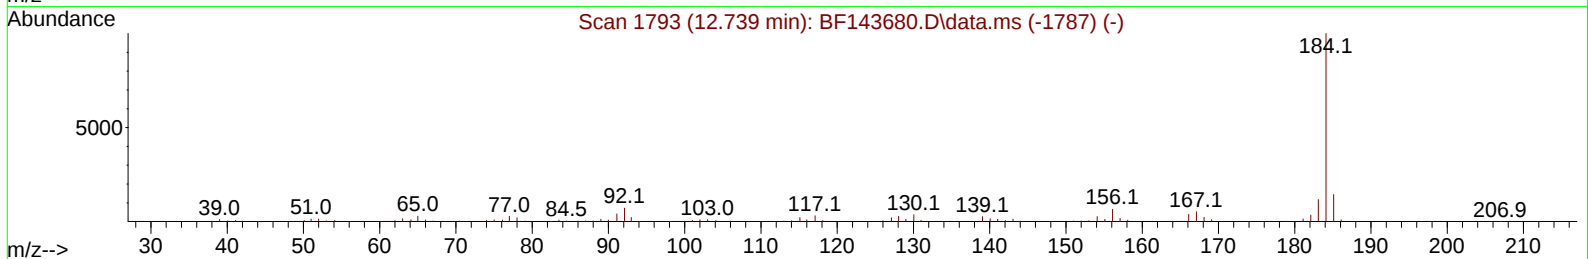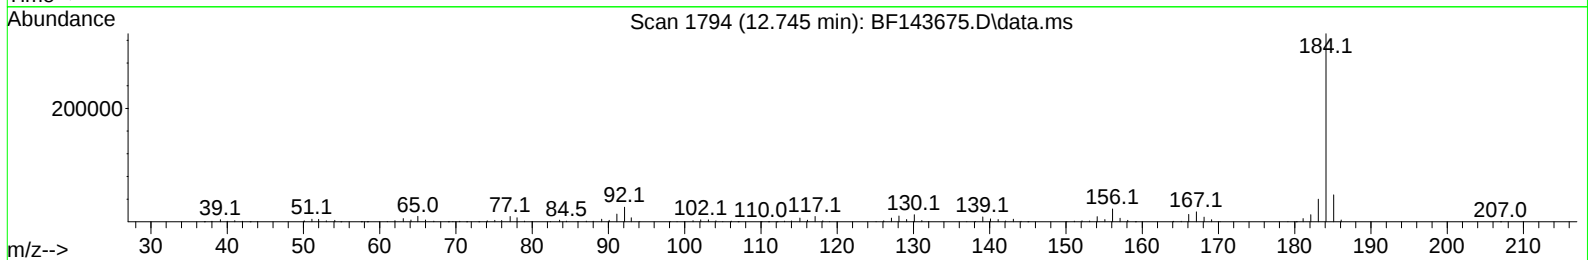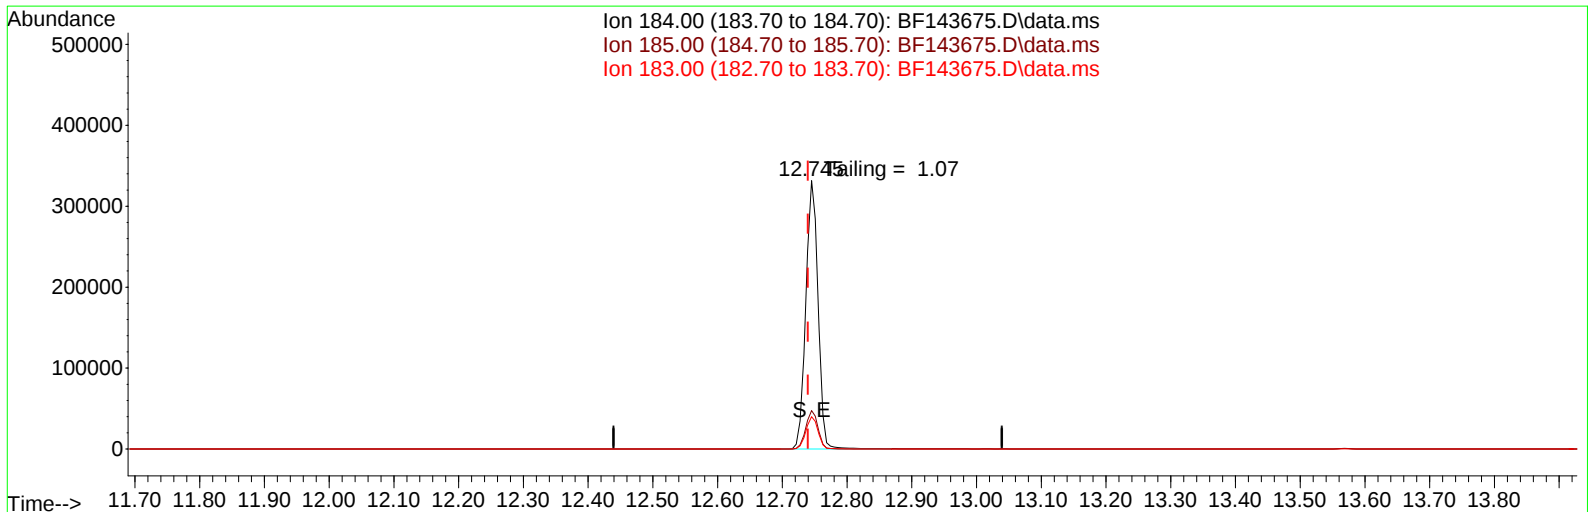

TIC: BF143675.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng

response 436264

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.34
183.00	11.80	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2025	BNA_F	<u>BF143675.D</u>
Compound Name	Response	Retention Time
DDT	210187	13.568
DDD	4000	13.269
DDE	110	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4110	214297	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP