
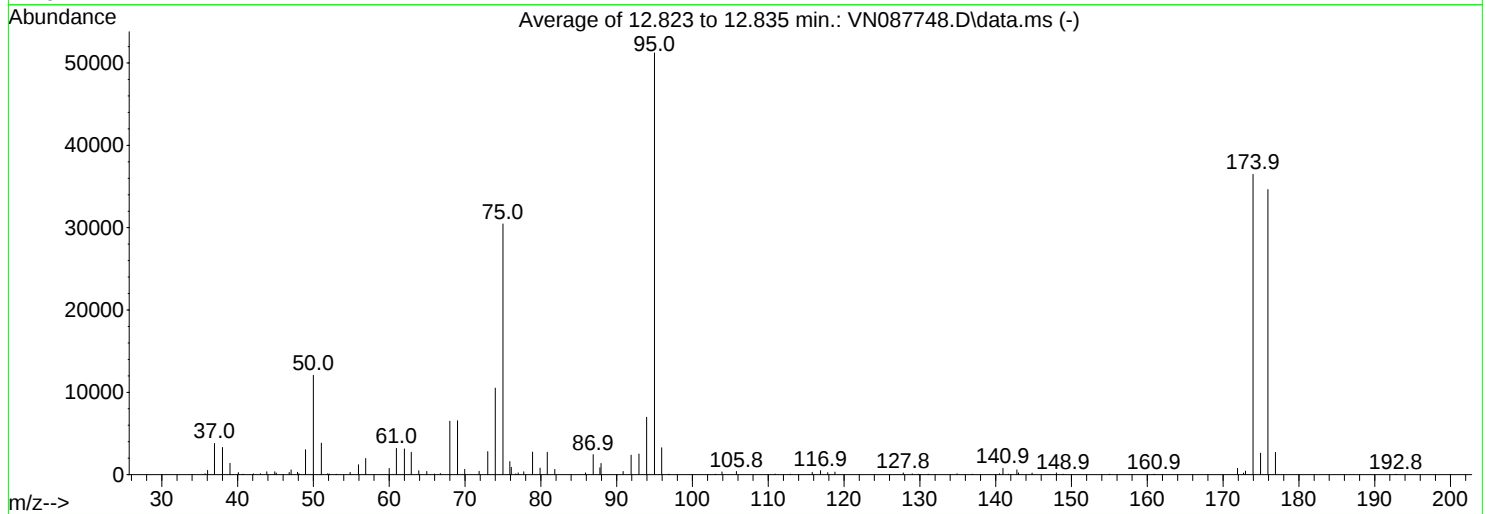


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN087748\
Data File : VN087748.D
Acq On : 08 Sep 2025 07:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

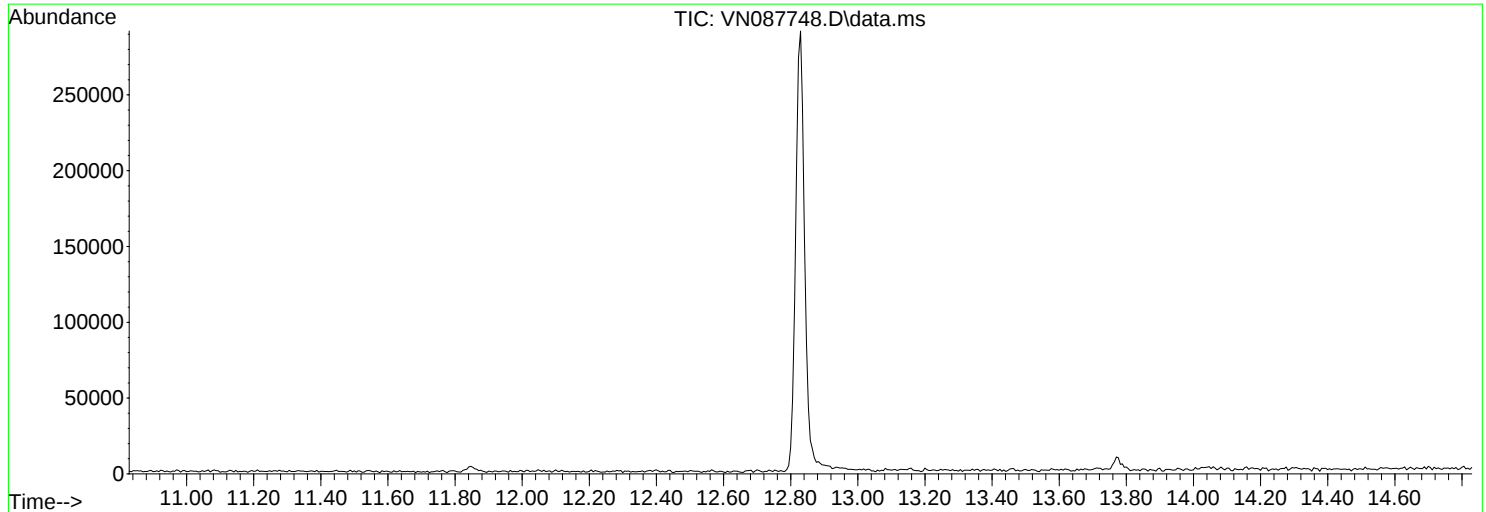

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	12076	PASS
75	95	30	60	59.4	30448	PASS
95	95	100	100	100.0	51237	PASS
96	95	5	9	6.4	3271	PASS
173	174	0.00	2	1.2	436	PASS
174	95	50	100	71.2	36485	PASS
175	174	5	9	7.1	2597	PASS
176	174	95	101	94.9	34635	PASS
177	176	5	9	7.8	2708	PASS

Average of 12.823 to 12.835 min.: VN087748.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	108	45.10	205	54.85	271	68.00	648
36.05	526	46.80	279	55.95	1206	69.00	654
36.95	3799	47.05	583	56.90	1964	69.95	63
38.00	3302	47.90	297	60.00	765	71.85	40
39.00	1377	48.10	114	60.95	3189	73.00	2808
40.10	260	48.95	3042	62.00	3134	74.00	10519
40.70	69	50.00	12076	62.90	2719	75.00	30448
42.10	98	51.05	3834	63.90	484	75.90	1593
43.00	123	51.90	118	64.95	399	76.10	898
43.85	347	52.10	72	66.00	77	76.70	92
44.90	361	53.00	63	66.75	136	77.00	214

Average of 12.823 to 12.835 min.: VN087748.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.75	346	92.95	2509	116.90	480	141.70	57
78.90	2745	93.95	6984	117.85	253	142.80	574
79.90	802	95.00	51237	118.80	311	143.00	209
80.85	2727	95.95	3271	127.80	219	144.80	191
81.85	639	96.90	57	129.00	103	148.00	224
85.90	207	103.00	52	129.80	50	148.90	63
86.90	2424	103.90	334	131.10	53	155.00	63
87.80	845	105.80	384	134.90	108	160.90	52
87.95	1356	110.90	70	136.90	57	171.90	755
90.85	380	112.90	63	140.50	118	172.70	187
91.90	2367	115.80	290	140.95	770	172.95	436

Average of 12.823 to 12.835 min.: VN087748.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.95	36485						
174.95	2597						
175.90	34635						
176.90	2708						
192.80	54						

Instrument :

MSVOA_N

ClientSampleId :

BFB