
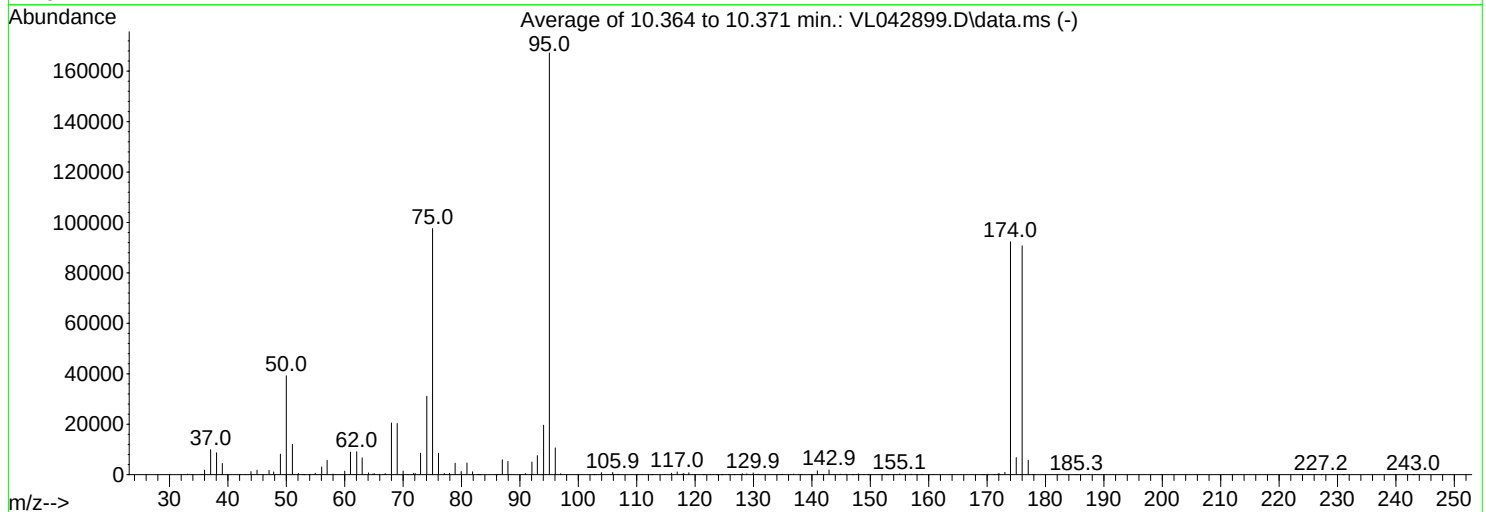


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090825\
Data File : VL042899.D
Acq On : 08 Sep 2025 08:41
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 09 00:52:26 2025

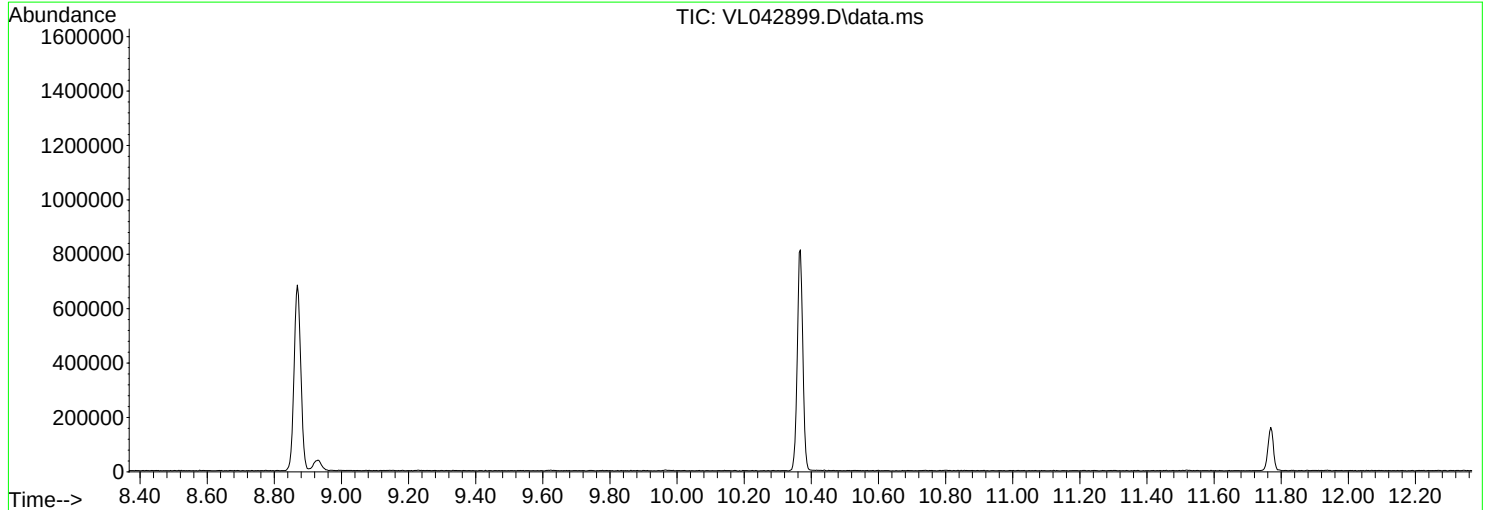

AutoFind: Scans 3175, 3176, 3177; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	39187	PASS
75	95	30	66	58.3	97600	PASS
95	95	100	100	100.0	167275	PASS
96	95	5	9	6.4	10626	PASS
173	174	0.00	2	1.0	912	PASS
174	95	50	120	55.2	92299	PASS
175	174	4	9	7.3	6771	PASS
176	174	93	101	98.3	90712	PASS
177	176	5	9	6.3	5742	PASS

Average of 10.364 to 10.371 min.: VL042899.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	277	47.05	1703	57.00	5718	68.00	2049
33.90	76	47.85	1098	58.00	264	69.00	2031
36.00	1753	49.00	8120	60.00	1371	70.00	145
37.05	9902	50.00	39187	61.00	8956	70.85	8
38.05	8709	51.05	12023	62.05	9092	71.80	573
39.05	4451	52.05	538	63.00	6674	72.10	455
42.20	43	52.80	70	64.10	689	73.00	8527
43.00	155	53.00	34	64.80	191	74.05	31123
43.95	1185	53.90	19	65.05	457	75.05	97600
45.00	1756	54.95	607	65.95	113	76.05	8503
46.10	88	56.05	3033	66.95	475	77.05	485

Average of 10.364 to 10.371 min.: VL042899.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	573	87.95	5283	104.75	99	118.05	490
78.90	4606	90.95	451	105.90	886	118.95	748
79.95	1303	92.05	4997	106.80	189	121.40	28
80.95	4620	93.00	7539	110.15	132	122.65	45
81.90	1148	94.05	19635	110.90	167	123.10	45
82.70	56	95.05	167275	112.00	165	123.70	23
82.90	163	96.05	10626	112.60	37	124.60	30
83.10	23	97.00	366	114.85	160	125.75	80
85.90	69	102.70	25	115.95	603	126.70	21
86.10	24	103.10	60	116.95	1113	127.80	118
87.00	5921	103.95	835	117.80	269	128.10	385

Average of 10.364 to 10.371 min.: VL042899.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.85	290	141.95	142	152.00	18	169.10	55
129.95	727	142.95	1818	152.70	36	169.40	20
130.80	191	143.80	58	153.00	24	170.20	135
131.10	55	144.85	184	154.00	144	171.20	19
134.05	42	145.85	181	154.45	64	171.80	185
134.70	75	147.00	27	155.05	308	172.05	532
134.95	219	147.70	102	156.00	56	173.05	912
136.85	269	147.95	342	157.00	194	174.00	92299
138.20	68	148.90	78	158.00	17	175.00	6771
140.00	141	149.60	29	158.85	156	176.00	90712
140.95	1550	150.00	159	160.75	151	177.05	5742

Average of 10.364 to 10.371 min.: VL042899.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.85	114						
178.10	127						
185.30	42						
227.20	22						
231.00	19						
243.00	18						