
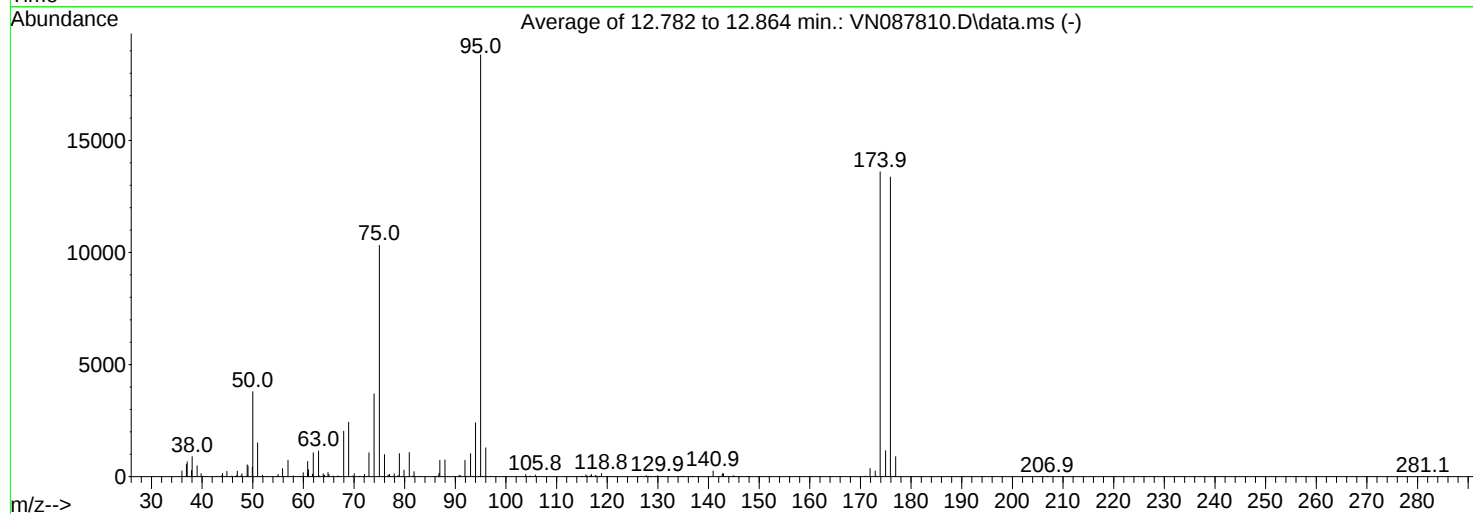


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091225\
Data File : VN087810.D
Acq On : 12 Sep 2025 08:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090425W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 05 03:29:53 2025

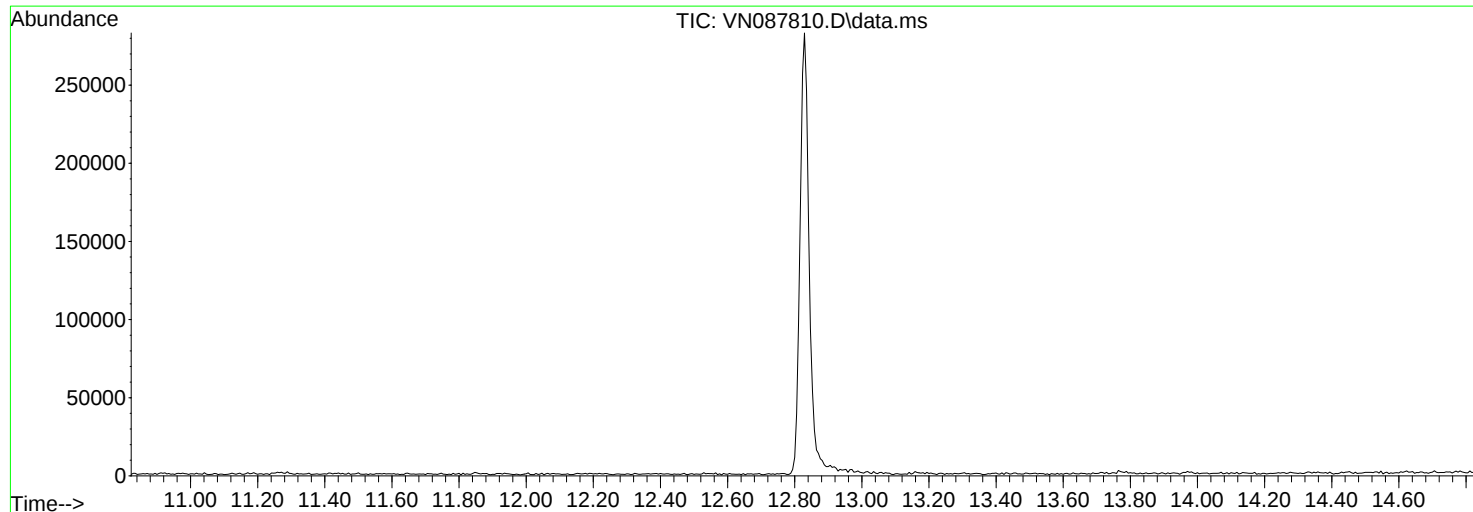

AutoFind: Averaged scan 1841 to 1855; Bkg corrected with scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	3792	PASS
75	95	30	60	54.8	10319	PASS
95	95	100	100	100.0	18821	PASS
96	95	5	9	6.8	1284	PASS
173	174	0.00	2	1.8	249	PASS
174	95	50	100	72.2	13598	PASS
175	174	5	9	8.5	1158	PASS
176	174	95	101	98.3	13372	PASS
177	176	5	9	6.7	894	PASS