
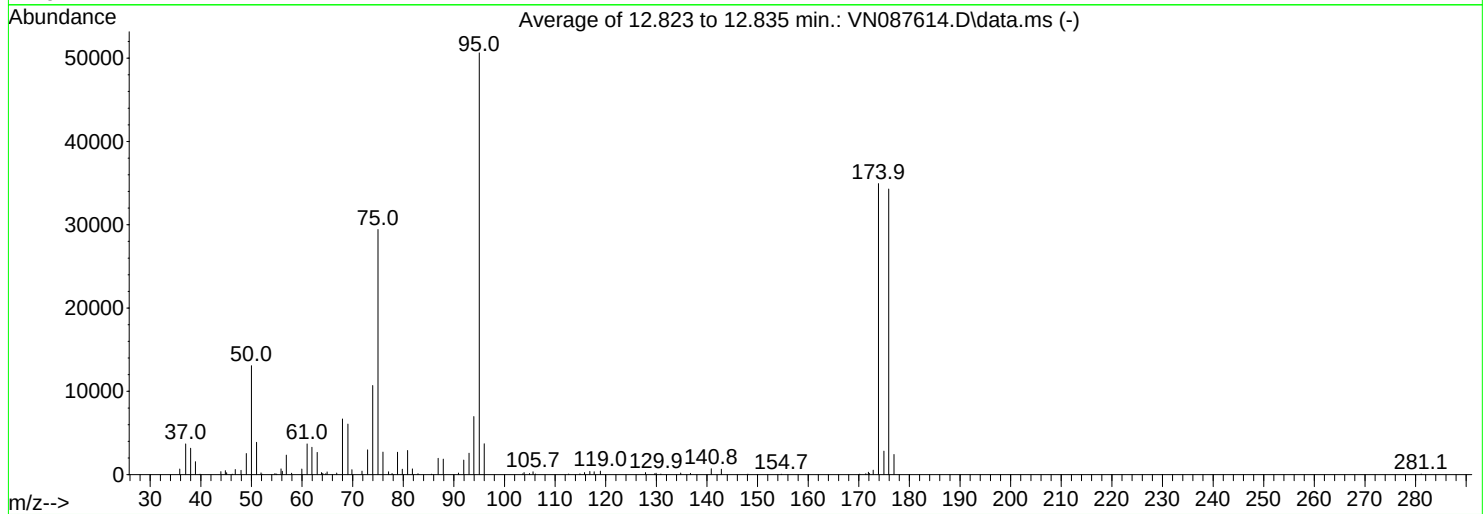


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082125\
Data File : VN087614.D
Acq On : 21 Aug 2025 09:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

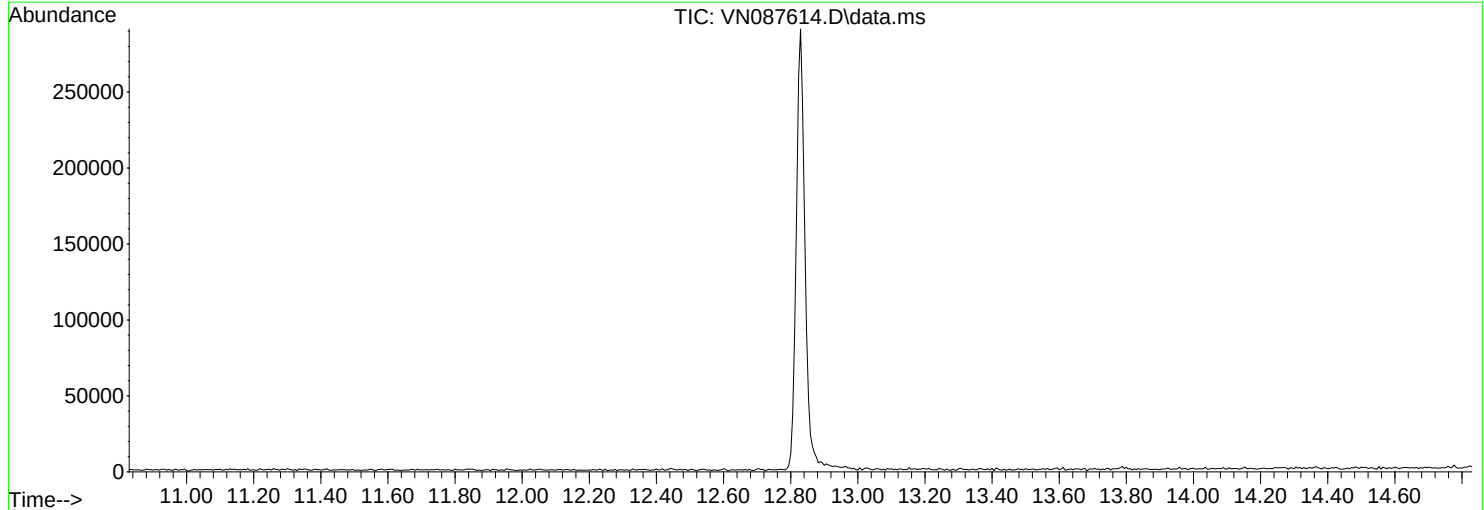

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.8	13089	PASS
75	95	30	60	58.1	29435	PASS
95	95	100	100	100.0	50640	PASS
96	95	5	9	7.3	3712	PASS
173	174	0.00	2	1.6	548	PASS
174	95	50	100	69.0	34952	PASS
175	174	5	9	8.1	2829	PASS
176	174	95	101	98.1	34291	PASS
177	176	5	9	7.1	2426	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	675	49.00	2529	59.95	672	69.85	591
37.00	3688	50.00	13089	61.00	3695	71.85	411
38.00	3178	51.00	3882	61.95	3294	72.95	297
38.95	1555	51.90	219	63.00	2681	73.95	1069
39.85	60	52.10	64	63.85	251	75.00	29435
43.95	374	54.65	128	64.10	153	76.00	2714
44.85	476	55.00	70	64.70	121	77.10	352
45.10	237	55.85	685	64.95	324	77.80	133
46.20	55	56.10	397	66.85	193	78.85	2691
46.80	616	56.90	2340	68.00	6681	79.80	662
47.95	526	57.95	176	69.05	6065	80.85	2901

Average of 12.823 to 12.835 min.: VN087614.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	684	103.60	98	127.85	257	171.40	114
82.90	109	103.85	252	129.70	113	171.90	297
85.60	55	104.95	136	129.95	176	172.10	131
86.90	1959	105.65	343	130.90	79	172.85	548
87.90	1858	106.10	71	134.80	197	173.90	34952
90.90	194	112.70	85	136.75	152	174.95	2829
91.95	1755	114.90	88	140.85	705	175.90	34291
93.00	2573	115.80	249	142.85	649	176.95	2426
93.95	6967	116.85	391	148.10	51	281.10	79
95.00	50640	117.70	342	154.70	64		
96.00	3712	118.95	421	170.20	52		

Instrument :

MSVOA_N

ClientSampleId :

BFB