
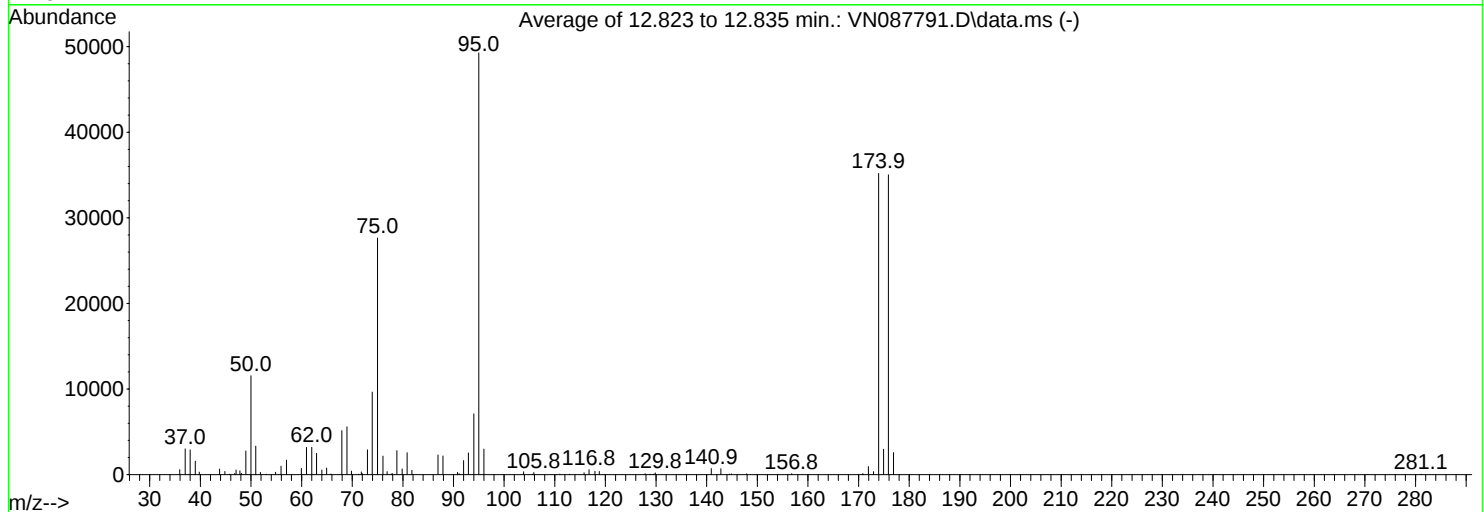


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091125\
Data File : VN087791.D
Acq On : 11 Sep 2025 09:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

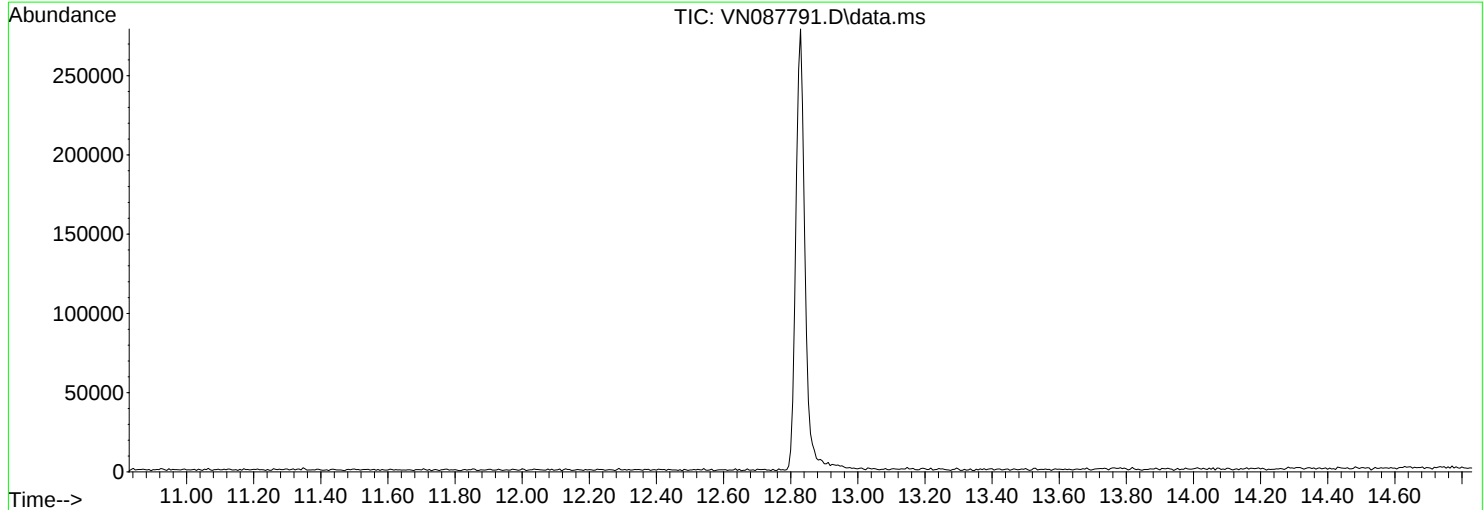

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	11550	PASS
75	95	30	60	56.1	27645	PASS
95	95	100	100	100.0	49280	PASS
96	95	5	9	6.1	2984	PASS
173	174	0.00	2	1.0	352	PASS
174	95	50	100	71.4	35203	PASS
175	174	5	9	8.4	2970	PASS
176	174	95	101	99.5	35032	PASS
177	176	5	9	7.4	2589	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	587	48.10	150	62.00	3203	73.00	289
37.00	3017	49.00	2770	62.95	2489	73.95	964
38.00	2907	50.00	11550	64.00	551	75.00	2764
39.00	1570	50.95	3320	64.95	772	76.05	217
39.80	307	51.85	264	65.80	79	76.90	357
43.80	661	53.00	65	67.95	5134	77.70	74
44.85	382	54.85	287	68.95	5590	77.90	129
45.80	61	55.95	997	69.85	408	78.80	2806
46.80	137	57.00	1694	71.30	60	79.85	681
47.05	543	59.95	722	71.80	323	80.85	2565
47.80	449	60.95	3173	72.00	117	81.80	498

Average of 12.823 to 12.835 min.: VN087791.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	2296	105.85	247	140.90	705	174.95	2970
87.90	2183	111.00	53	142.80	695	175.90	35032
90.80	267	112.90	60	144.50	59	176.90	2589
91.10	107	115.80	229	144.90	88	281.10	51
92.00	1650	116.75	587	147.90	91		
92.95	2543	117.95	384	156.80	120		
94.00	7098	118.80	376	170.80	113		
95.00	49280	127.85	122	171.00	52		
96.00	2984	128.80	56	171.95	940		
103.85	347	129.60	85	172.95	352		
105.60	53	129.85	215	173.95	35203		

Instrument :

MSVOA_N

ClientSampleId :

BFB