

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
 Data File : BG064395.D
 Acq On : 16 Sep 2025 22:12
 Operator : RC/JU
 Sample : PB169710BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK710

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG064395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.224	21	23	26	rBV2	1301	1022	0.13%	0.014%
2	3.312	35	38	43	rBV3	5402	7394	0.96%	0.101%
3	3.717	103	107	116	rBV	72187	124660	16.20%	1.702%
4	4.052	161	164	168	rBV3	1789	2191	0.28%	0.030%
5	4.316	207	209	214	rVB3	940	1212	0.16%	0.017%
6	4.463	230	234	237	rVB2	1063	1532	0.20%	0.021%
7	4.504	237	241	242	rBV2	916	1167	0.15%	0.016%
8	4.575	248	253	254	rBV2	745	1166	0.15%	0.016%
9	4.857	298	301	304	rBV2	668	1000	0.13%	0.014%
10	5.333	377	382	385	rBV	972	1301	0.17%	0.018%
11	5.862	470	472	476	rBV2	782	1011	0.13%	0.014%
12	7.013	661	668	676	rBV	98314	170610	22.18%	2.330%
13	7.096	680	682	685	rBV	876	1083	0.14%	0.015%
14	7.178	689	696	704	rBV	57038	96408	12.53%	1.317%
15	7.378	722	730	737	rBV	95595	166973	21.70%	2.280%
16	7.842	802	809	817	rVB	87589	148499	19.30%	2.028%
17	8.547	922	929	938	rBV	124285	211815	27.53%	2.893%
18	8.647	943	946	949	rVB	676	992	0.13%	0.014%
19	8.993	998	1005	1013	rBV	93015	160233	20.83%	2.188%
20	9.716	1121	1128	1135	rBV2	85076	153098	19.90%	2.091%
21	10.039	1178	1183	1184	rBV	973	1139	0.15%	0.016%
22	10.251	1213	1219	1227	rBV2	120937	213788	27.79%	2.919%
23	10.633	1276	1284	1290	rBV	111797	198198	25.76%	2.707%
24	10.762	1298	1306	1318	rBV	107694	196628	25.56%	2.685%
25	11.937	1500	1506	1509	rVB	545	979	0.13%	0.013%
26	12.225	1551	1555	1559	rBV	1737	2642	0.34%	0.036%
27	13.088	1699	1702	1707	rVB	737	967	0.13%	0.013%
28	13.876	1828	1836	1843	rBV	242739	347752	45.20%	4.749%
29	14.158	1877	1884	1891	rBV	233282	364352	47.36%	4.976%
30	14.463	1930	1936	1944	rVB	176297	281449	36.58%	3.843%
31	14.663	1964	1970	1979	rBV2	92390	163424	21.24%	2.232%
32	14.816	1994	1996	2000	rBV3	962	1034	0.13%	0.014%
33	14.957	2018	2020	2022	rBV	1007	1050	0.14%	0.014%
34	15.456	2099	2105	2112	rBV	309964	468365	60.88%	6.396%
35	15.574	2120	2125	2136	rBV2	116639	179559	23.34%	2.452%
36	15.662	2138	2140	2142	rVB	1451	1493	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
 Data File : BG064395.D
 Acq On : 16 Sep 2025 22:12
 Operator : RC/JU
 Sample : PB169710BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK710

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
 Title : SVOA CALIBRATION

37	15.697	2144	2146	2150	rVB3	1497	1332	0.17%	0.018%
38	16.714	2314	2319	2322	rBV	694	985	0.13%	0.013%
39	17.207	2396	2403	2410	rBV2	259282	389785	50.66%	5.323%
40	17.307	2413	2420	2433	rVB	378059	565853	73.55%	7.727%
41	17.566	2462	2464	2471	rBV	1150	1465	0.19%	0.020%
42	18.376	2598	2602	2605	rBV	819	1031	0.13%	0.014%
43	19.070	2719	2720	2723	rBV	1198	1094	0.14%	0.015%
44	19.158	2730	2735	2741	rVB3	5281	7181	0.93%	0.098%
45	19.228	2743	2747	2752	rVB2	4960	6270	0.81%	0.086%
46	19.410	2777	2778	2784	rBV	1646	1358	0.18%	0.019%
47	19.469	2786	2788	2793	rVB	1270	1616	0.21%	0.022%
48	19.534	2797	2799	2802	rVB	2506	1871	0.24%	0.026%
49	19.593	2802	2809	2815	rBV	506051	715595	93.01%	9.772%
50	19.798	2842	2844	2846	rVB2	1534	1002	0.13%	0.014%
51	19.822	2846	2848	2849	rBV2	1921	1286	0.17%	0.018%
52	19.928	2863	2866	2868	rBV2	1991	1772	0.23%	0.024%
53	20.251	2919	2921	2923	rBV	1419	1312	0.17%	0.018%
54	20.304	2928	2930	2931	rBV	1353	1055	0.14%	0.014%
55	20.351	2936	2938	2939	rBV2	1724	1018	0.13%	0.014%
56	20.409	2947	2948	2951	rBV2	1976	1375	0.18%	0.019%
57	20.503	2958	2964	2965	rBV4	2343	3169	0.41%	0.043%
58	20.556	2971	2973	2975	rBV3	1600	1461	0.19%	0.020%
59	20.609	2979	2982	2983	rBV3	1637	1750	0.23%	0.024%
60	20.627	2983	2985	2988	rBV3	1500	1323	0.17%	0.018%
61	20.826	3017	3019	3020	rBV2	2044	1362	0.18%	0.019%
62	20.844	3020	3022	3023	rVV2	1773	1117	0.15%	0.015%
63	21.073	3059	3061	3064	rVB3	2889	2287	0.30%	0.031%
64	21.432	3116	3122	3133	rBV2	326225	540127	70.20%	7.376%
65	21.902	3200	3202	3205	rBV3	2584	2405	0.31%	0.033%
66	22.389	3284	3285	3286	rBV	2980	1697	0.22%	0.023%
67	22.489	3300	3302	3305	rBV4	2921	3100	0.40%	0.042%
68	22.848	3359	3363	3369	rVB6	6520	10403	1.35%	0.142%
69	23.506	3473	3475	3477	rBV3	3546	2061	0.27%	0.028%
70	23.588	3485	3489	3495	rBV7	7294	14901	1.94%	0.203%
71	23.899	3540	3542	3545	rBV4	2661	2144	0.28%	0.029%
72	24.228	3588	3598	3611	rVB	308770	769358	100.00%	10.506%
73	24.434	3623	3633	3646	rBV2	208324	566778	73.67%	7.740%
74	26.020	3901	3903	3906	rBV4	2640	2521	0.33%	0.034%
75	26.602	4000	4002	4003	rBV2	2664	1573	0.20%	0.021%
76	26.637	4006	4008	4009	rBV2	3555	2384	0.31%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064395.D
Acq On : 16 Sep 2025 22:12
Operator : RC/JU
Sample : PB169710BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK710

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Title : SVOA CALIBRATION

77	26.849	4042	4044	4046	rBV3	2950	2689	0.35%	0.037%
78	30.257	4622	4624	4626	rBV3	3507	2923	0.38%	0.040%
79	31.584	4848	4850	4852	rBV2	3362	3459	0.45%	0.047%
80	32.260	4963	4965	4966	rVB2	3207	1386	0.18%	0.019%


Sum of corrected areas: 7322820

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064395.D
Acq On : 16 Sep 2025 22:12
Operator : RC/JU
Sample : PB169710BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK710

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

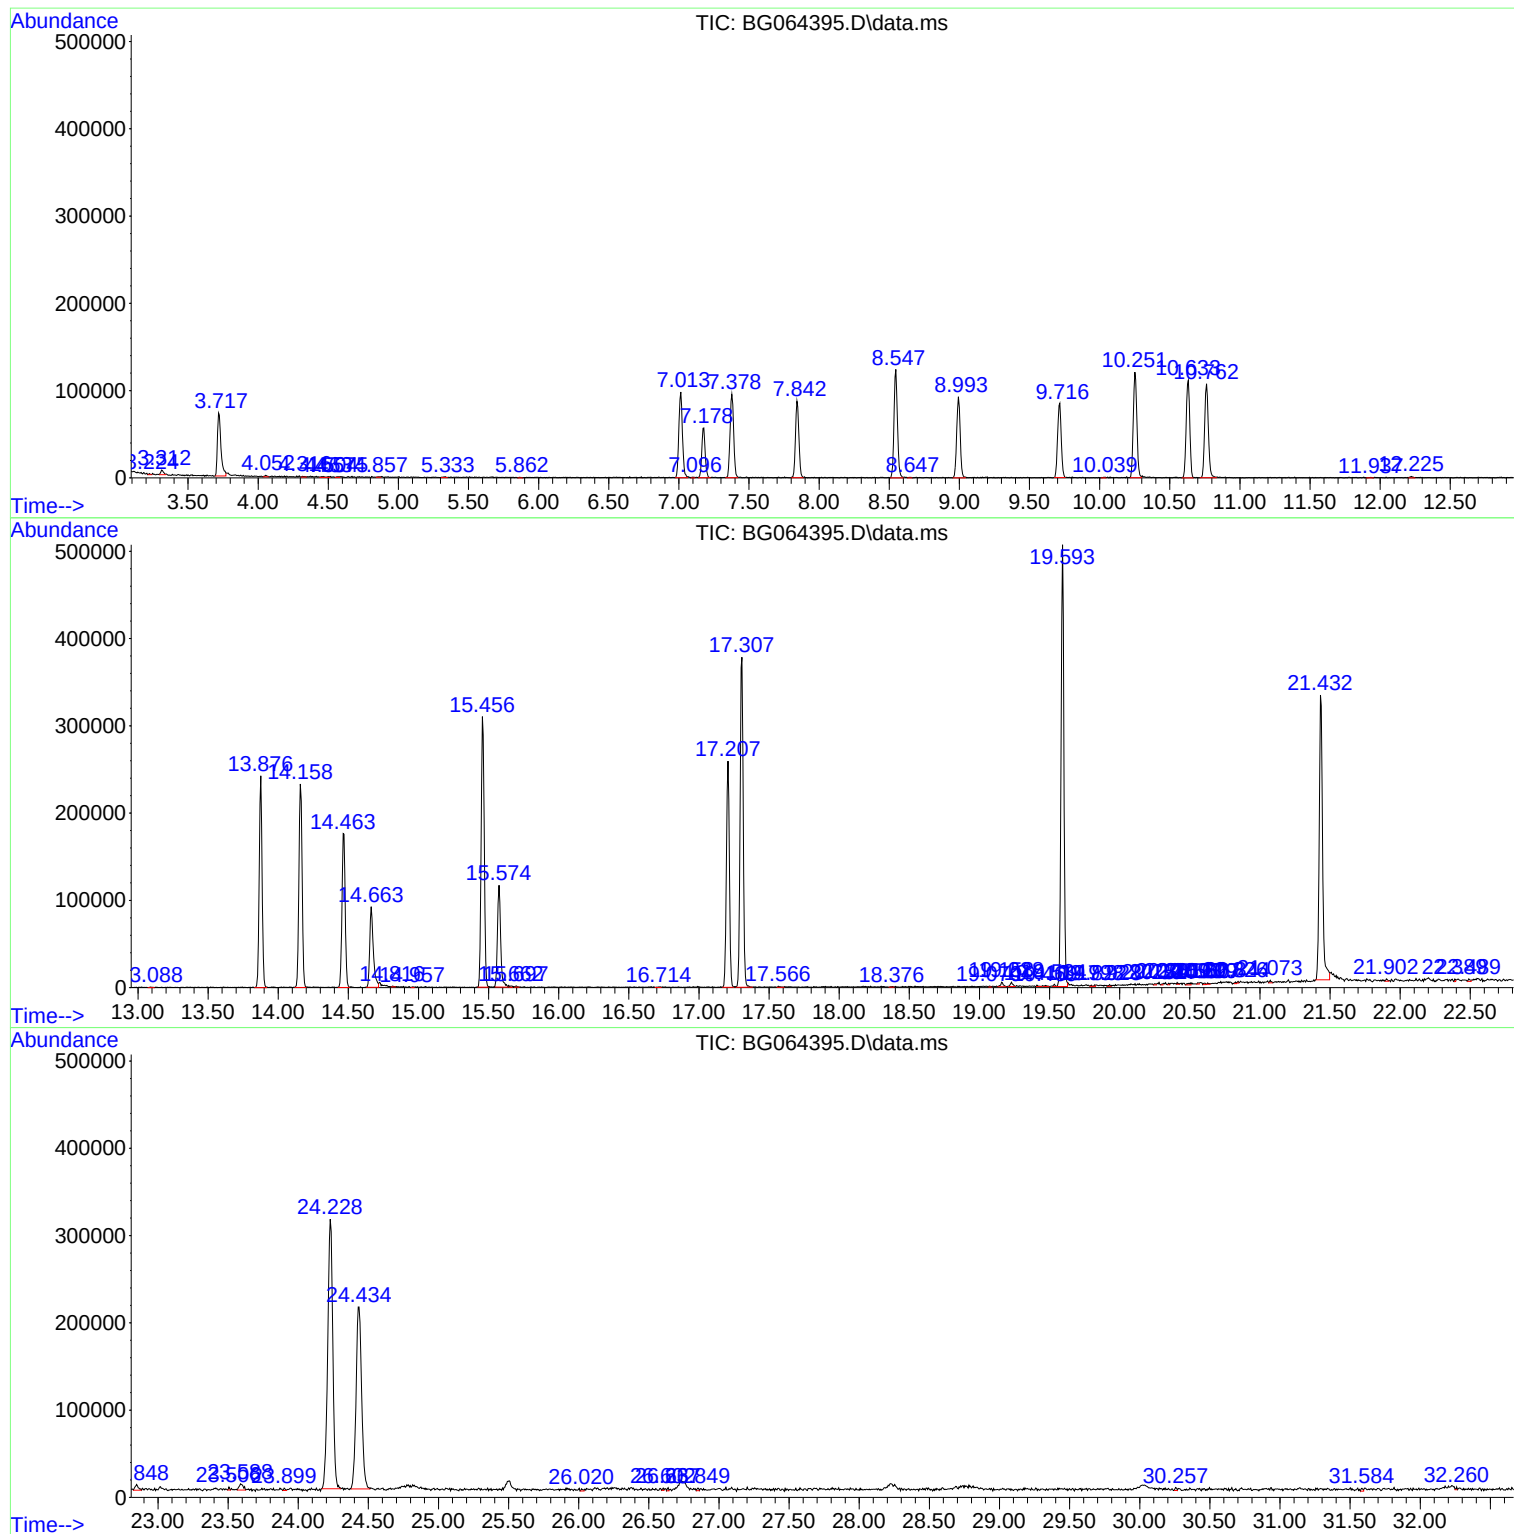

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064395.D
Acq On : 16 Sep 2025 22:12
Operator : RC/JU
Sample : PB169710BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK710

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064395.D
Acq On : 16 Sep 2025 22:12
Operator : RC/JU
Sample : PB169710BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK710

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc