

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
 Data File : BG064396.D
 Acq On : 16 Sep 2025 22:53
 Operator : RC/JU
 Sample : PB169711BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK711

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG064396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.314	34	38	44	rVB3	5294	7897	0.89%	0.097%
2	3.720	102	107	120	rBV	86756	144469	16.36%	1.783%
3	4.019	156	158	160	rBV2	1047	1207	0.14%	0.015%
4	4.055	161	164	168	rVB4	1833	2336	0.26%	0.029%
5	4.160	180	182	186	rVB2	1153	1321	0.15%	0.016%
6	4.777	284	287	290	rBV2	810	1177	0.13%	0.015%
7	7.010	659	667	675	rBV	115997	201125	22.77%	2.483%
8	7.174	689	695	706	rVB2	64930	110550	12.52%	1.365%
9	7.380	721	730	739	rVB	109611	189793	21.49%	2.343%
10	7.844	803	809	817	rVB	82909	140303	15.89%	1.732%
11	8.543	922	928	937	rBV	143614	242716	27.48%	2.996%
12	8.996	998	1005	1013	rBV	105876	184149	20.85%	2.273%
13	9.713	1119	1127	1135	rBB2	98909	178717	20.24%	2.206%
14	10.253	1211	1219	1230	rBV	144979	254711	28.84%	3.144%
15	10.629	1276	1283	1290	rBV	110235	193610	21.92%	2.390%
16	10.764	1298	1306	1315	rBV	126139	234180	26.52%	2.891%
17	12.216	1548	1553	1555	rBV2	1510	2342	0.27%	0.029%
18	13.878	1829	1836	1843	rBV	284318	413092	46.78%	5.099%
19	14.160	1876	1884	1892	rBV	274734	427360	48.39%	5.275%
20	14.466	1929	1936	1942	rBV	184005	279521	31.65%	3.450%
21	14.666	1963	1970	1985	rBV2	108810	202166	22.89%	2.495%
22	15.459	2098	2105	2116	rVB2	368769	550795	62.37%	6.799%
23	15.576	2118	2125	2135	rBV	131425	207170	23.46%	2.557%
24	15.688	2143	2144	2152	rVB2	1780	3150	0.36%	0.039%
25	17.204	2396	2402	2410	rBV	259720	385165	43.61%	4.754%
26	17.304	2413	2419	2427	rVV	460990	666341	75.45%	8.225%
27	17.880	2514	2517	2520	rBV2	1324	1332	0.15%	0.016%
28	18.250	2578	2580	2586	rVB2	985	1544	0.17%	0.019%
29	19.149	2731	2733	2734	rBV2	3977	3009	0.34%	0.037%
30	19.166	2734	2736	2740	rVB4	6373	5508	0.62%	0.068%
31	19.231	2742	2747	2751	rVB	4838	7030	0.80%	0.087%
32	19.595	2802	2809	2815	rBV	579647	816106	92.41%	10.073%
33	19.766	2833	2838	2840	rBV3	1294	2218	0.25%	0.027%
34	19.813	2844	2846	2849	rBV2	1472	1707	0.19%	0.021%
35	19.895	2859	2860	2863	rBV2	1691	1144	0.13%	0.014%
36	19.948	2866	2869	2871	rBV	1323	1664	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
 Data File : BG064396.D
 Acq On : 16 Sep 2025 22:53
 Operator : RC/JU
 Sample : PB169711BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK711

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
 Title : SVOA CALIBRATION

37	20.059	2886	2888	2889	rBV	1775	1461	0.17%	0.018%
38	20.206	2910	2913	2915	rBV2	1599	2003	0.23%	0.025%
39	20.418	2947	2949	2950	rBV2	1602	1395	0.16%	0.017%
40	20.512	2963	2965	2966	rBV	1750	1526	0.17%	0.019%
41	20.688	2993	2995	2997	rBV2	1634	1299	0.15%	0.016%
42	20.976	3043	3044	3046	rBV	2439	1463	0.17%	0.018%
43	21.434	3116	3122	3129	rBV	322990	481884	54.57%	5.948%
44	21.605	3149	3151	3154	rBV3	3352	4364	0.49%	0.054%
45	22.104	3234	3236	3237	rBV	2226	1401	0.16%	0.017%
46	22.844	3360	3362	3368	rVB5	7511	11096	1.26%	0.137%
47	22.997	3387	3388	3389	rBV	2647	1480	0.17%	0.018%
48	23.026	3389	3393	3399	rVB6	4735	7954	0.90%	0.098%
49	24.231	3588	3598	3608	rBV	341273	883122	100.00%	10.901%
50	24.437	3622	3633	3647	rBV	201416	543755	61.57%	6.712%
51	24.689	3674	3676	3678	rBV3	2757	2415	0.27%	0.030%
52	25.336	3784	3786	3787	rVB2	3471	1640	0.19%	0.020%
53	25.500	3810	3814	3823	rVB5	12328	29411	3.33%	0.363%
54	25.999	3898	3899	3900	rBV	3967	2015	0.23%	0.025%
55	26.105	3916	3917	3920	rBV3	2908	3314	0.38%	0.041%
56	26.276	3945	3946	3950	rVB3	4156	2783	0.32%	0.034%
57	26.352	3957	3959	3960	rBV2	2165	1275	0.14%	0.016%
58	26.734	4019	4024	4032	rVB2	9998	30007	3.40%	0.370%
59	27.733	4190	4194	4195	rBV3	3422	4531	0.51%	0.056%
60	27.991	4236	4238	4241	rBV4	4217	4623	0.52%	0.057%
61	28.673	4353	4354	4356	rBV2	2562	1779	0.20%	0.022%
62	29.801	4544	4546	4552	rBV4	2511	3895	0.44%	0.048%
63	31.487	4831	4833	4835	rBV3	2706	1633	0.18%	0.020%
64	32.298	4969	4971	4973	rVB3	3447	1445	0.16%	0.018%


Sum of corrected areas: 8101594

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064396.D
Acq On : 16 Sep 2025 22:53
Operator : RC/JU
Sample : PB169711BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK711

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

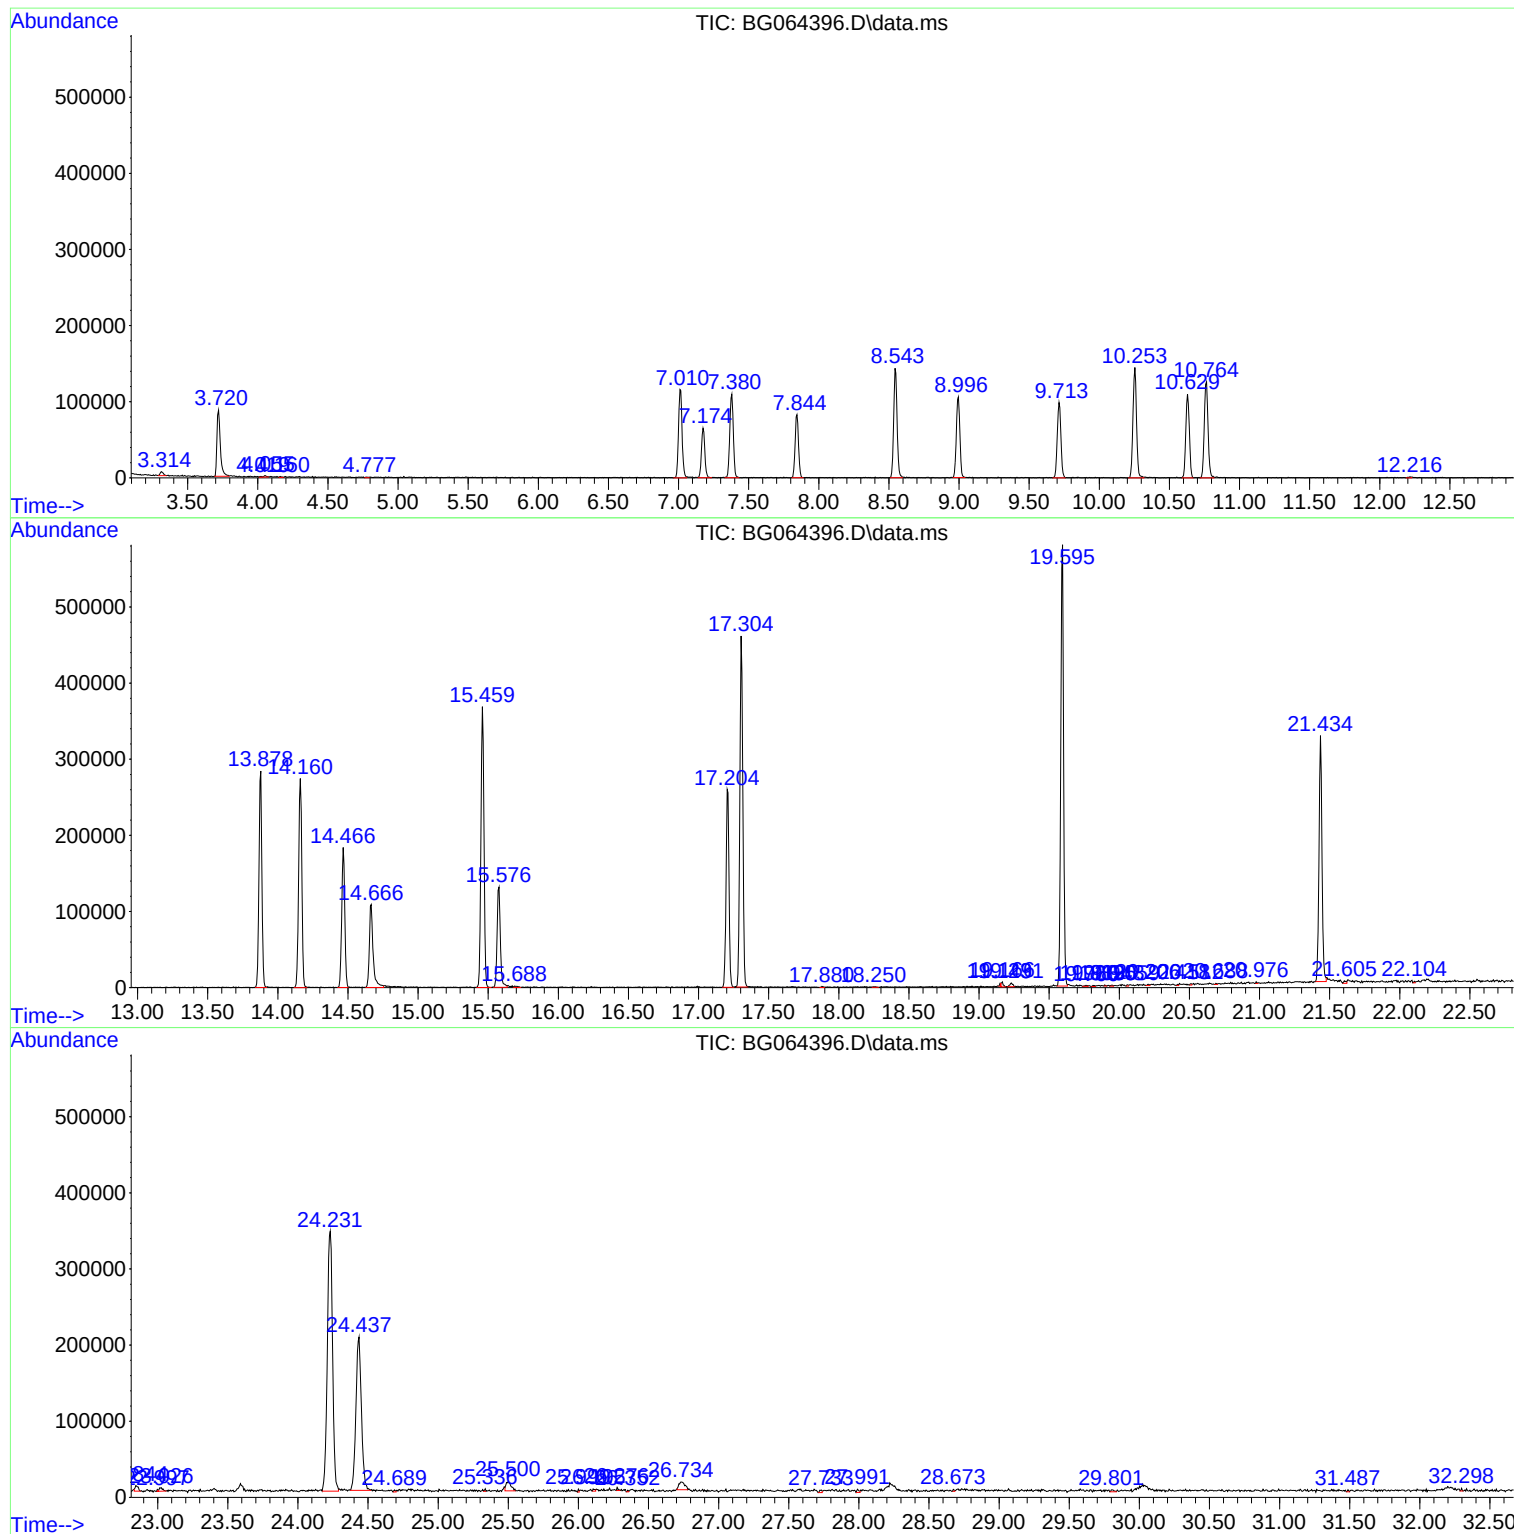

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064396.D
Acq On : 16 Sep 2025 22:53
Operator : RC/JU
Sample : PB169711BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK711

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064396.D
Acq On : 16 Sep 2025 22:53
Operator : RC/JU
Sample : PB169711BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK711

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc