
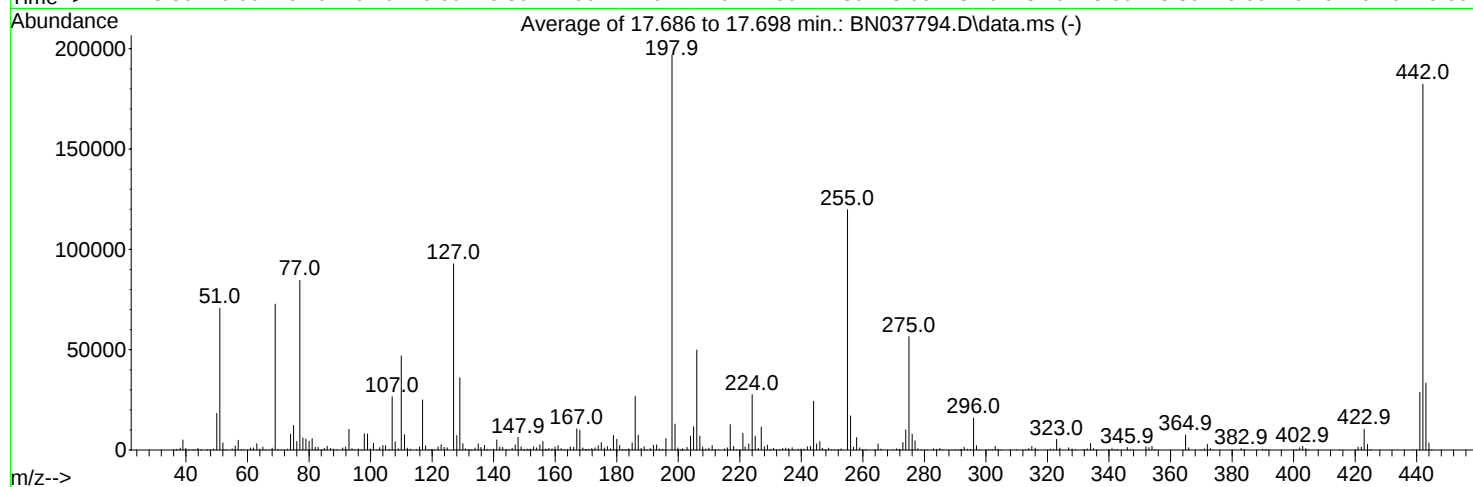


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091825\
Data File : BN037794.D
Acq On : 19 Sep 2025 02:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

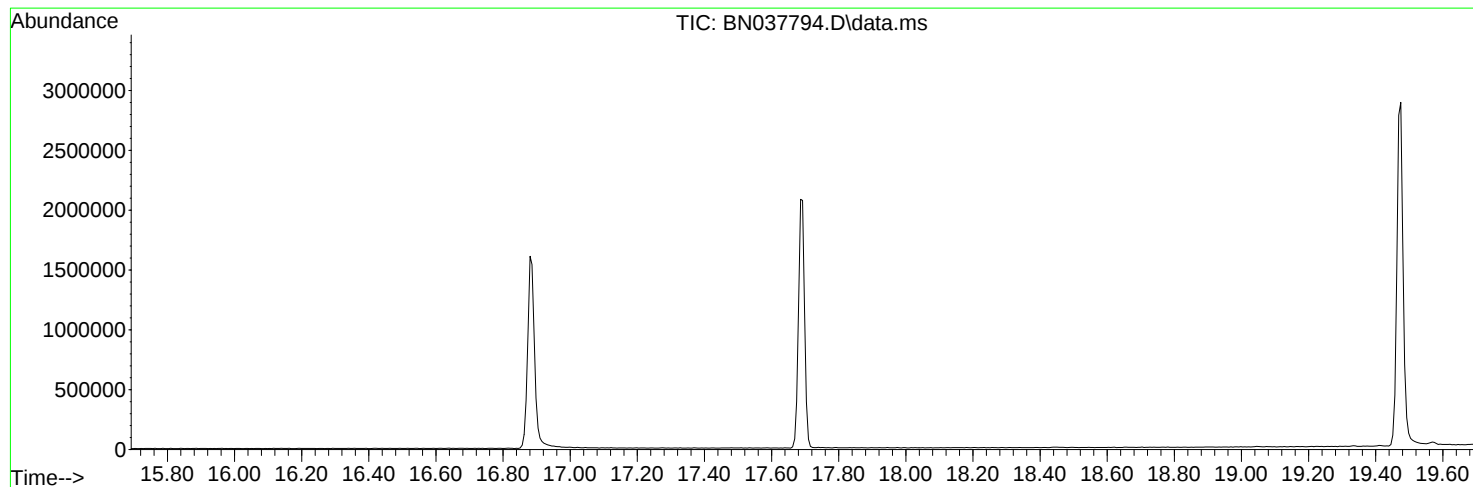




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.4	987	PASS
69	69	100	100	100.0	72725	PASS
70	69	0.00	2	0.6	414	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	196813	PASS
199	198	5	9	6.6	12909	PASS
365	198	1	100	3.8	7534	PASS
441	443	0.01	150	86.4	28805	PASS
442	442	100	100	100.0	182293	PASS
443	442	15	24	18.3	33347	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091825\
Data File : BN037794.D
Acq On : 19 Sep 2025 02:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 19 04:29:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 19 04:29:39 2025
Response via : Initial Calibration

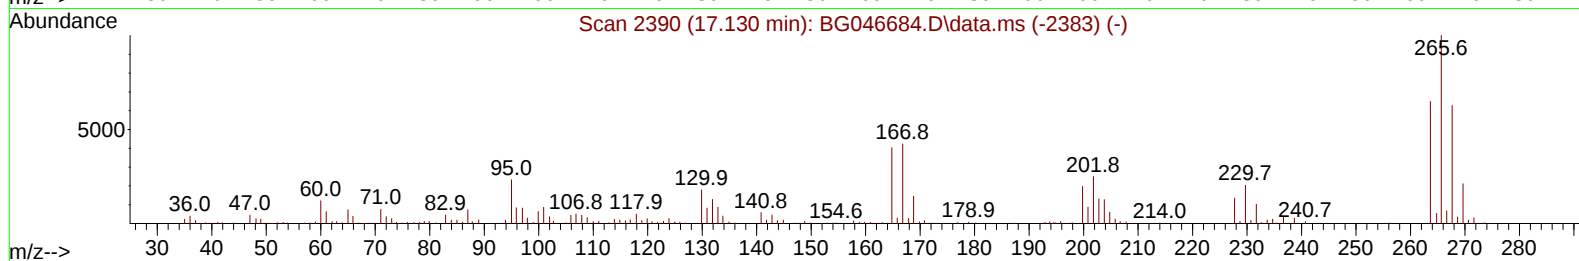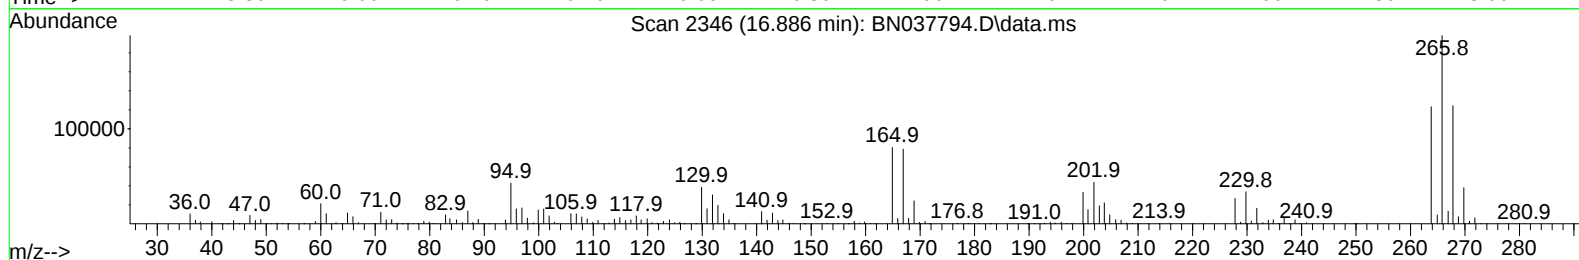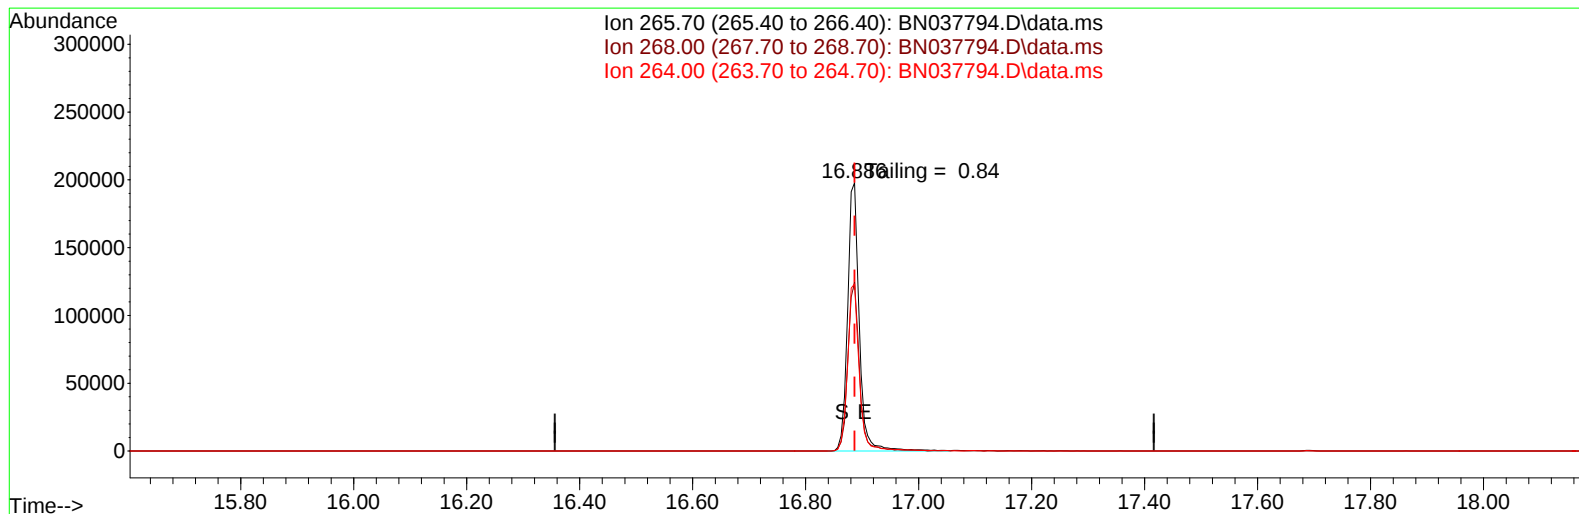

TIC: BN037794.D\data.ms

(70) Pentachlorophenol (C)

16.886min (0.000) 32518.88 ng




response 284548

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.85
264.00	61.60	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091825\
Data File : BN037794.D
Acq On : 19 Sep 2025 02:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 19 04:29:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 19 04:29:39 2025
Response via : Initial Calibration

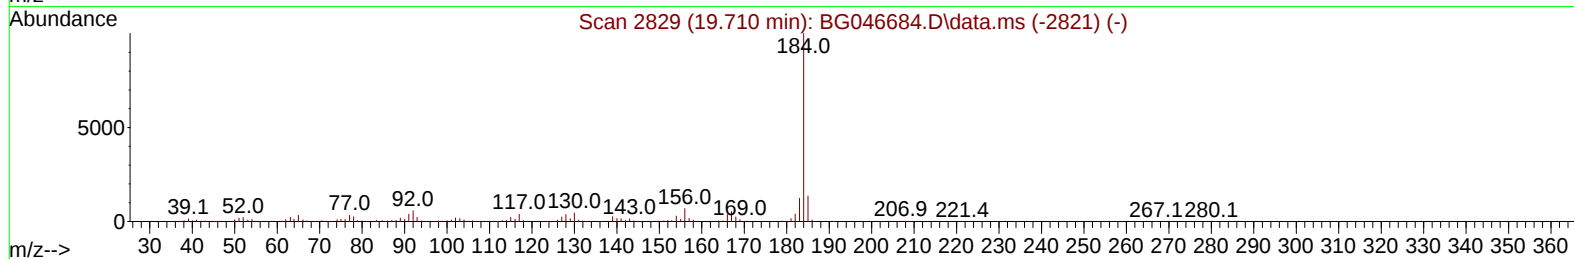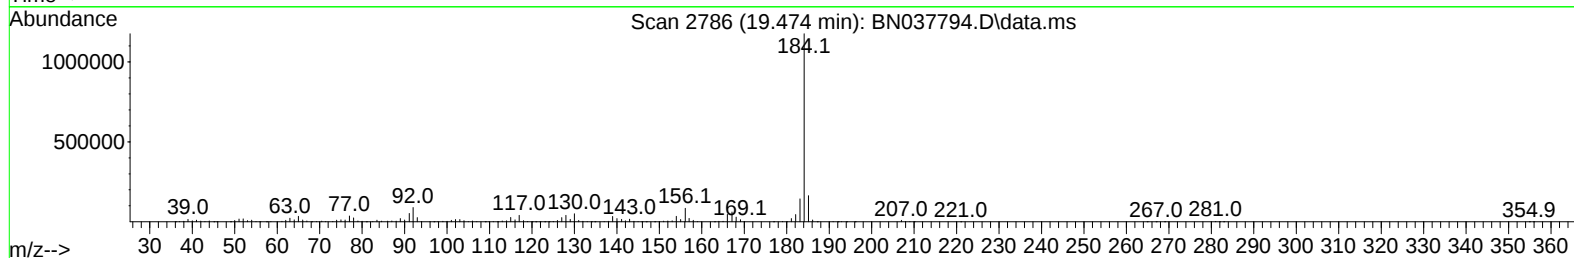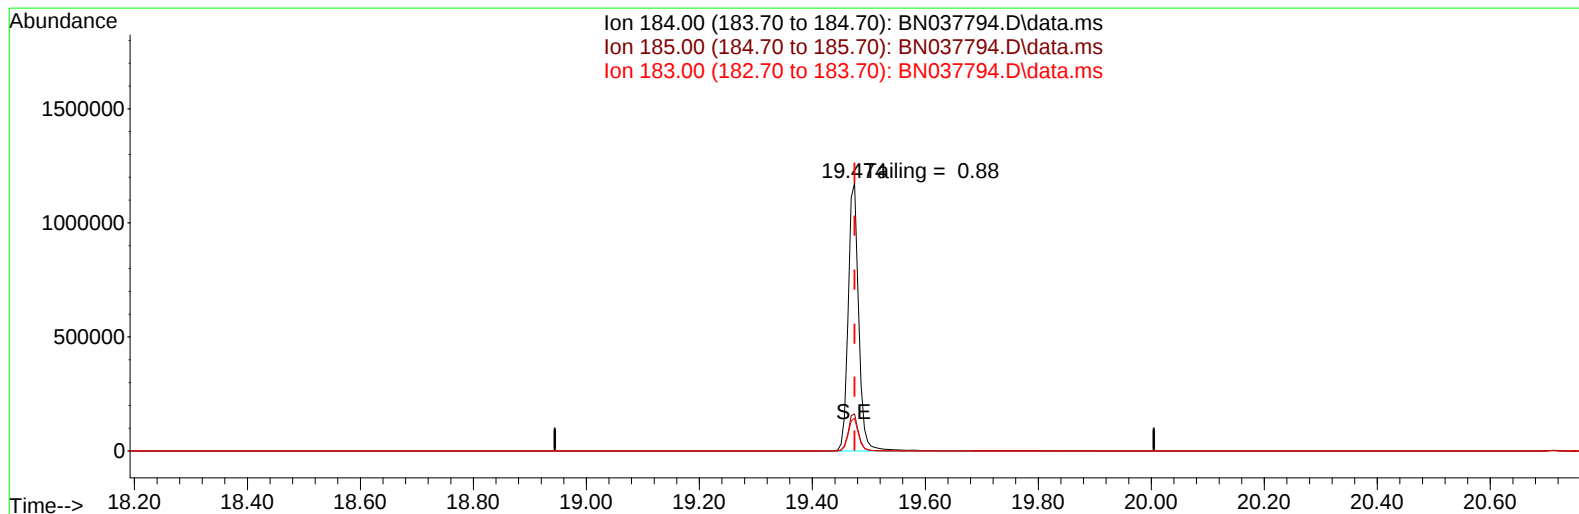

TIC: BN037794.D\data.ms

(77) Benzidine

19.474min (0.000) 0.00 ng

response 1527830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2025	BNA_N	<u>BN037794.D</u>
Compound Name	Response	Retention Time
DDT	688292	20.71
DDD	26538	20.269
DDE	1670	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28208	716500	3.94

Instrument :
BNA_N
ClientSampleId :
DFTPP