
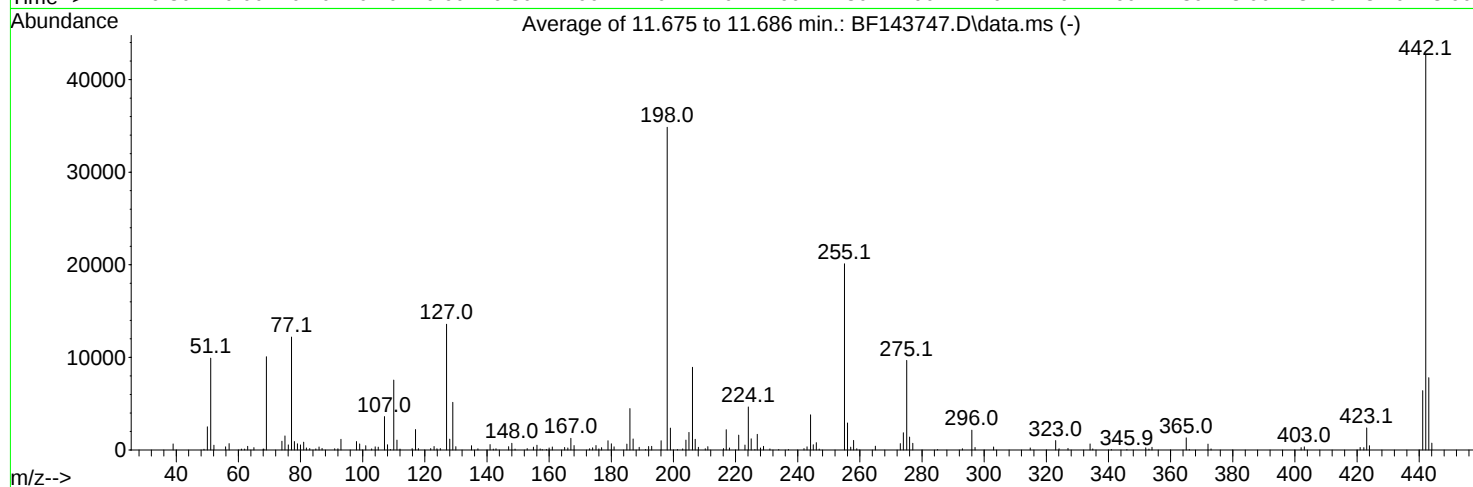


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091525\
Data File : BF143747.D
Acq On : 15 Sep 2025 12:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 09 15:20:16 2025

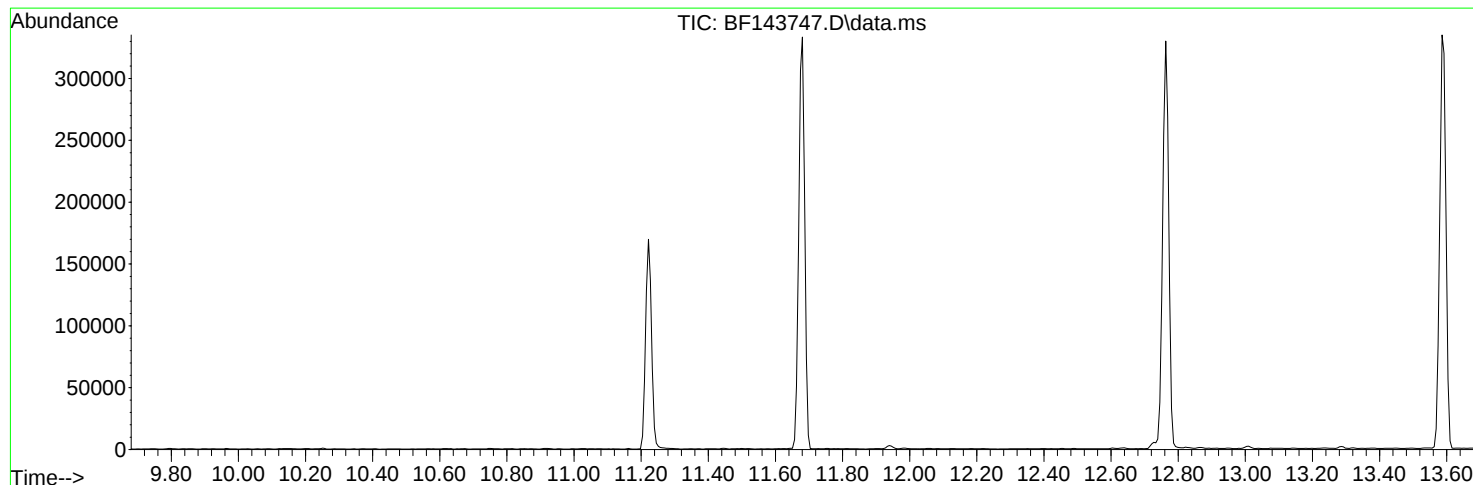

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.0	102	PASS
69	69	100	100	100.0	10068	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34851	PASS
199	198	5	9	6.8	2360	PASS
365	198	1	100	3.8	1309	PASS
441	443	0.01	150	82.1	6411	PASS
442	442	100	100	100.0	42632	PASS
443	442	15	24	18.3	7806	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
9/15/2025	BNA_F	<u>BF143747.D</u>
Compound Name	Response	Retention Time
DDT	88670	13.568
DDD	1050	13.286
DDE	201	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1251	89921	1.39

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091525\
Data File : BF143747.D
Acq On : 15 Sep 2025 12:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 12:51:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

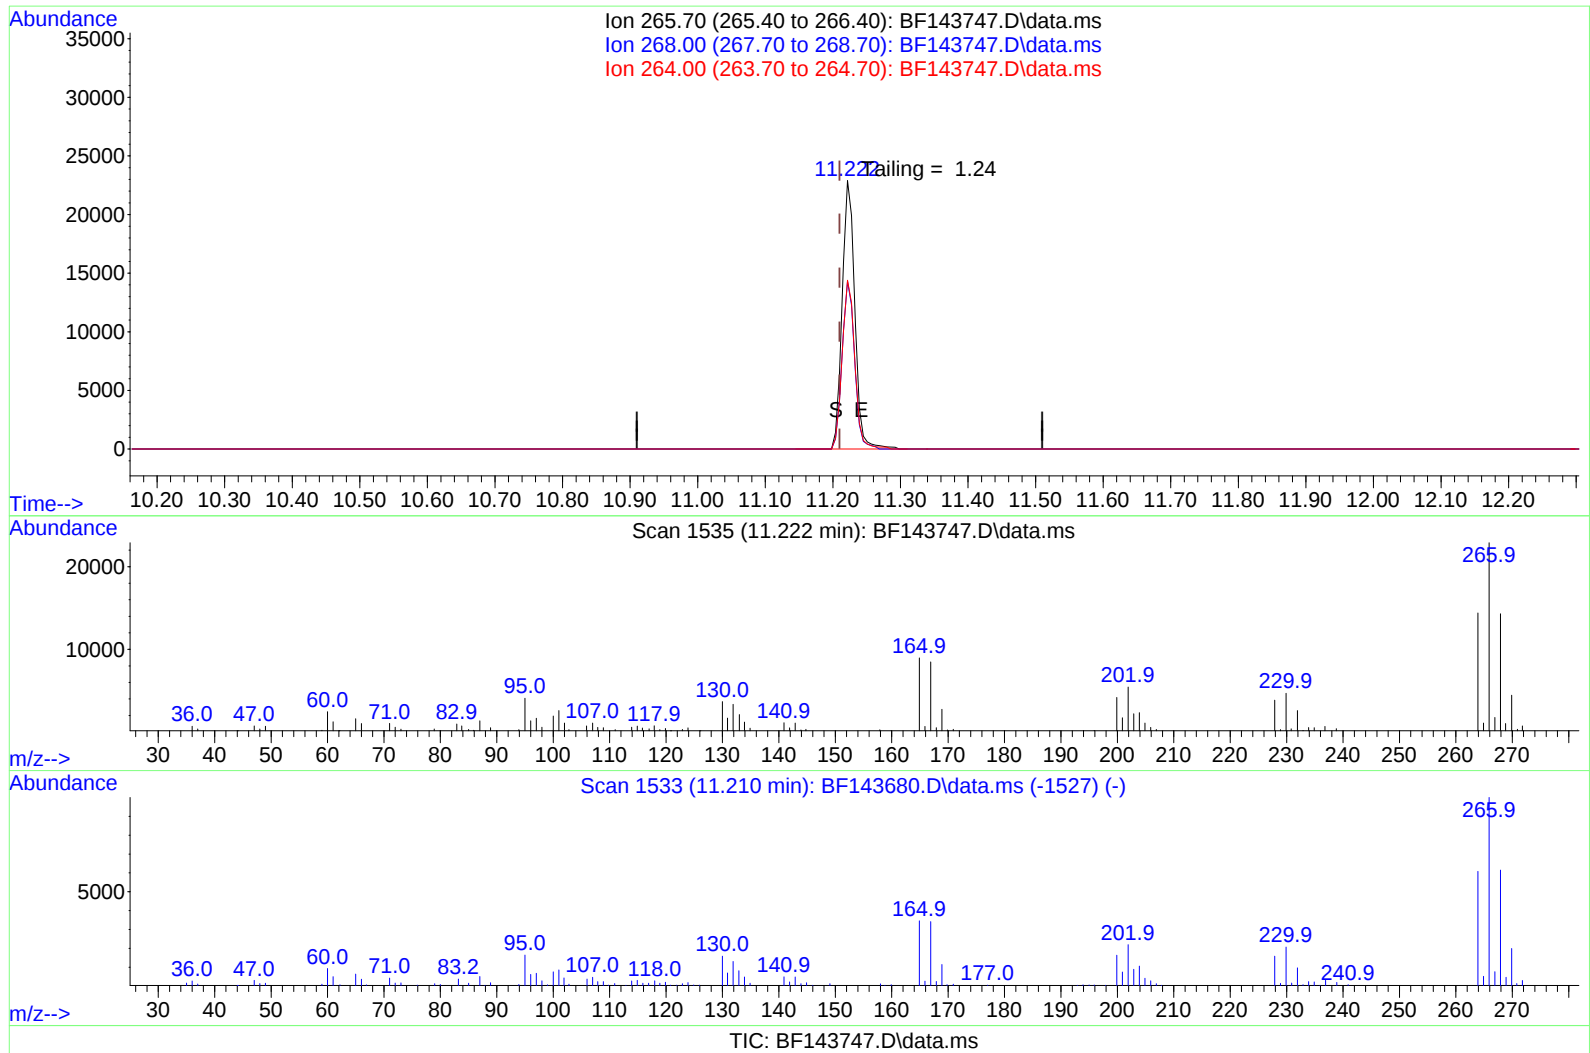

(70) Pentachlorophenol (C)

11.222min (+ 0.012) 0.00 ng


response 29705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.50
264.00	60.80	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091525\
Data File : BF143747.D
Acq On : 15 Sep 2025 12:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 12:51:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

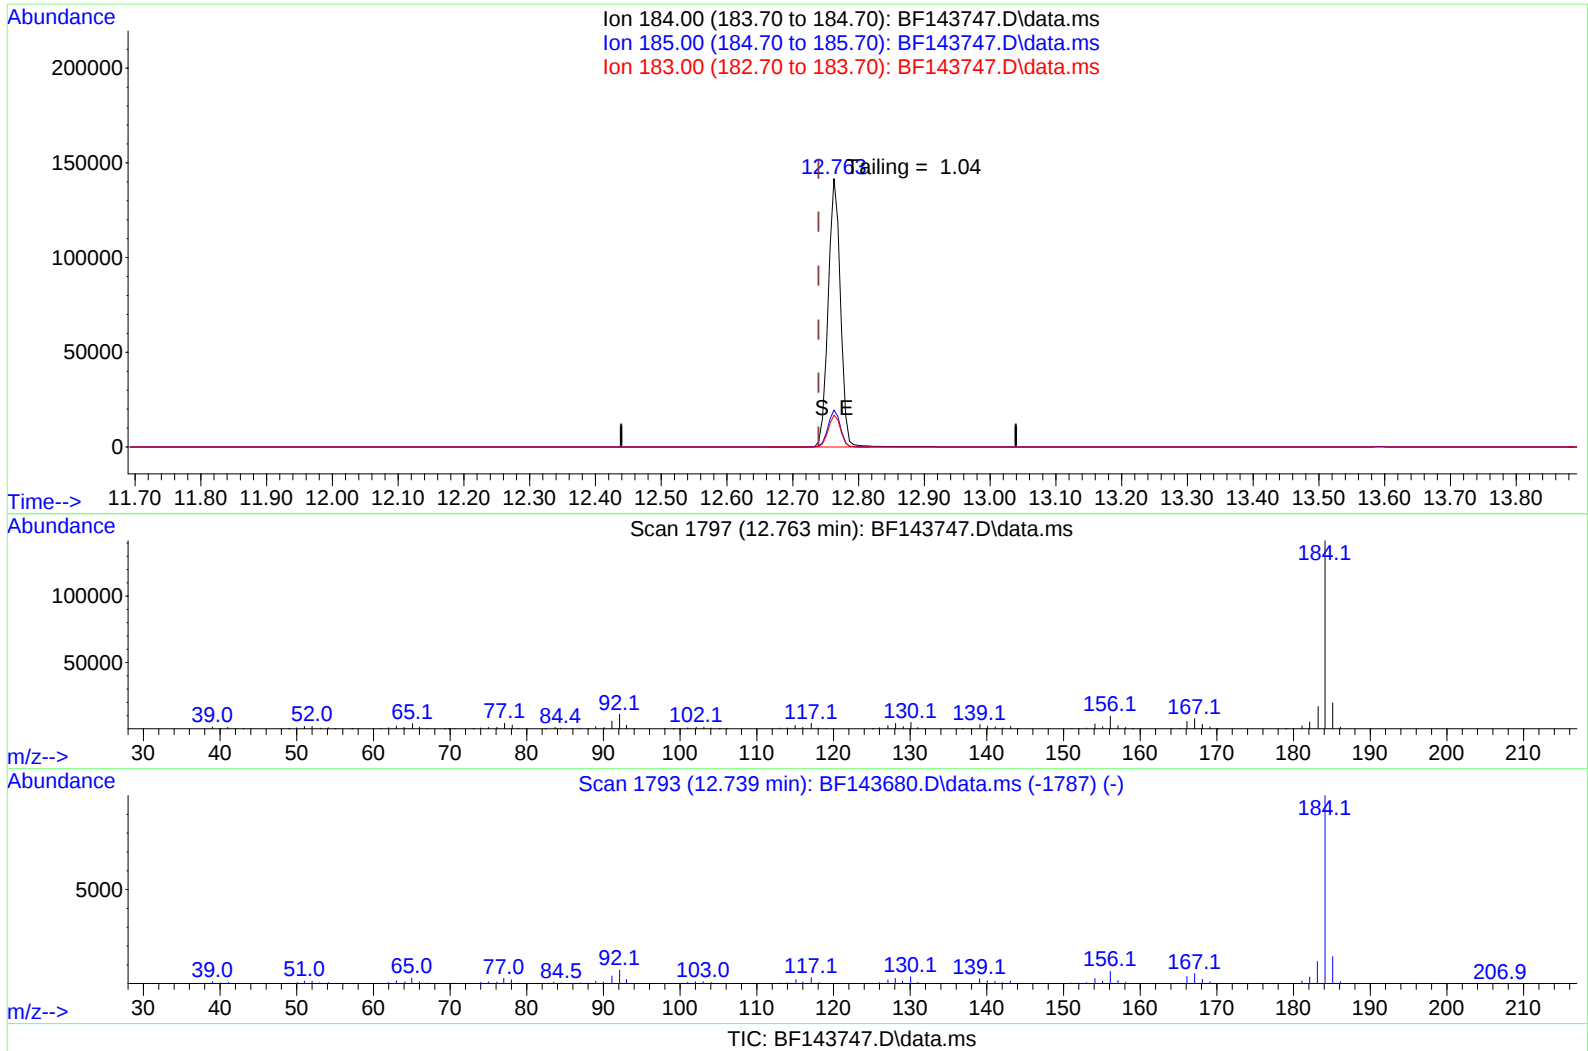

(77) Benzidine

12.763min (+ 0.023) 0.00 ng

response 184434

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.79
183.00	11.80	11.91
0.00	0.00	0.00