
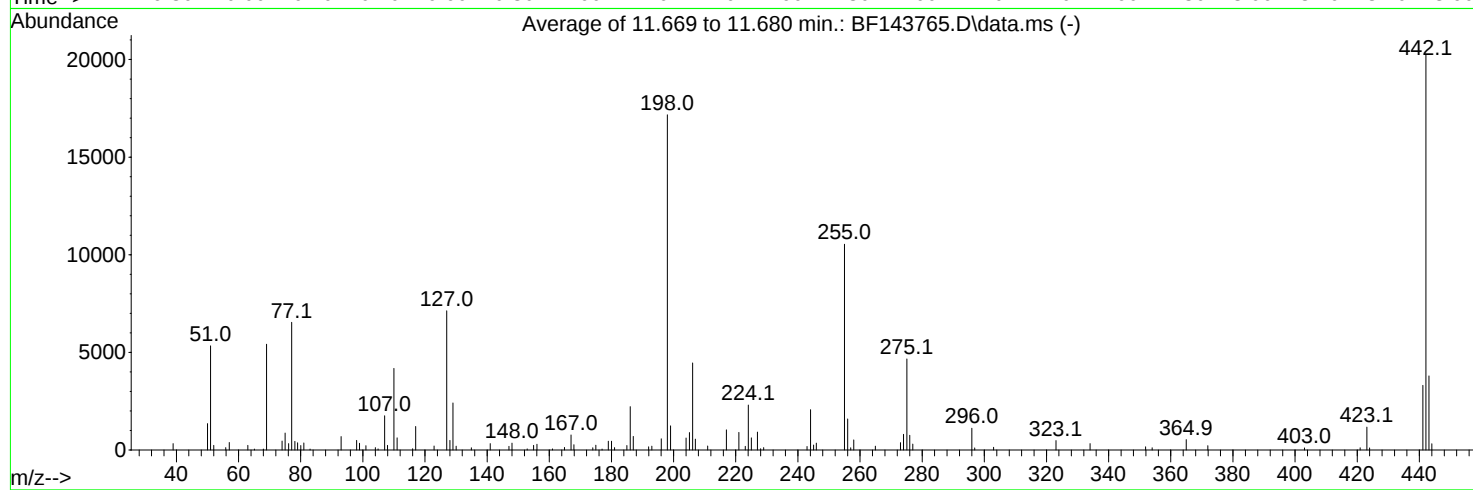


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143765.D
Acq On : 16 Sep 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 17 01:44:23 2025

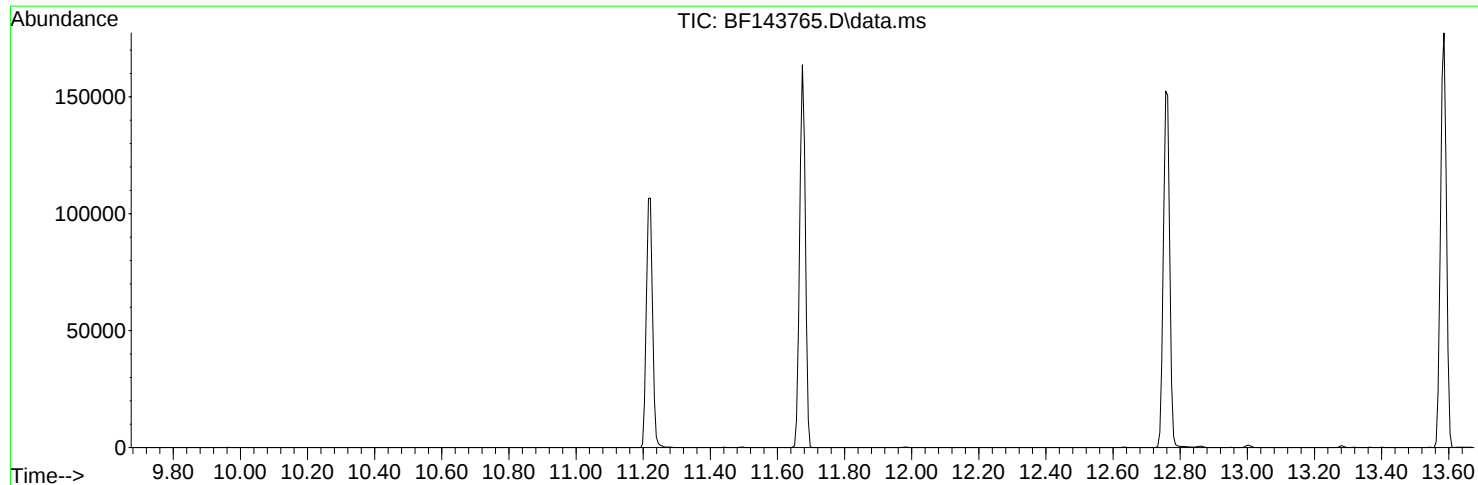

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	50	PASS
69	69	100	100	100.0	5419	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17166	PASS
199	198	5	9	7.2	1241	PASS
365	198	1	100	3.1	536	PASS
441	443	0.01	150	87.4	3313	PASS
442	442	100	100	100.0	20222	PASS
443	442	15	24	18.8	3792	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/16/2025	BNA_F	<u>BF143765.D</u>
Compound Name	Response	Retention Time
DDT	49271	13.586
DDD	524	13.28
DDE	54	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
578	49849	1.16

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143765.D
Acq On : 16 Sep 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 13:41:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

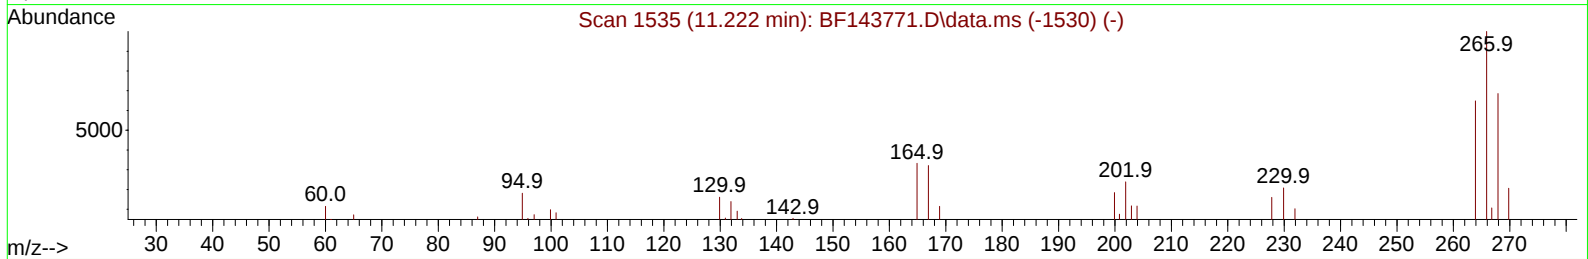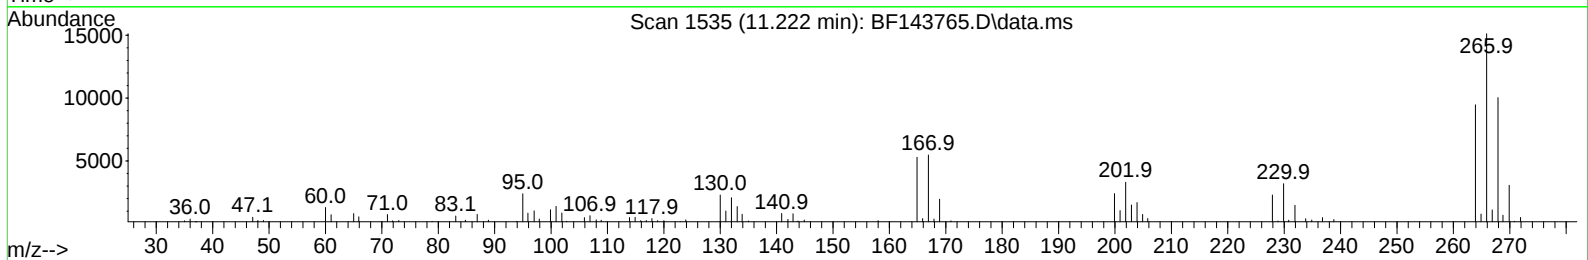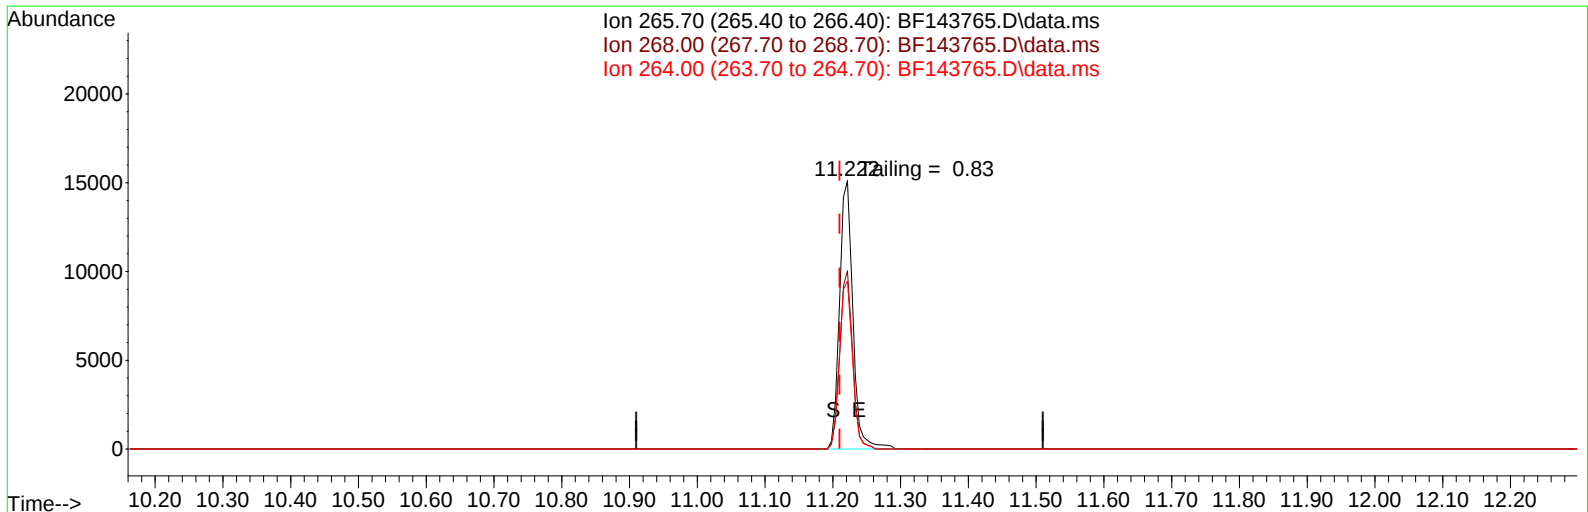

TIC: BF143765.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.012) 0.00 ng




response 20593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	66.43
264.00	60.80	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143765.D
Acq On : 16 Sep 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 13:41:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

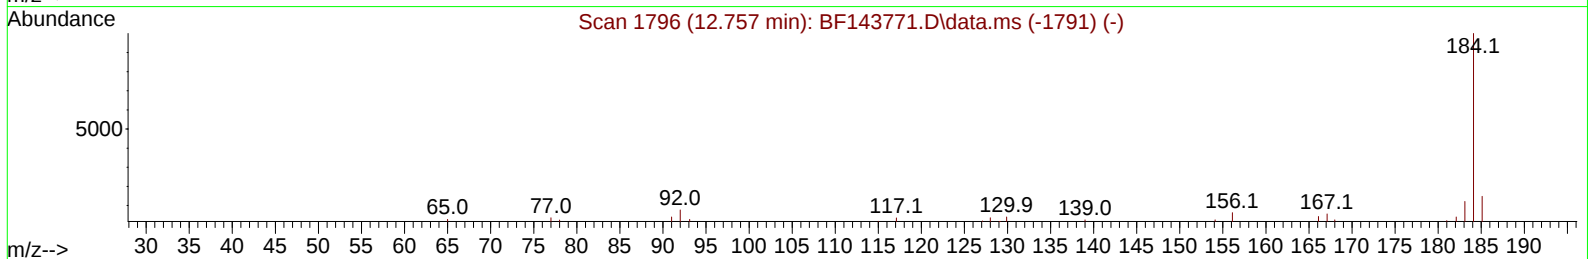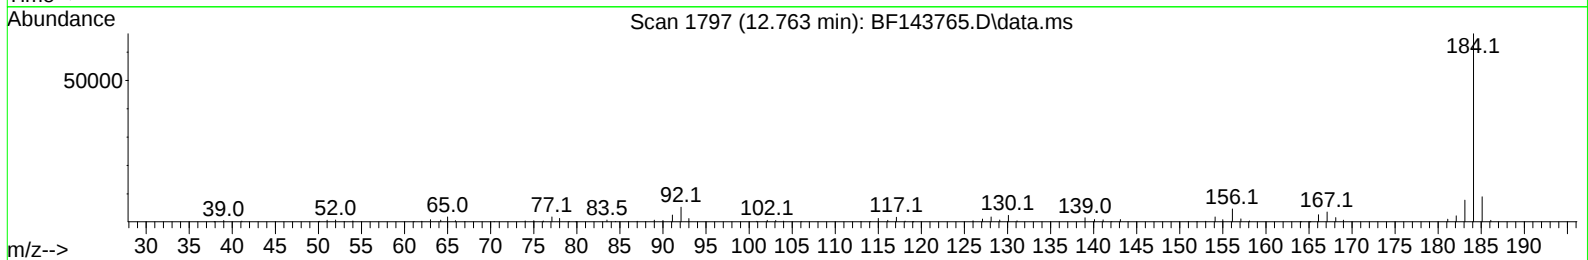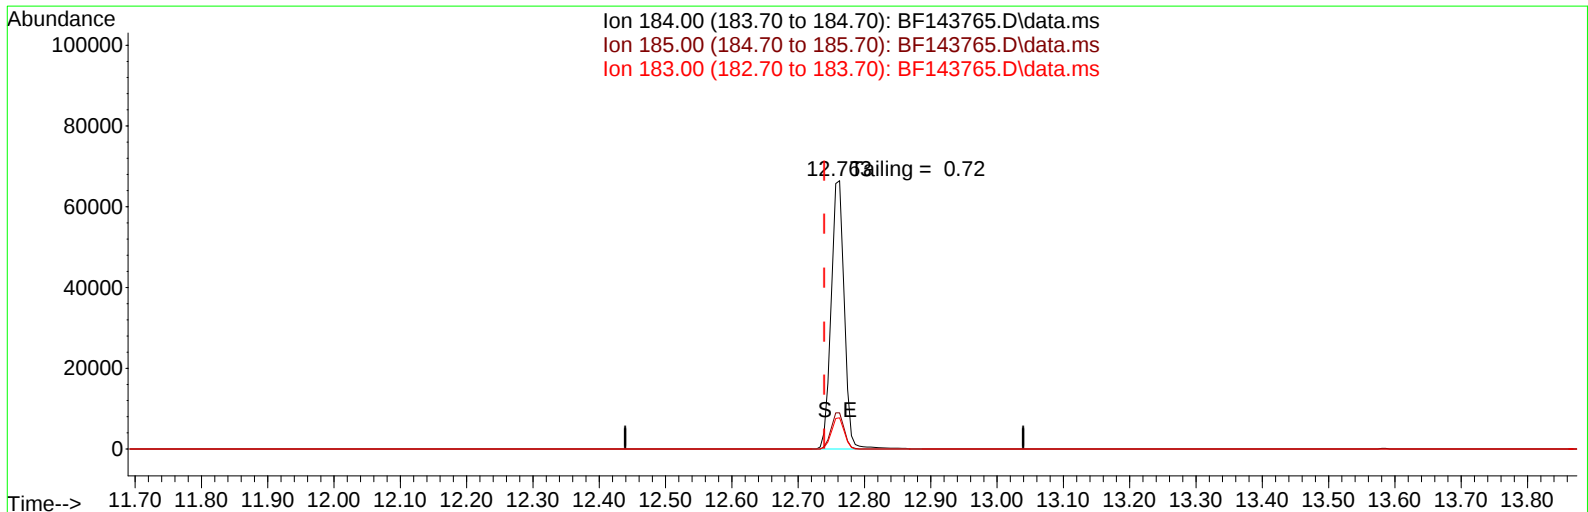

TIC: BF143765.D\data.ms

(77) Benzidine

12.763min (+ 0.023) 0.00 ng

response 91478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.48
183.00	11.80	11.66
0.00	0.00	0.00