


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091625\
Data File : BP025755.D
Acq On : 16 Sep 2025 12:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

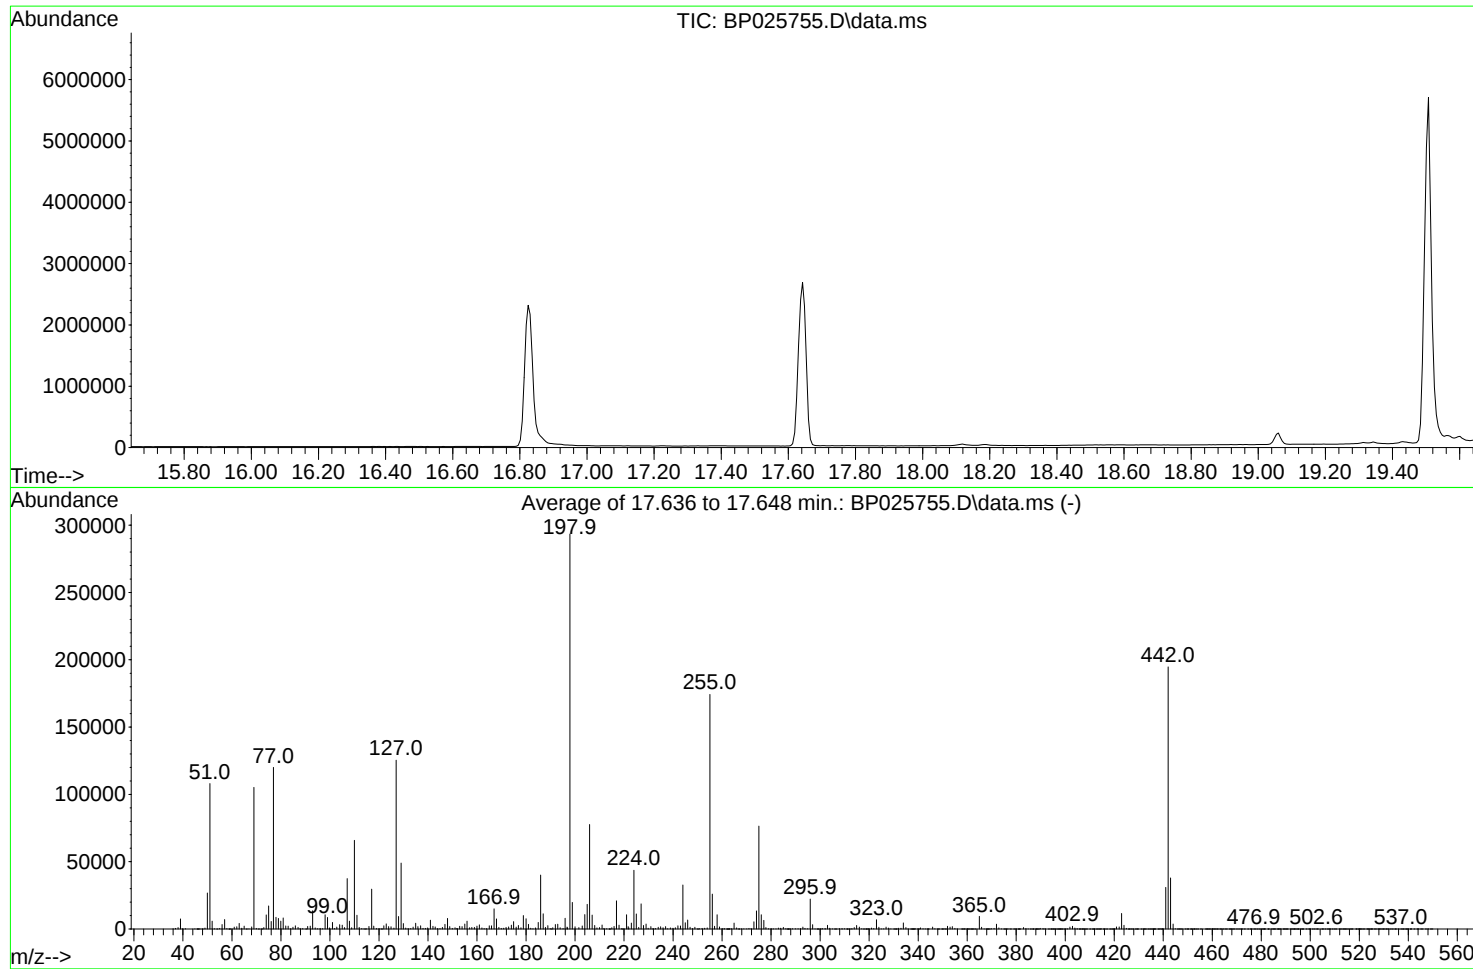

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2488

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	1545	PASS
69	69	100	100	100.0	105244	PASS
70	69	0.00	2	0.5	503	PASS
197	198	0.00	2	0.5	1479	PASS
198	198	100	100	100.0	293310	PASS
199	198	5	9	6.7	19695	PASS
365	198	1	100	3.2	9353	PASS
441	443	0.01	150	81.6	30963	PASS
442	442	100	100	100.0	194731	PASS
443	442	15	24	19.5	37947	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/16/2025	BNA_P	<u>BP025755.D</u>
Compound Name	Response	Retention Time
DDT	1668155	20.789
DDD	15960	20.336
DDE	2097	19.807
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18057	1686212	1.07

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091625\
Data File : BP025755.D
Acq On : 16 Sep 2025 12:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 13:17:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

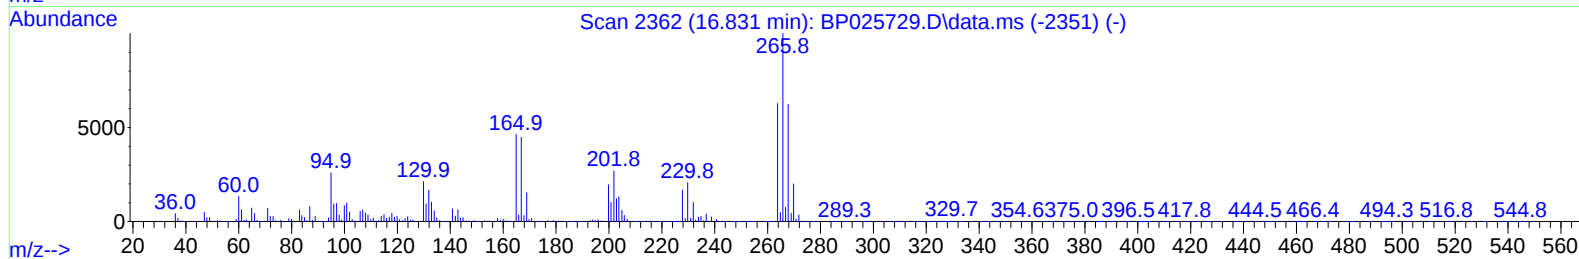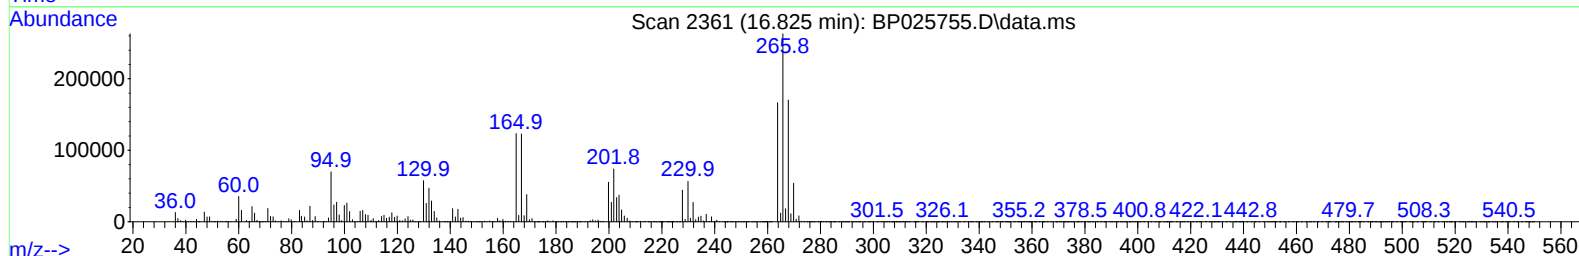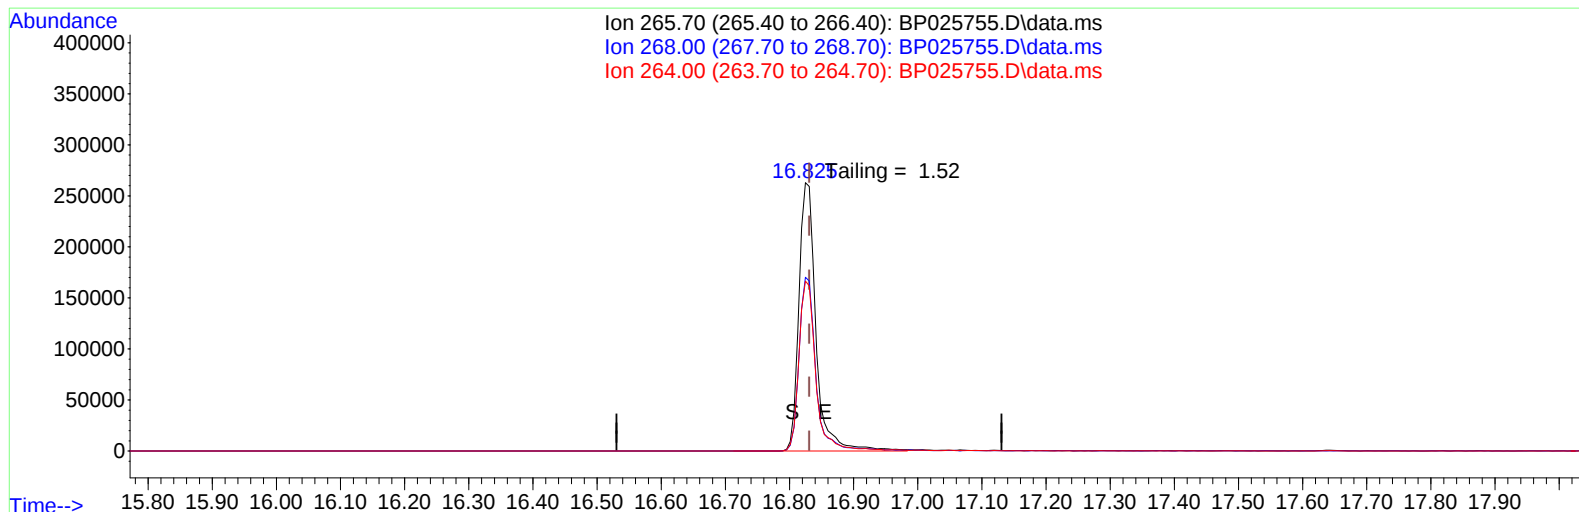

TIC: BP025755.D\data.ms

(70) Pentachlorophenol (C)

16.825min (-0.006) 2241284.43 ng




response 489303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.78
264.00	62.70	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091625\
Data File : BP025755.D
Acq On : 16 Sep 2025 12:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 13:17:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

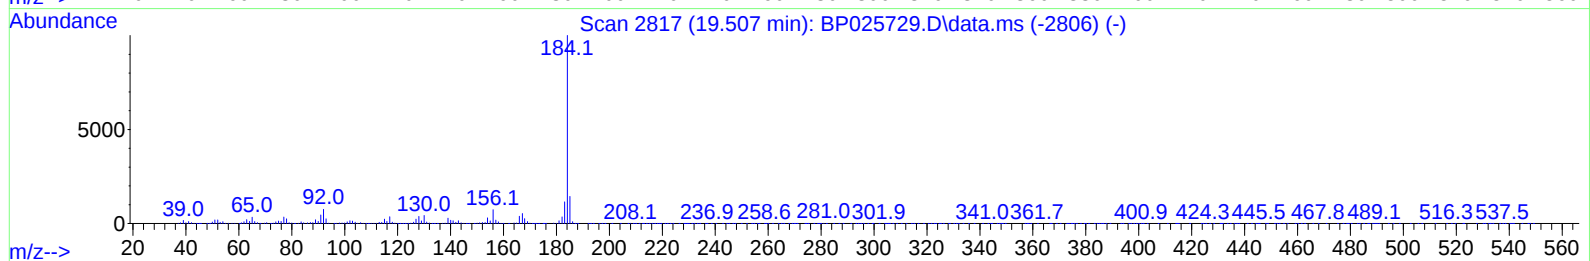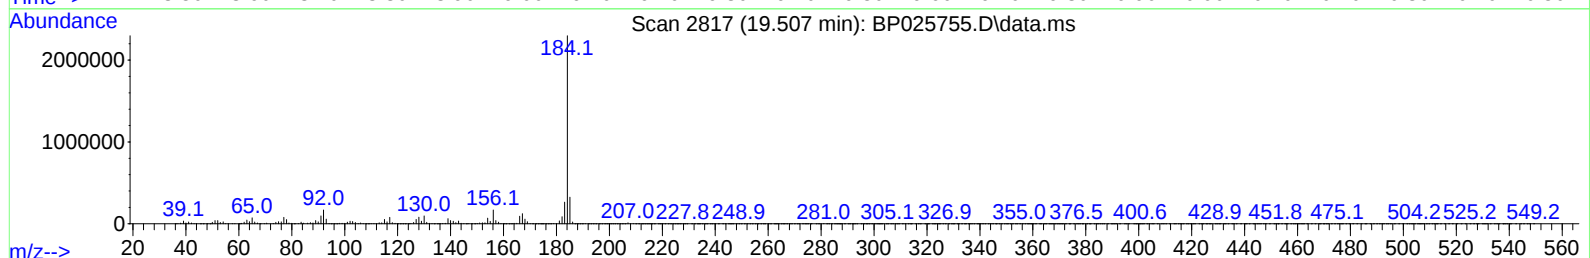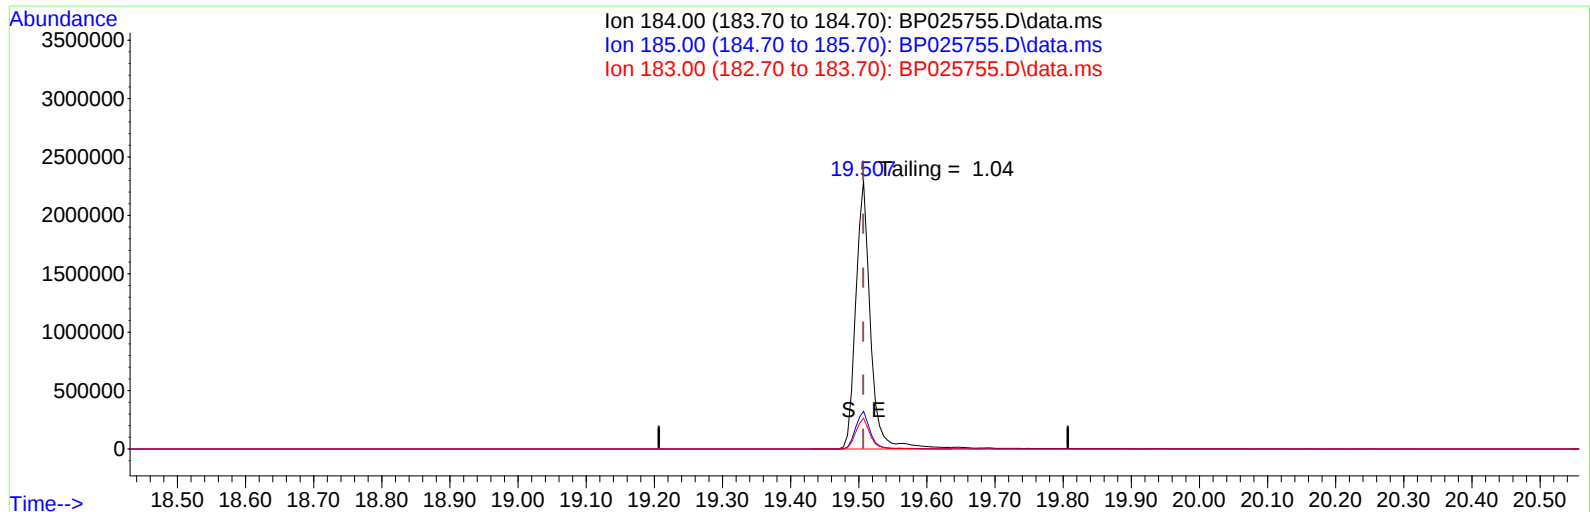

TIC: BP025755.D\data.ms

(77) Benzidine

19.507min (+ 0.000) 744639.67 ng

response 3324689

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.50	11.53
0.00	0.00	0.00