


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091525\
Data File : VN087819.D
Acq On : 15 Sep 2025 08:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

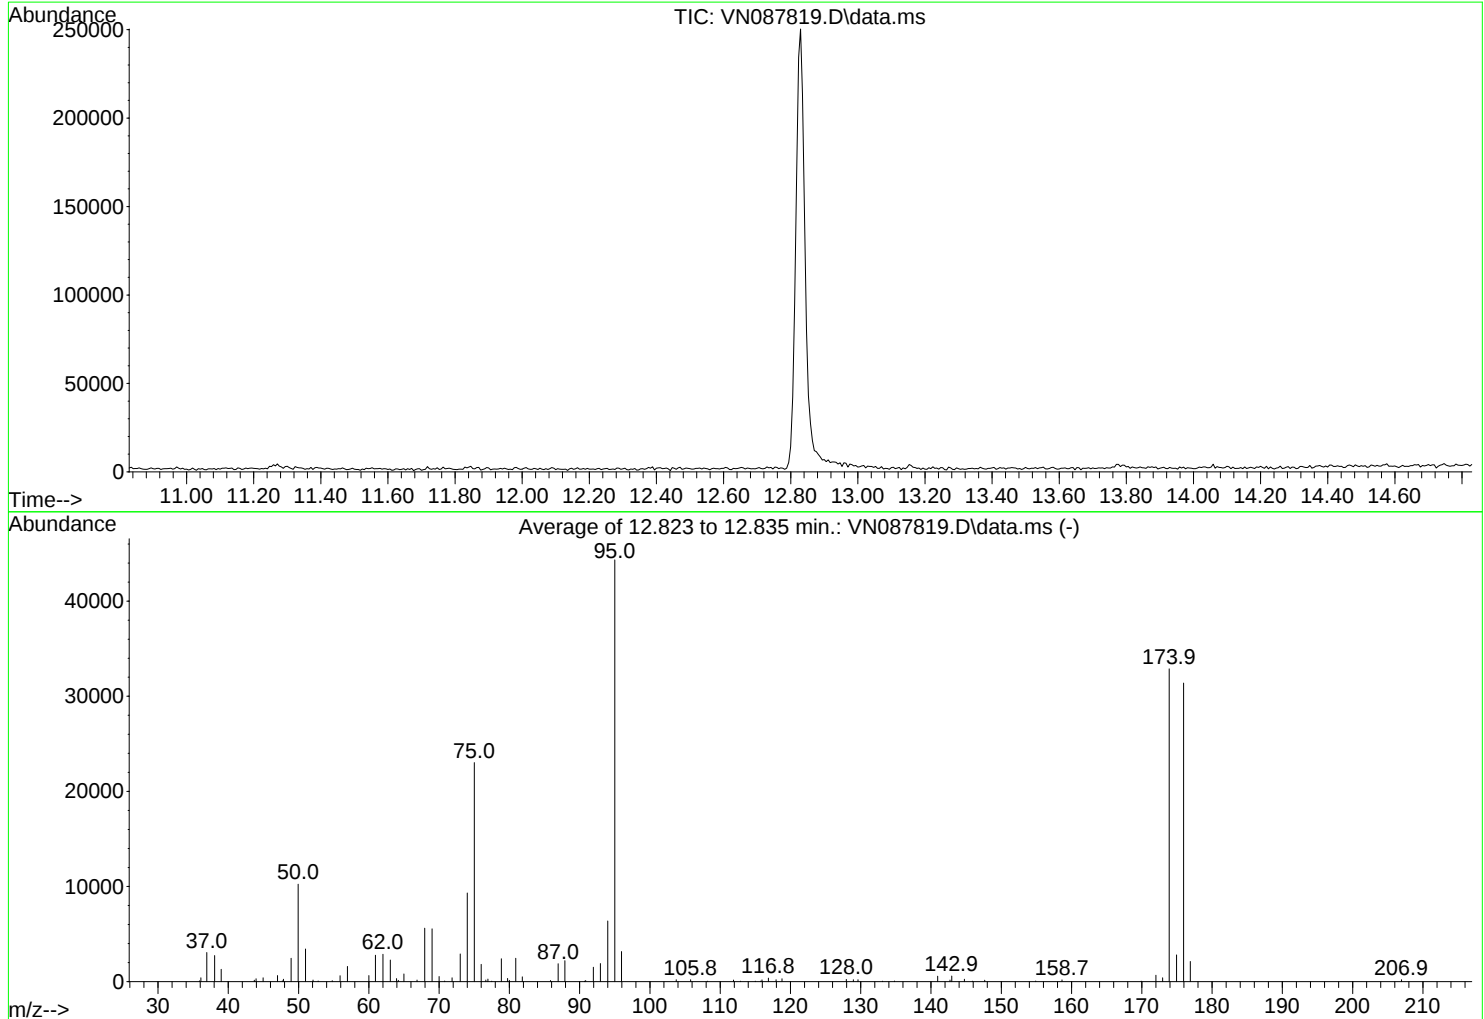

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.1	10243	PASS
75	95	30	60	51.9	23024	PASS
95	95	100	100	100.0	44339	PASS
96	95	5	9	7.1	3168	PASS
173	174	0.00	2	1.2	405	PASS
174	95	50	100	74.1	32877	PASS
175	174	5	9	8.5	2808	PASS
176	174	95	101	95.4	31381	PASS
177	176	5	9	6.8	2122	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	85	48.95	2452	63.05	2268	74.00	931
36.10	401	49.95	10243	63.95	318	75.00	2302
36.95	3064	51.00	3429	64.20	140	76.00	182
38.05	2743	52.05	165	65.00	815	76.65	17
39.00	1294	52.80	61	66.85	171	76.95	278
43.70	155	54.80	94	67.95	5622	77.50	52
43.95	302	55.90	617	69.00	5557	78.85	2406
44.95	398	56.95	1607	70.00	534	79.75	330
47.00	637	60.00	647	70.80	75	80.00	138
47.70	91	60.95	2784	71.85	404	80.90	2464
47.85	257	62.00	2871	73.00	2919	81.85	506

Average of 12.823 to 12.835 min.: VN087819.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.85	122	105.80	204	128.95	205	158.65	191
86.95	1883	108.20	55	129.60	198	169.90	50
87.90	2213	111.90	176	133.10	57	172.00	677
90.70	57	112.90	58	134.80	73	172.95	405
90.85	121	115.00	56	140.95	568	173.90	32877
91.95	1506	115.80	66	142.70	166	174.95	2808
92.95	1901	115.95	191	142.95	596	175.95	31381
94.00	6372	116.85	378	144.75	247	176.90	2122
95.00	44339	117.95	207	145.90	53	206.95	199
95.95	3168	118.80	310	147.65	155		
103.75	200	127.95	244	154.90	64		

Instrument :

MSVOA_N

ClientSampleId :

BFB