


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
Data File : BN037689.D
Acq On : 11 Sep 2025 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

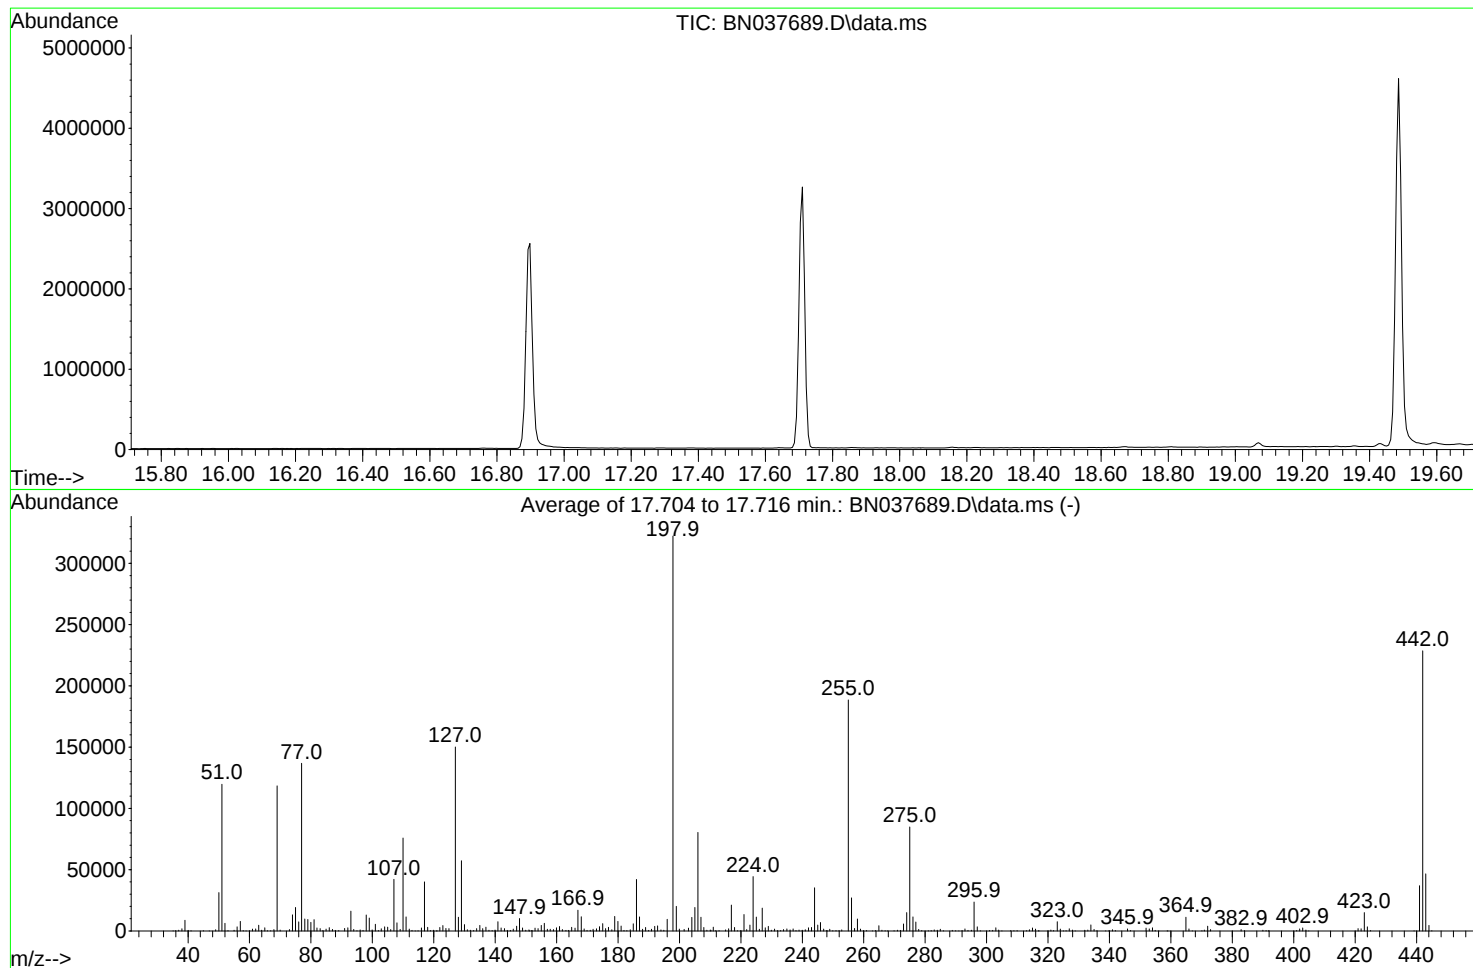




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.0	1148	PASS
69	69	100	100	100.0	118397	PASS
70	69	0.00	2	0.6	697	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	322261	PASS
199	198	5	9	6.2	20092	PASS
365	198	1	100	3.5	11183	PASS
441	443	0.01	150	79.2	36909	PASS
442	442	100	100	100.0	228651	PASS
443	442	15	24	20.4	46619	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
Data File : BN037689.D
Acq On : 11 Sep 2025 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 11 13:15:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 13:14:53 2025
Response via : Initial Calibration

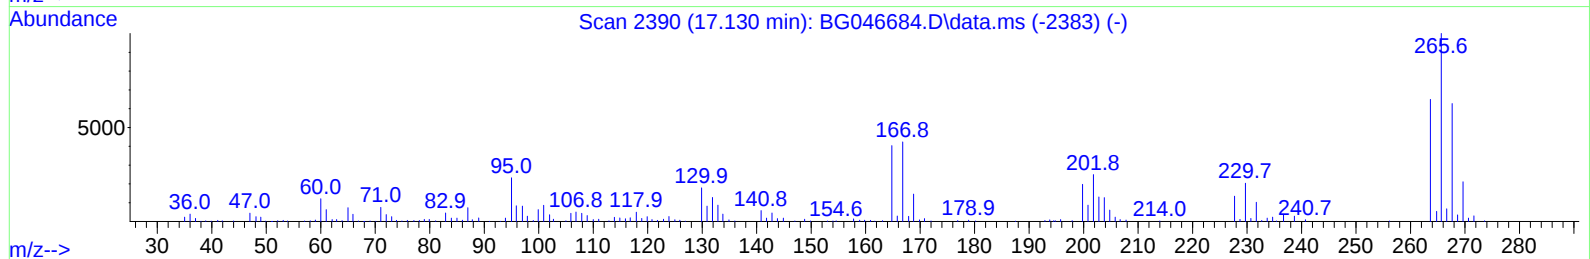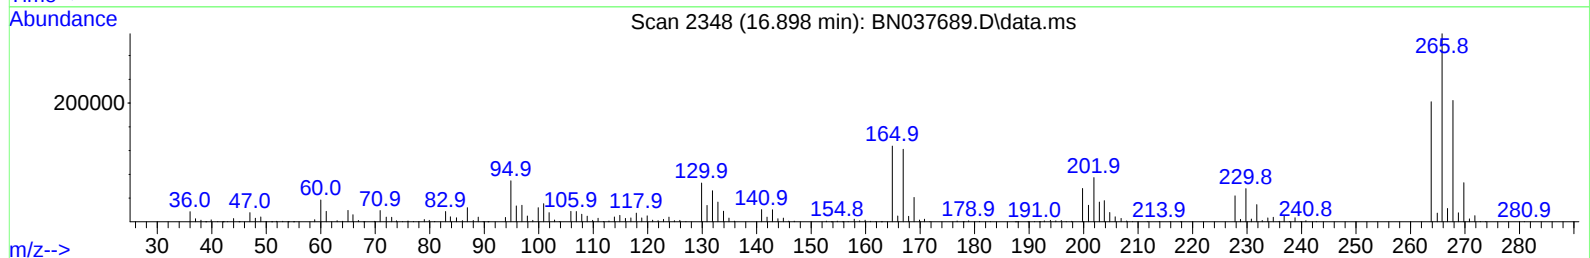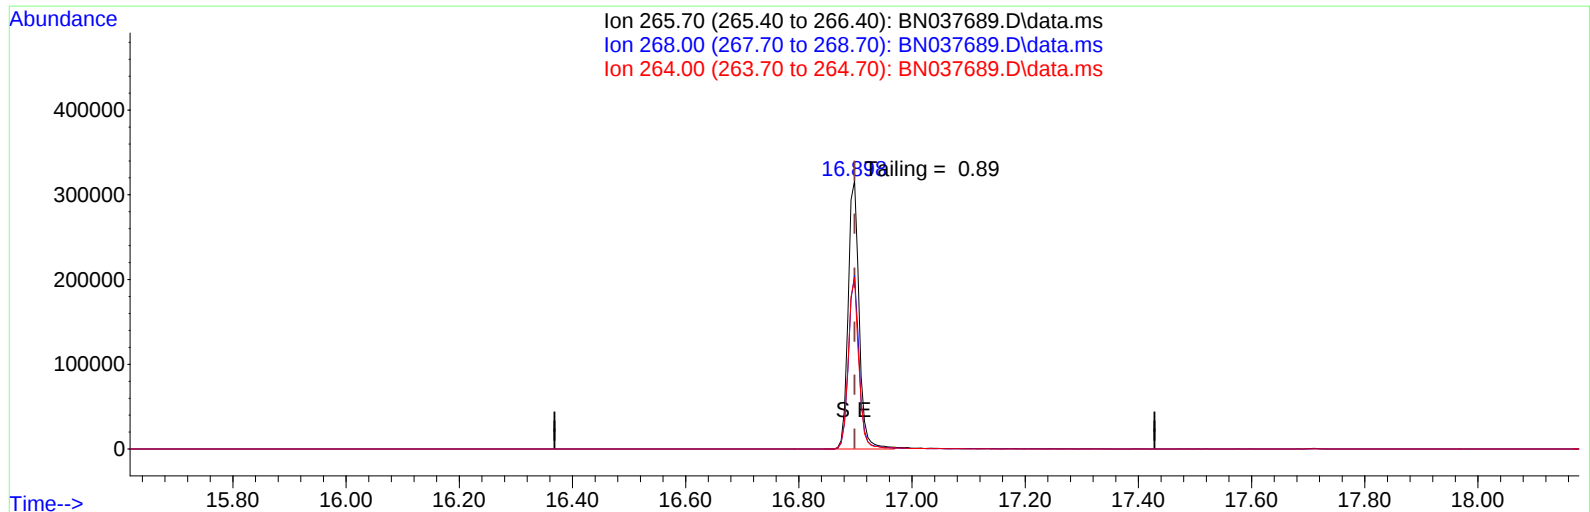

TIC: BN037689.D\data.ms

(70) Pentachlorophenol (C)

16.898min (0.000) 277.63 ng




response 430126

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.54
264.00	63.90	63.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
Data File : BN037689.D
Acq On : 11 Sep 2025 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 11 13:15:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 13:14:53 2025
Response via : Initial Calibration

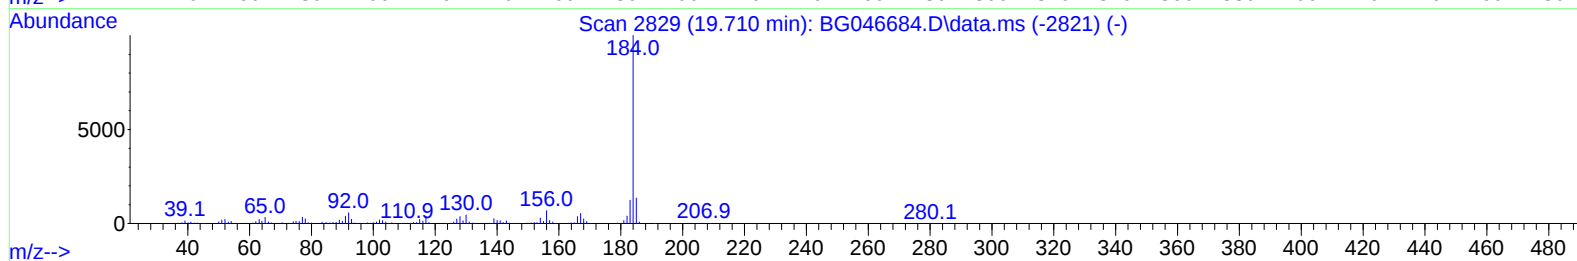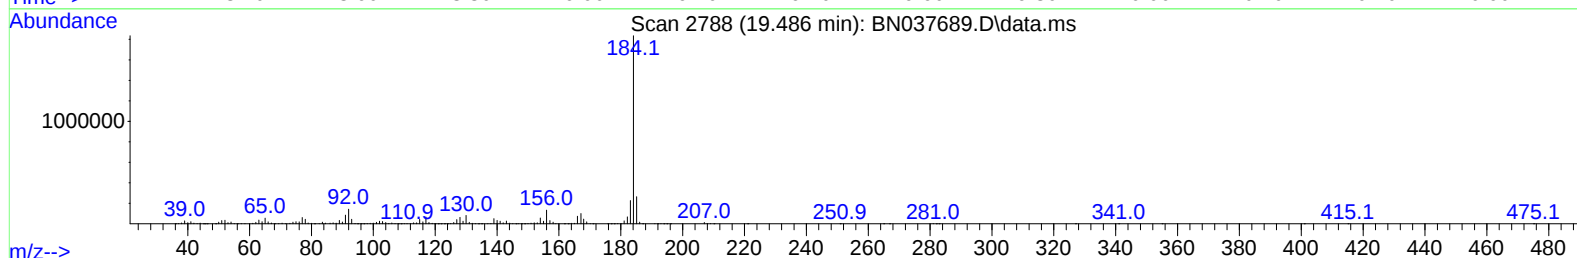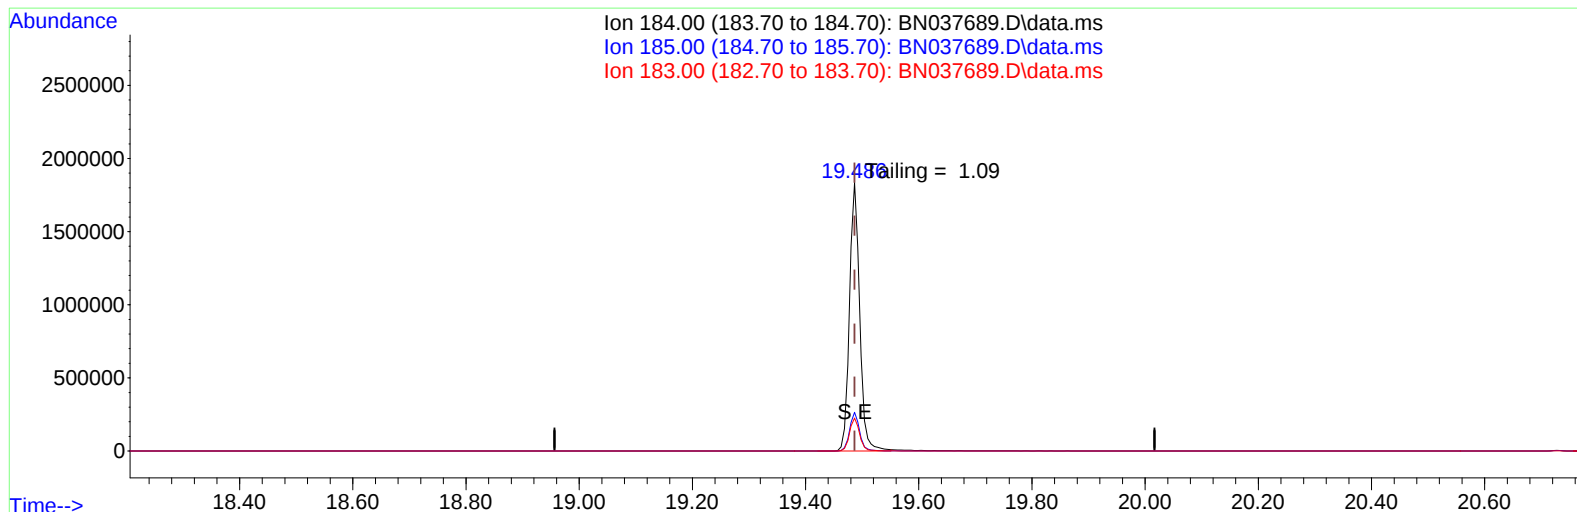

TIC: BN037689.D\data.ms

(77) Benzidine

19.486min (0.000) 64237.37 ng

response 2281946

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.43
183.00	12.30	12.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/11/2025	BNA_N	<u>BN037689.D</u>
Compound Name	Response	Retention Time
DDT	1069016	20.727
DDD	7982	20.286
DDE	769	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8751	1077767	0.81

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP