


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037739.D
Acq On : 17 Sep 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

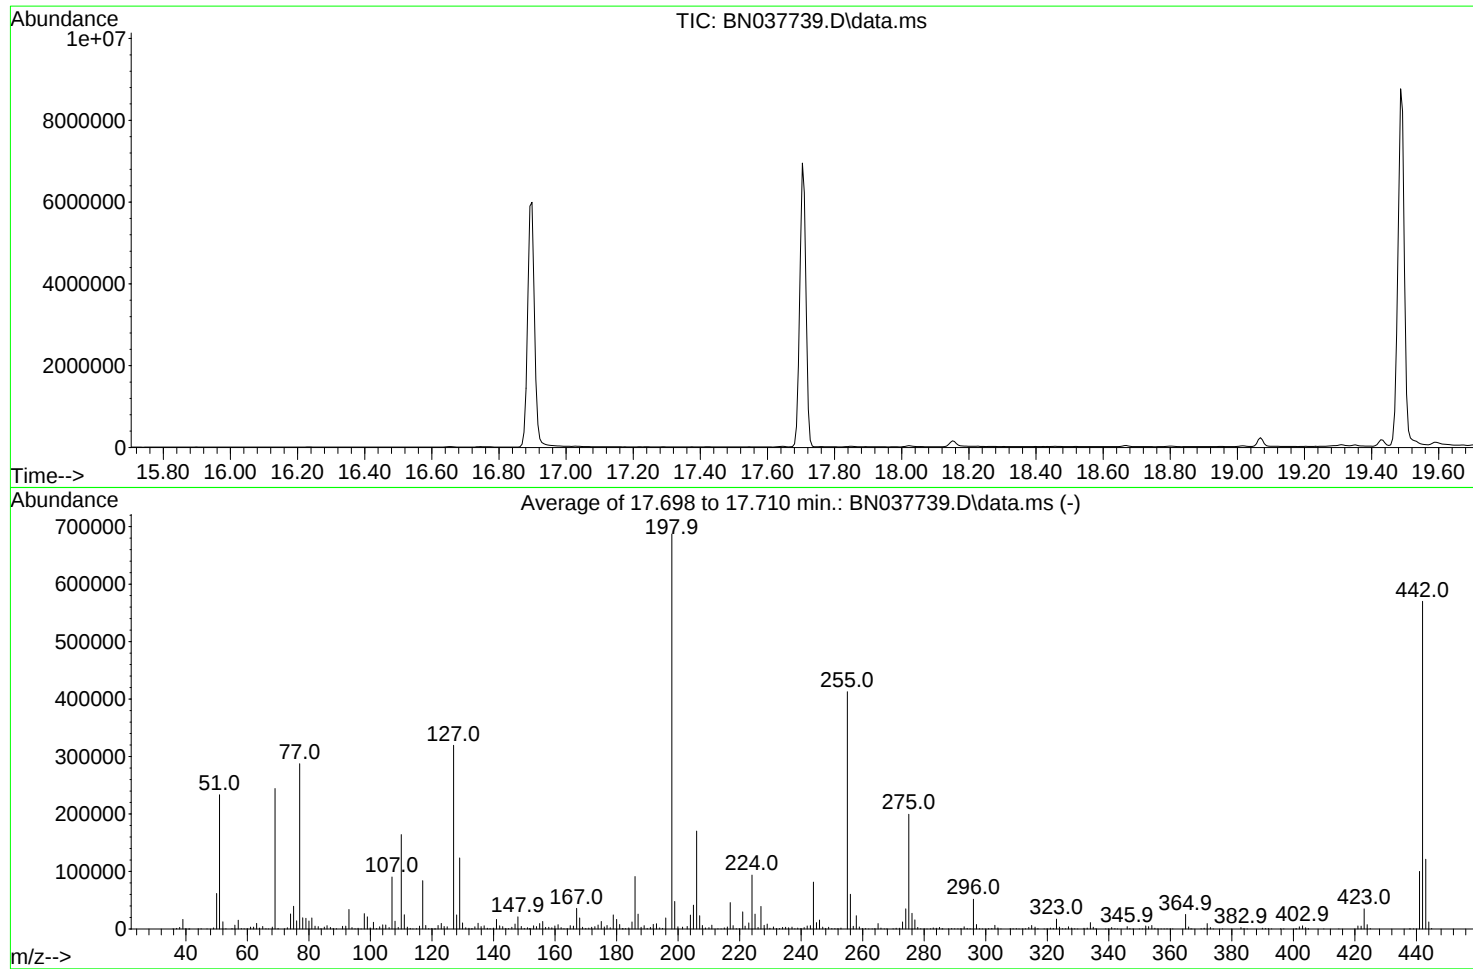




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	3107	PASS
69	69	100	100	100.0	244250	PASS
70	69	0.00	2	0.4	1067	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	687061	PASS
199	198	5	9	6.9	47709	PASS
365	198	1	100	3.7	25139	PASS
441	443	0.01	150	82.6	100245	PASS
442	442	100	100	100.0	570155	PASS
443	442	15	24	21.3	121381	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037739.D
Acq On : 17 Sep 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 17 12:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 17 12:55:52 2025
Response via : Initial Calibration

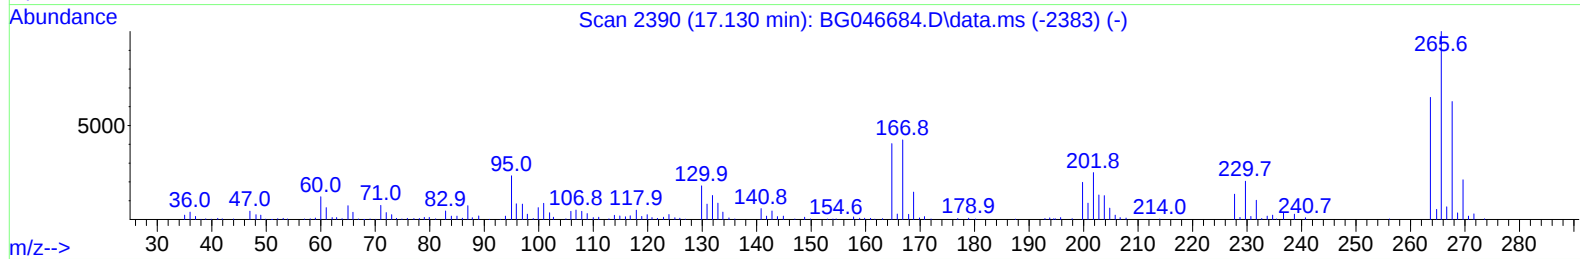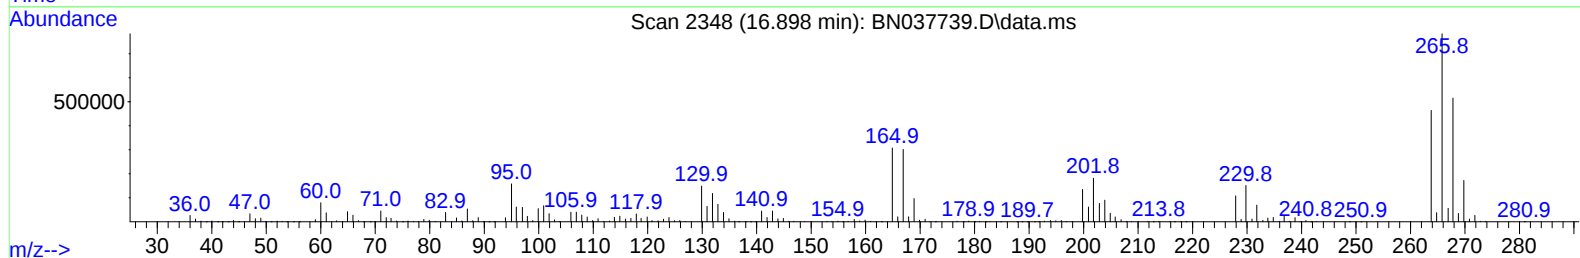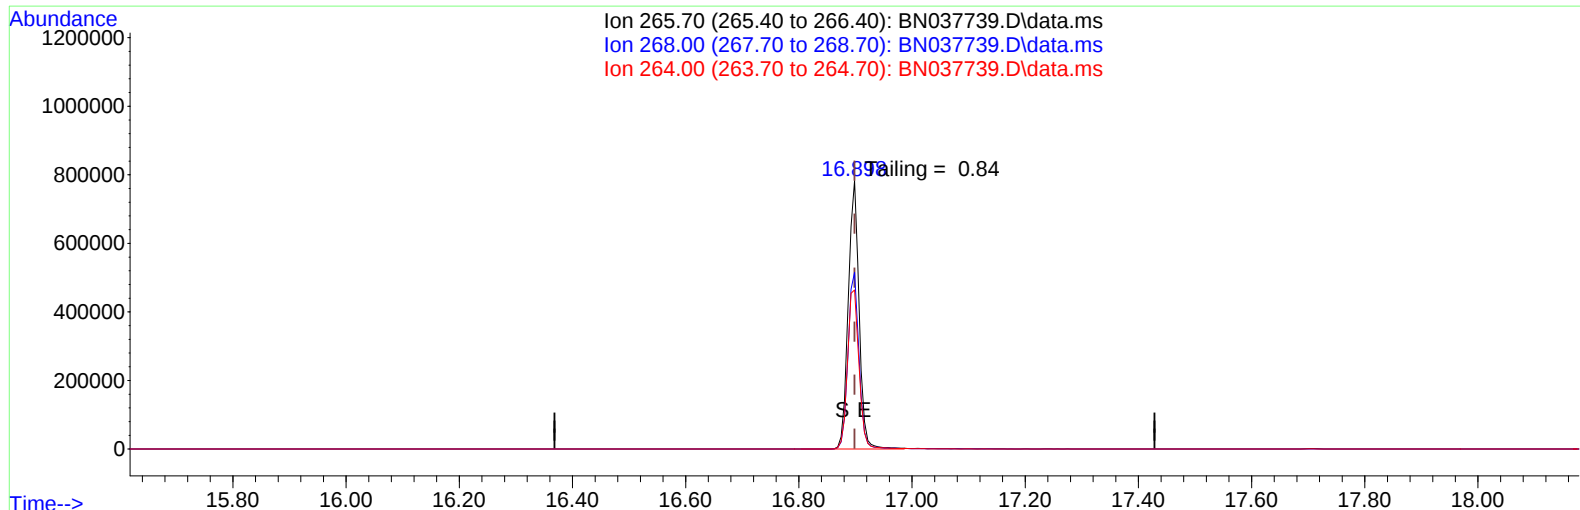

TIC: BN037739.D\data.ms

(70) Pentachlorophenol (C)

16.898min (0.000) 620.62 ng




response 1035710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.84
264.00	61.60	59.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037739.D
Acq On : 17 Sep 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 17 12:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 17 12:55:52 2025
Response via : Initial Calibration

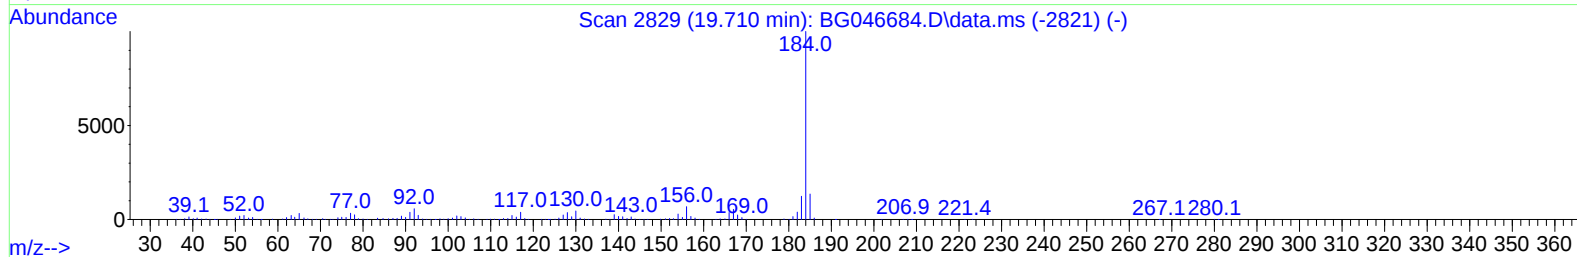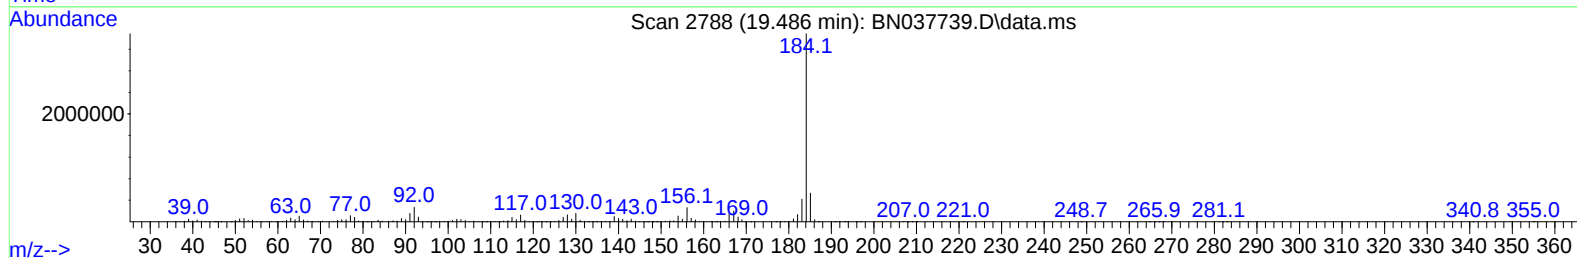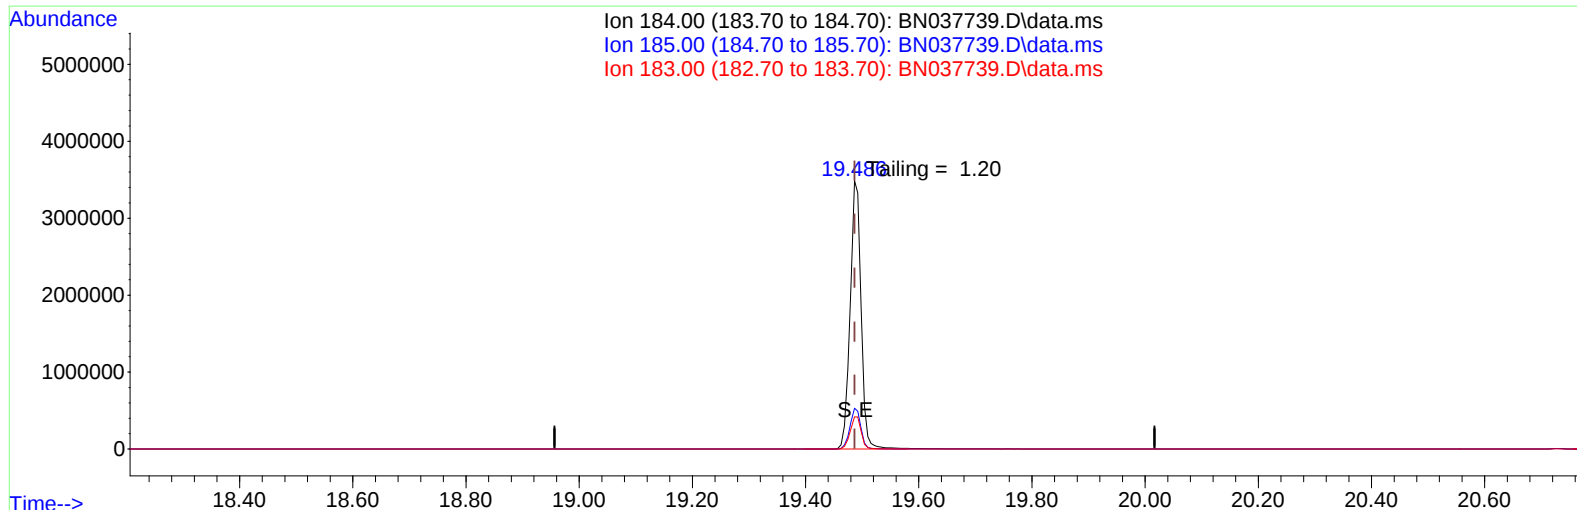

TIC: BN037739.D\data.ms

(77) Benzidine

19.486min (0.000) 3519.75 ng

response 4617215

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.21
183.00	13.20	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2025	BNA_N	<u>BN037739.D</u>
Compound Name	Response	Retention Time
DDT	2253525	20.727
DDD	23969	20.286
DDE	1849	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25818	2279343	1.13

Instrument :
BNA_N
ClientSampleId :
DFTPP