
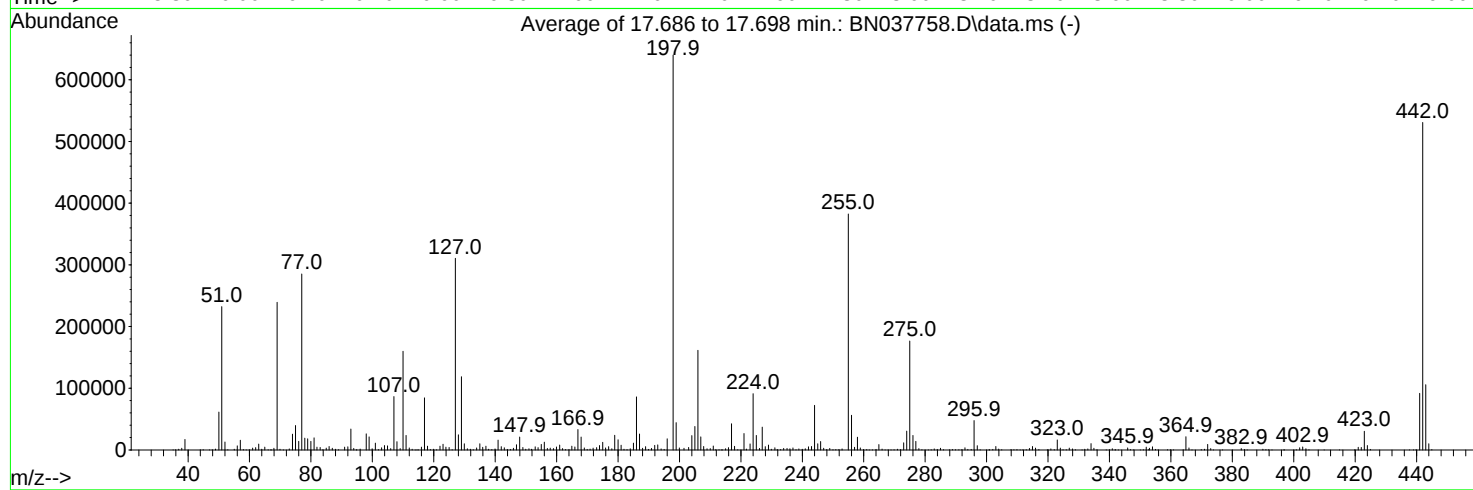


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037758.D
Acq On : 18 Sep 2025 02:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

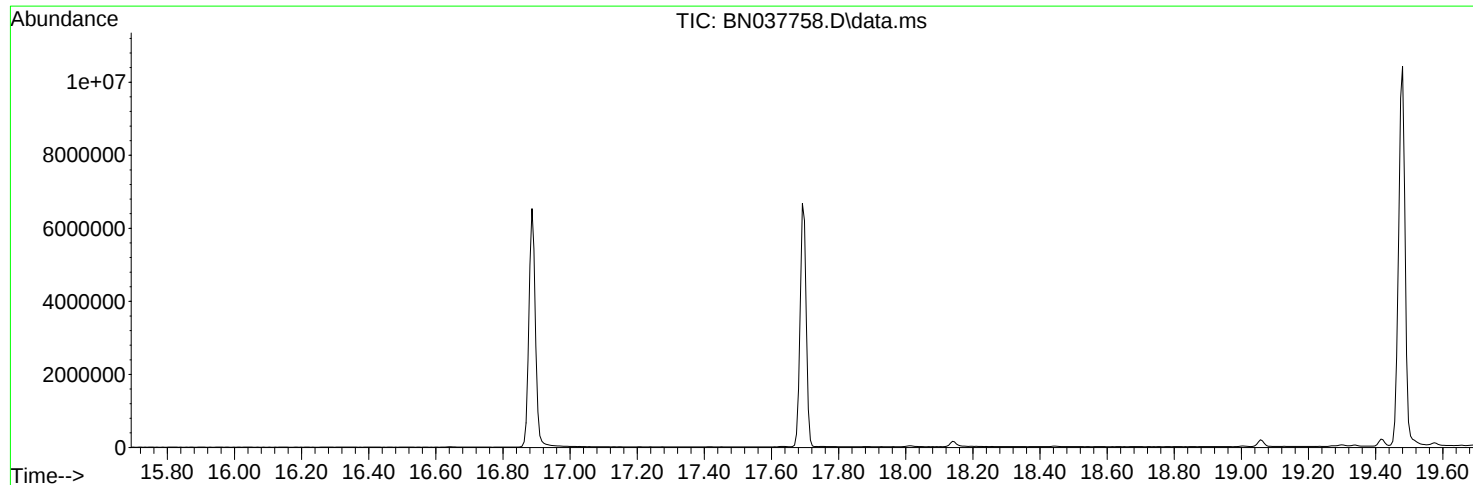




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.1	2651	PASS
69	69	100	100	100.0	239192	PASS
70	69	0.00	2	0.5	1177	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	640043	PASS
199	198	5	9	6.9	44243	PASS
365	198	1	100	3.3	21358	PASS
441	443	0.01	150	86.6	91685	PASS
442	442	100	100	100.0	530709	PASS
443	442	15	24	19.9	105811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037758.D
Acq On : 18 Sep 2025 02:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 08:37:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 18 08:37:03 2025
Response via : Initial Calibration

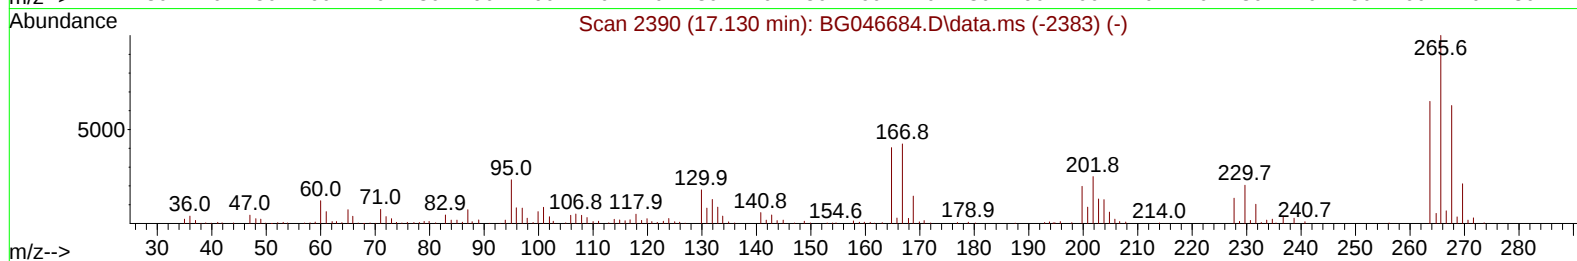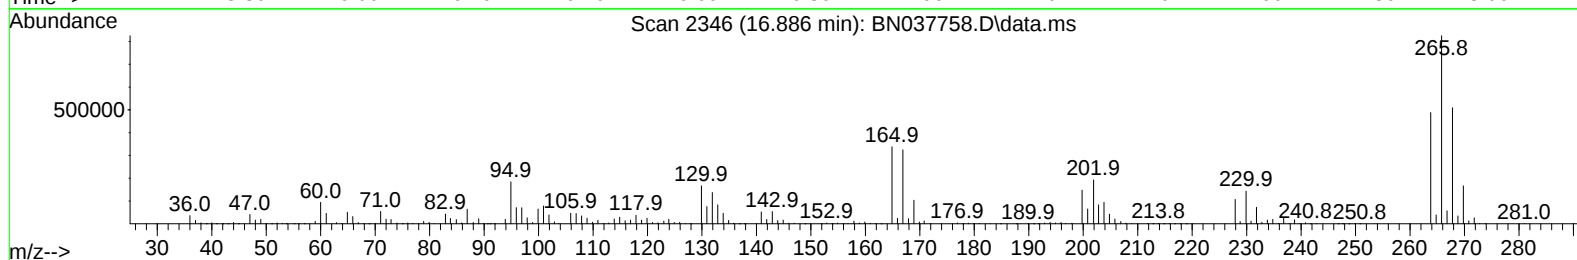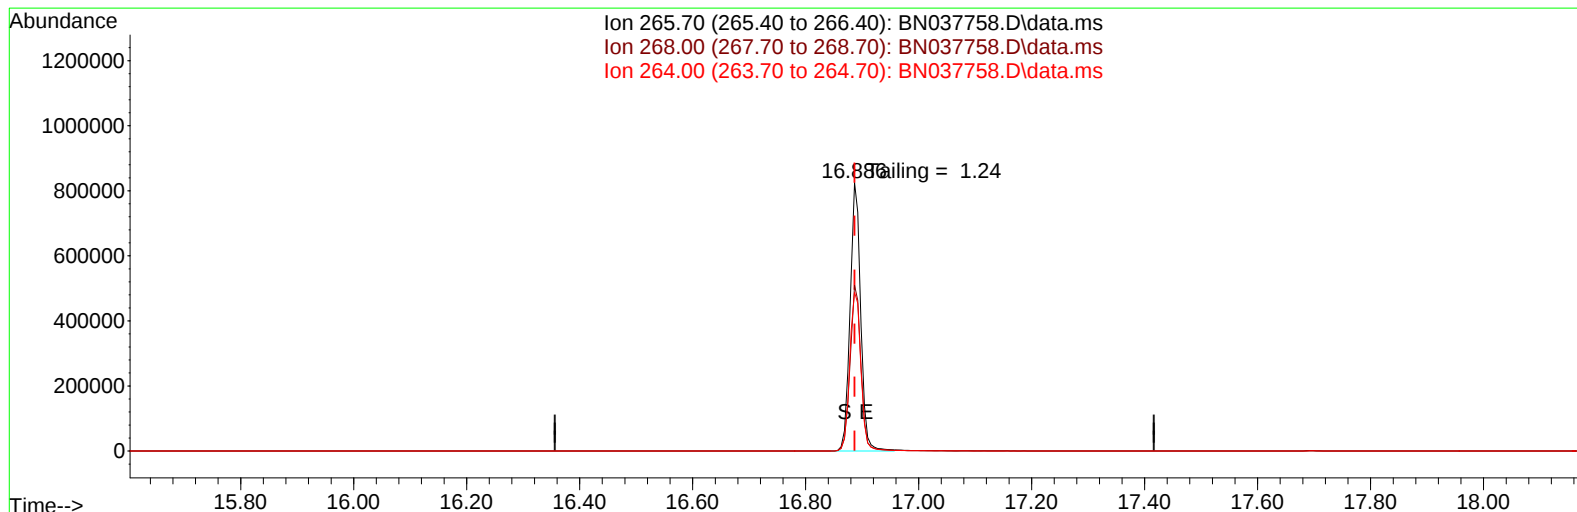

TIC: BN037758.D\data.ms

(70) Pentachlorophenol (C)

16.886min (0.000) 150096.94 ng




response 1070732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.72
264.00	61.60	59.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037758.D
Acq On : 18 Sep 2025 02:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 08:37:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 18 08:37:03 2025
Response via : Initial Calibration

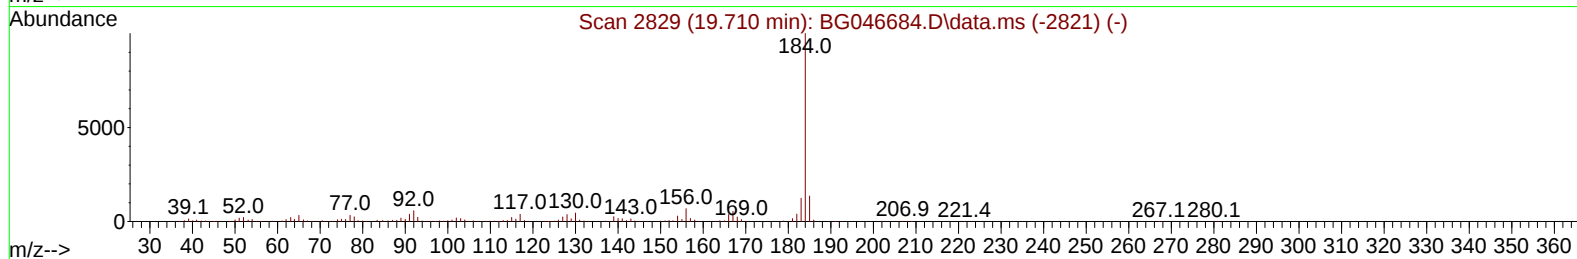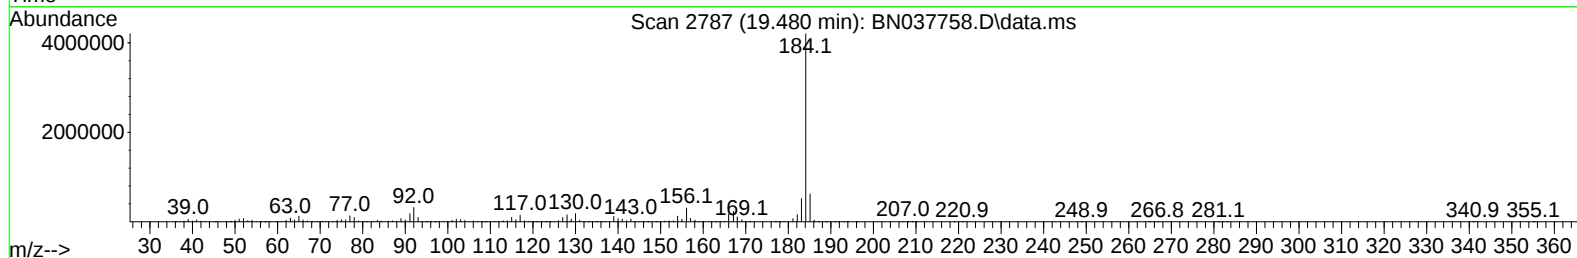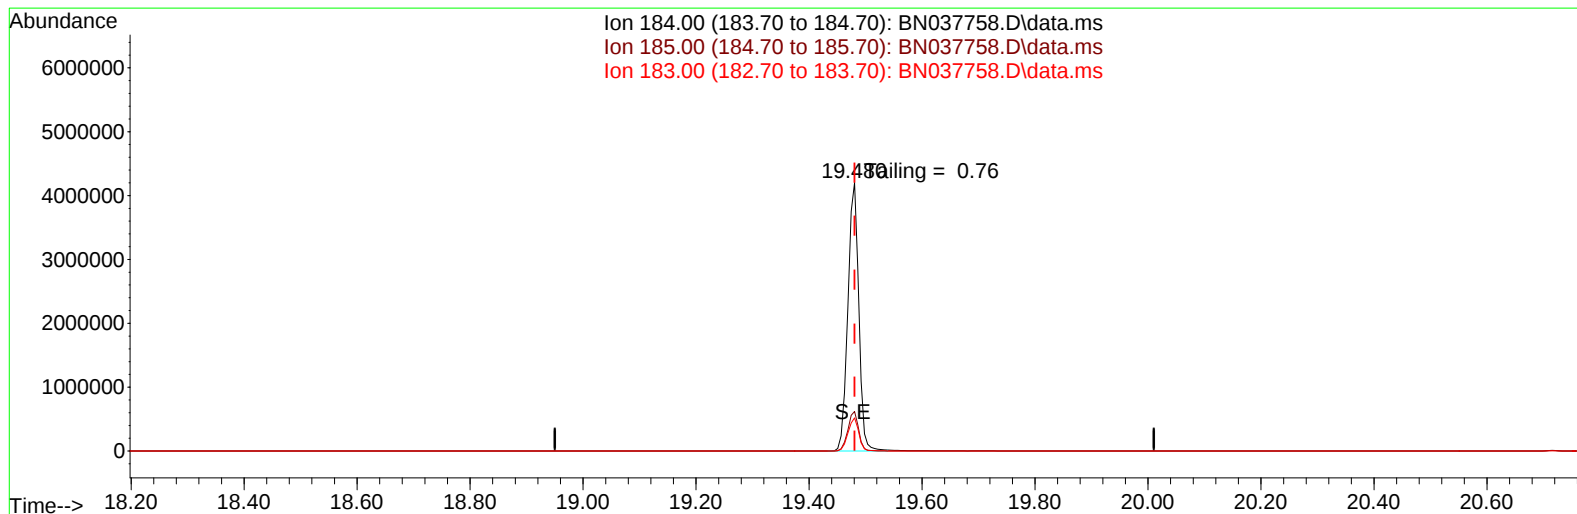

TIC: BN037758.D\data.ms

(77) Benzidine

19.480min (0.000) 95951.94 ng

response 5587198

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2025	BNA_N	<u>BN037758.D</u>
Compound Name	Response	Retention Time
DDT	2444036	20.716
DDD	52273	20.274
DDE	1911	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
54184	2498220	2.17

Instrument :
BNA_N
ClientSampleId :
DFTPP