
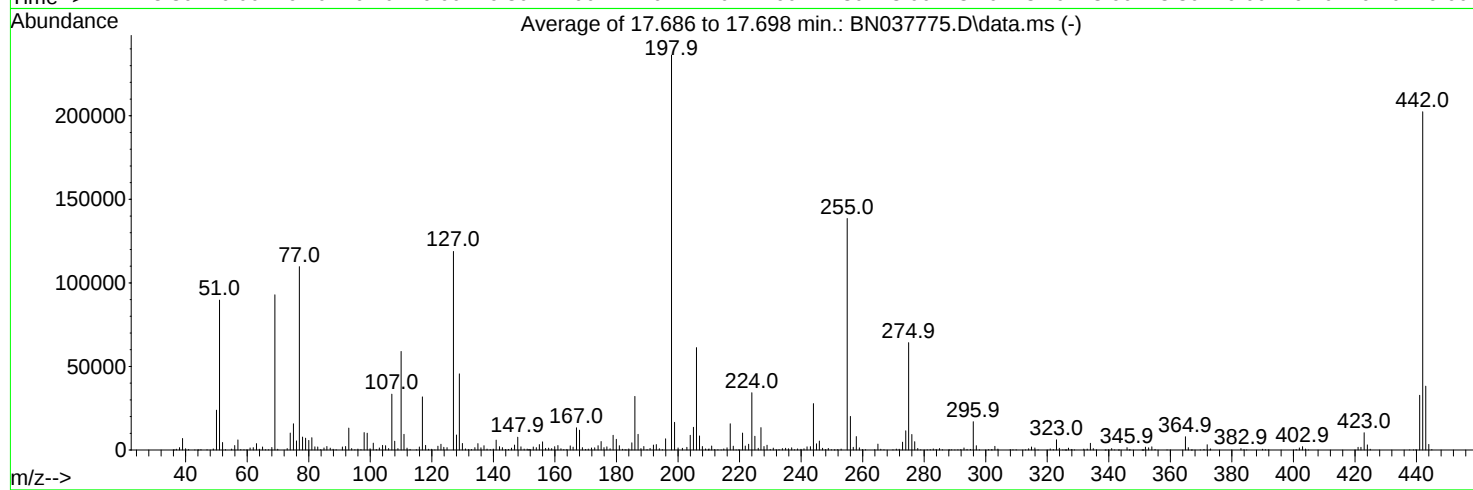


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091825\
Data File : BN037775.D
Acq On : 18 Sep 2025 13:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

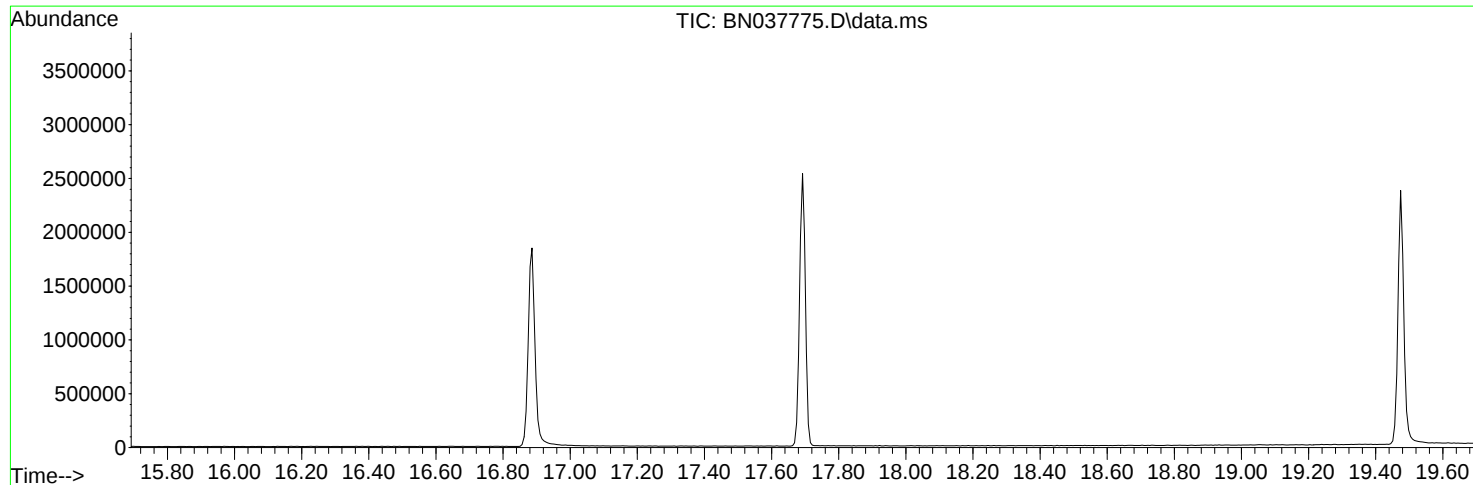




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	1536	PASS
69	69	100	100	100.0	92893	PASS
70	69	0.00	2	0.5	488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	236267	PASS
199	198	5	9	7.0	16530	PASS
365	198	1	100	3.4	7963	PASS
441	443	0.01	150	85.6	32739	PASS
442	442	100	100	100.0	202432	PASS
443	442	15	24	18.9	38232	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091825\
Data File : BN037775.D
Acq On : 18 Sep 2025 13:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 14:26:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 18 14:26:16 2025
Response via : Initial Calibration

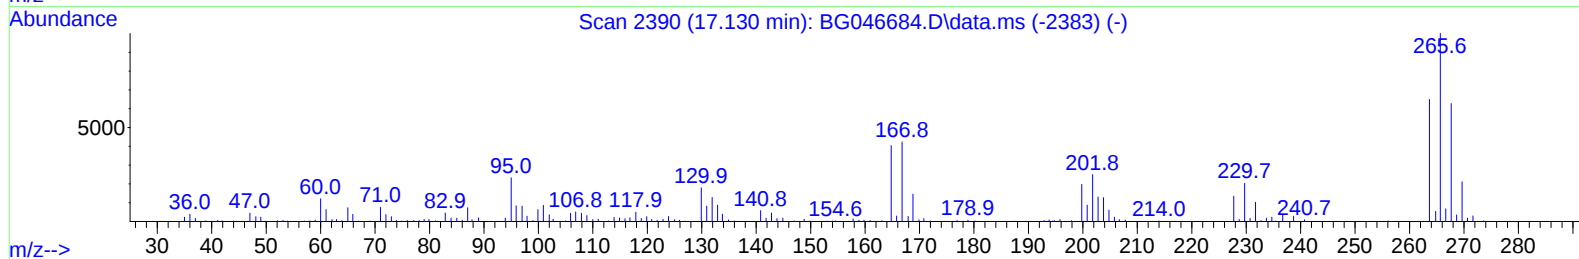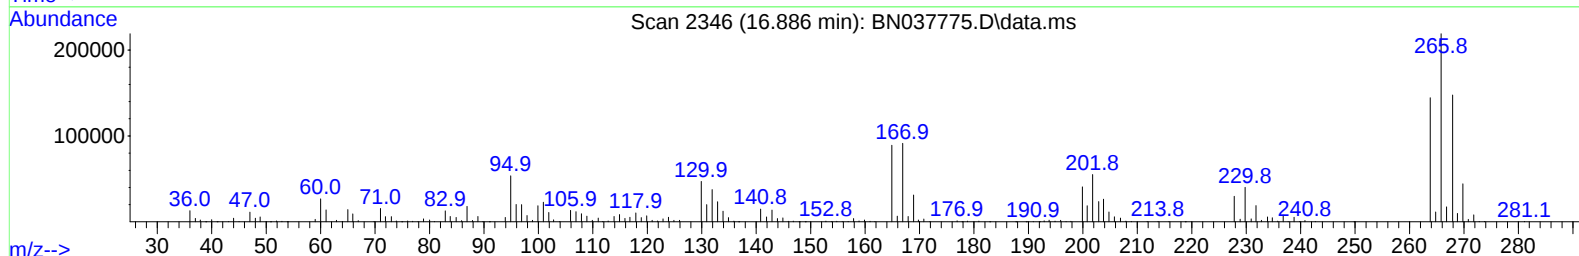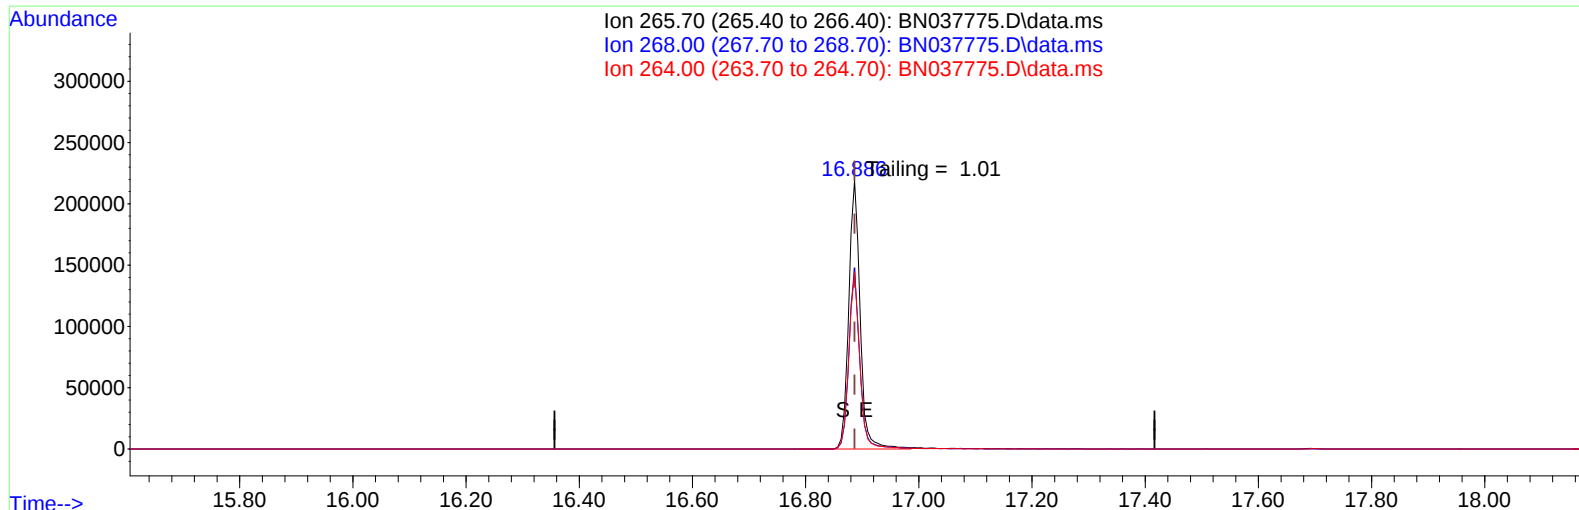

TIC: BN037775.D\data.ms

(70) Pentachlorophenol (C)

16.886min (0.000) 277.80 ng




response 307595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.44
264.00	61.60	66.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091825\
Data File : BN037775.D
Acq On : 18 Sep 2025 13:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 14:26:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 18 14:26:16 2025
Response via : Initial Calibration

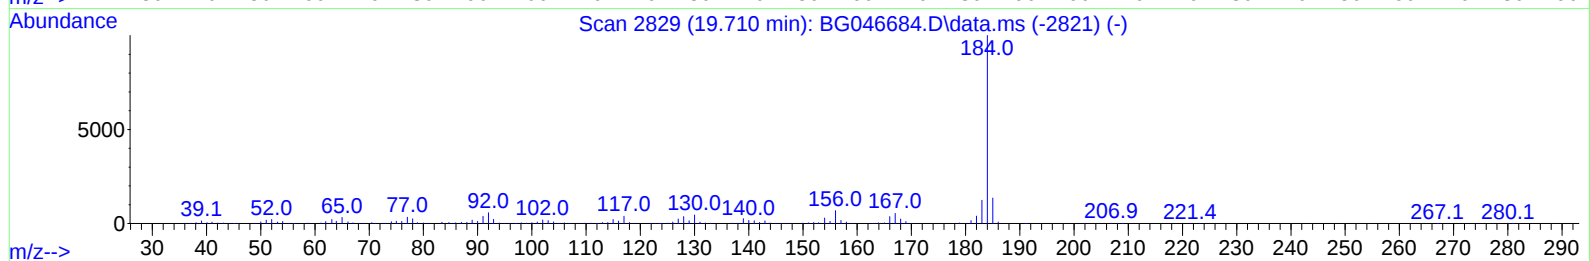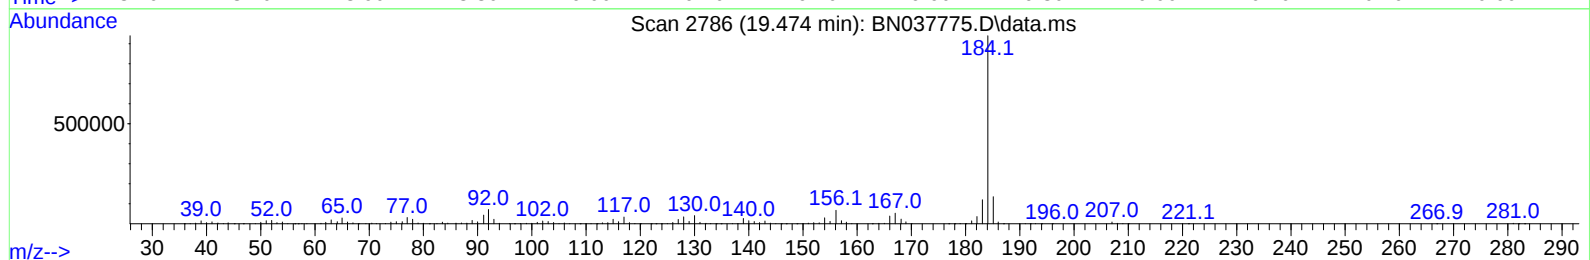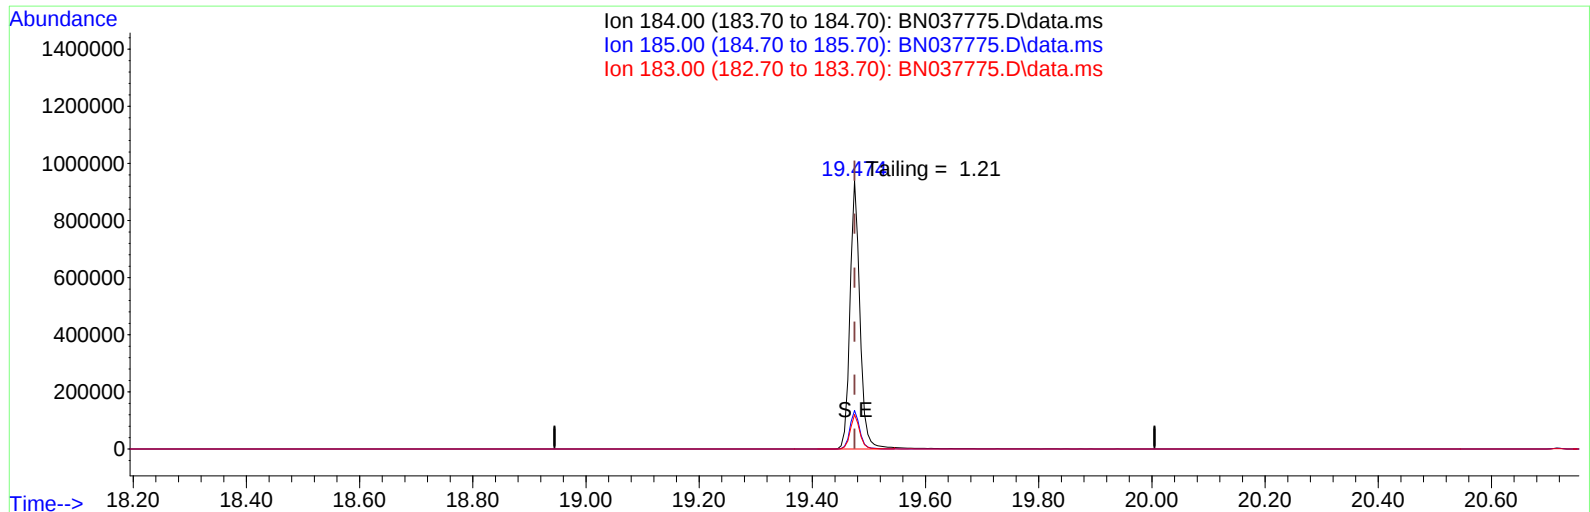

TIC: BN037775.D\data.ms

(77) Benzidine

19.474min (0.000) 0.00 ng

response 1155100

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	12.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2025	BNA_N	<u>BN037775.D</u>
Compound Name	Response	Retention Time
DDT	760598	20.715
DDD	22424	20.274
DDE	1646	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24070	784668	3.07

Instrument :
BNA_N
ClientSampleId :
DFTPP