
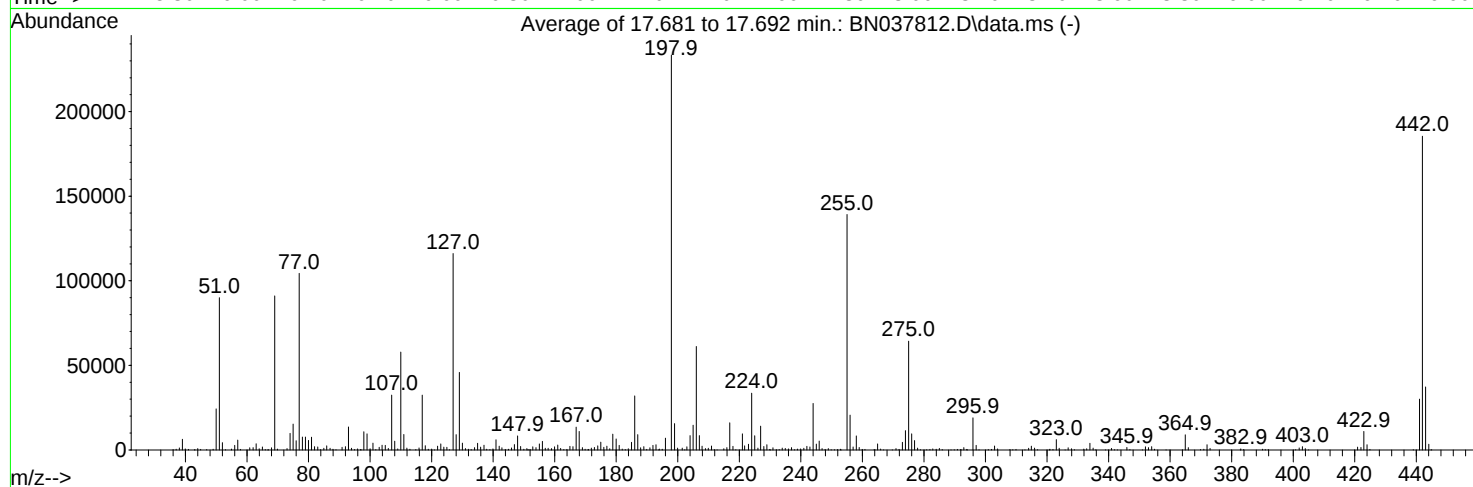


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037812.D
Acq On : 19 Sep 2025 13:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

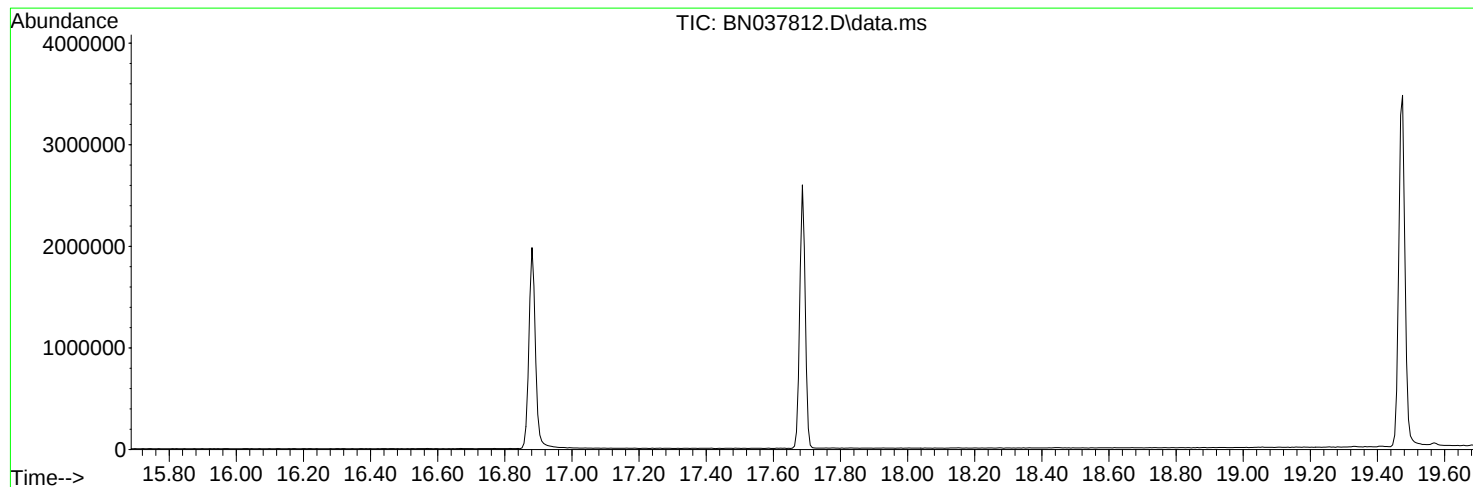




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	1252	PASS
69	69	100	100	100.0	91029	PASS
70	69	0.00	2	0.6	539	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	233408	PASS
199	198	5	9	6.7	15546	PASS
365	198	1	100	3.8	8907	PASS
441	443	0.01	150	80.8	30061	PASS
442	442	100	100	100.0	185456	PASS
443	442	15	24	20.1	37200	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037812.D
Acq On : 19 Sep 2025 13:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 20:01:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

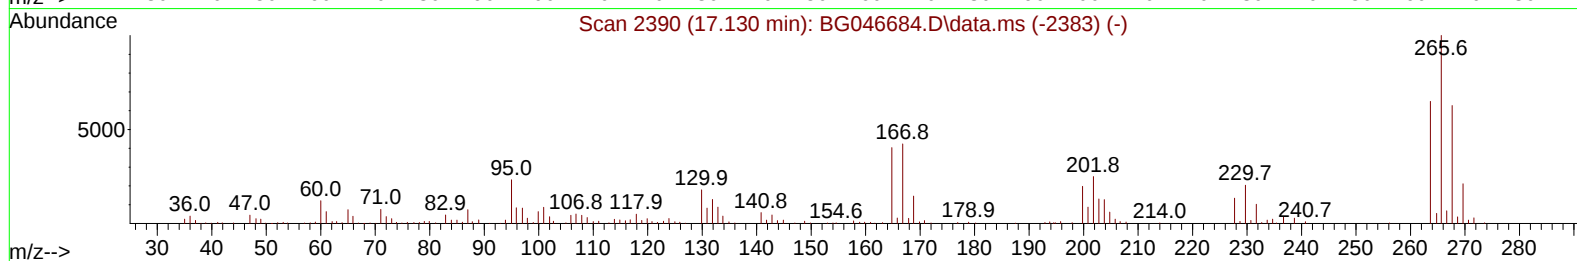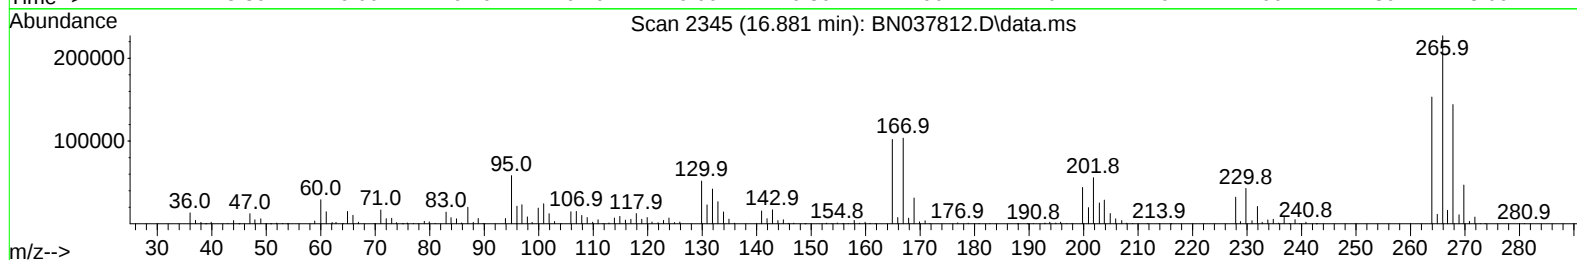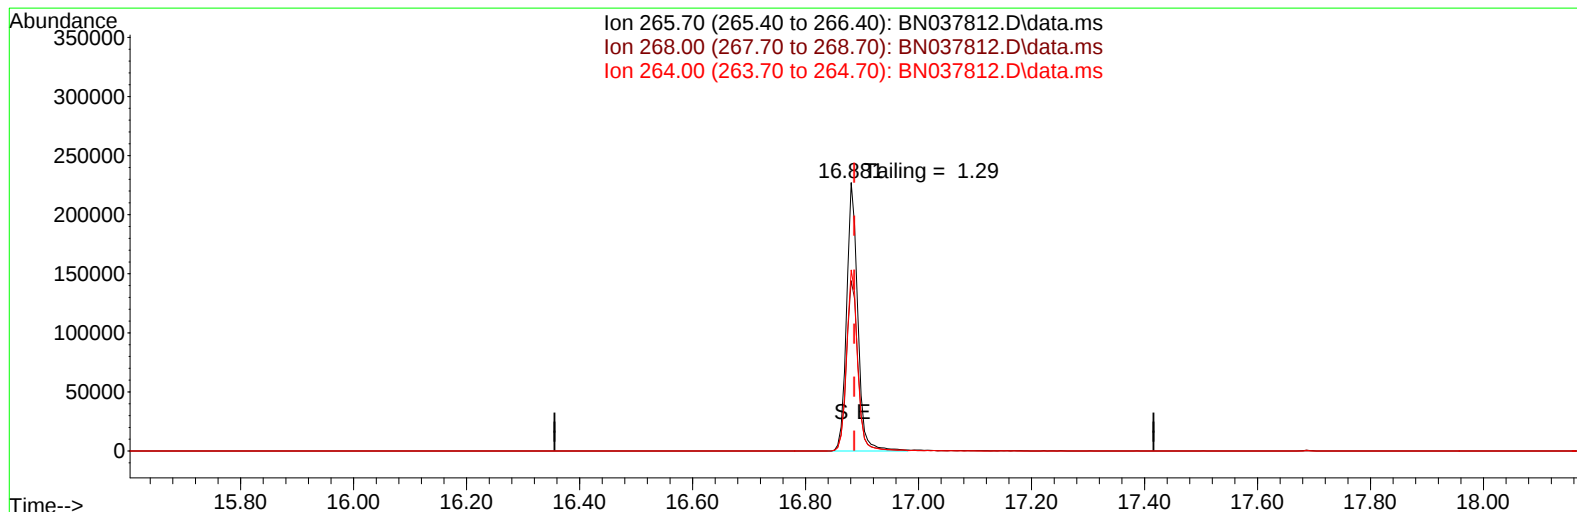

TIC: BN037812.D\data.ms

(70) Pentachlorophenol (C)

16.881min (-0.005) 23824.83 ng




response 312055

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.43
264.00	61.60	67.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037812.D
Acq On : 19 Sep 2025 13:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 20:01:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

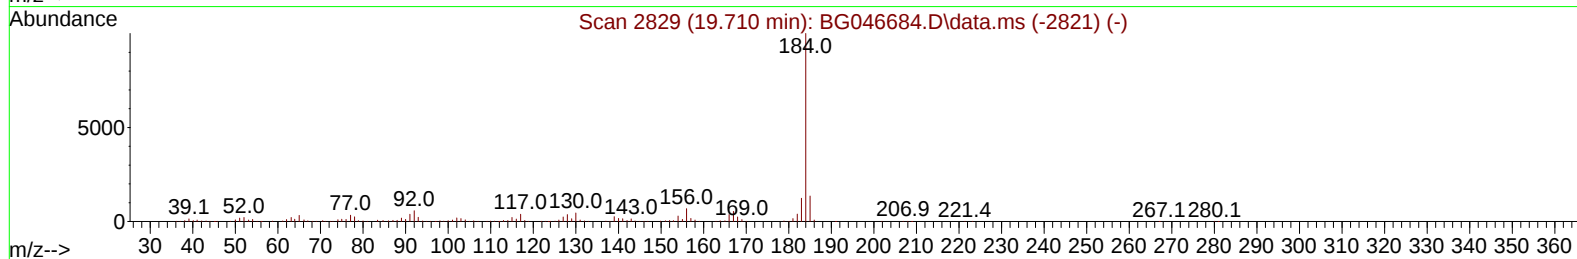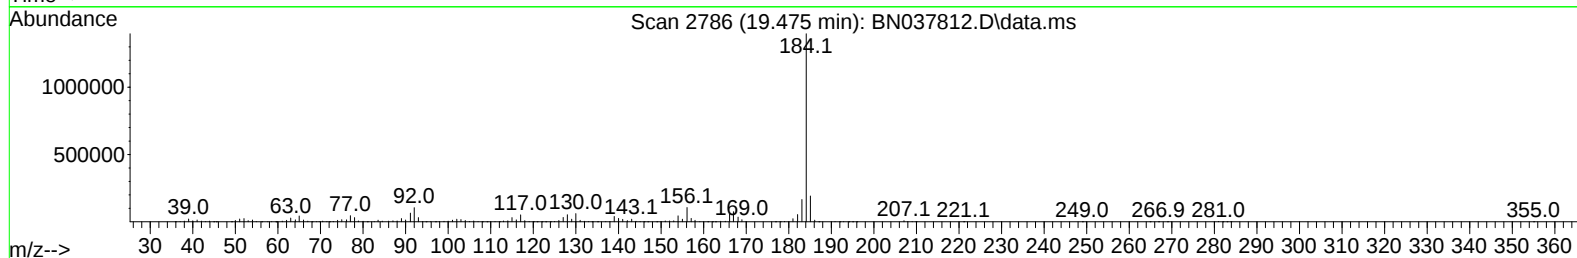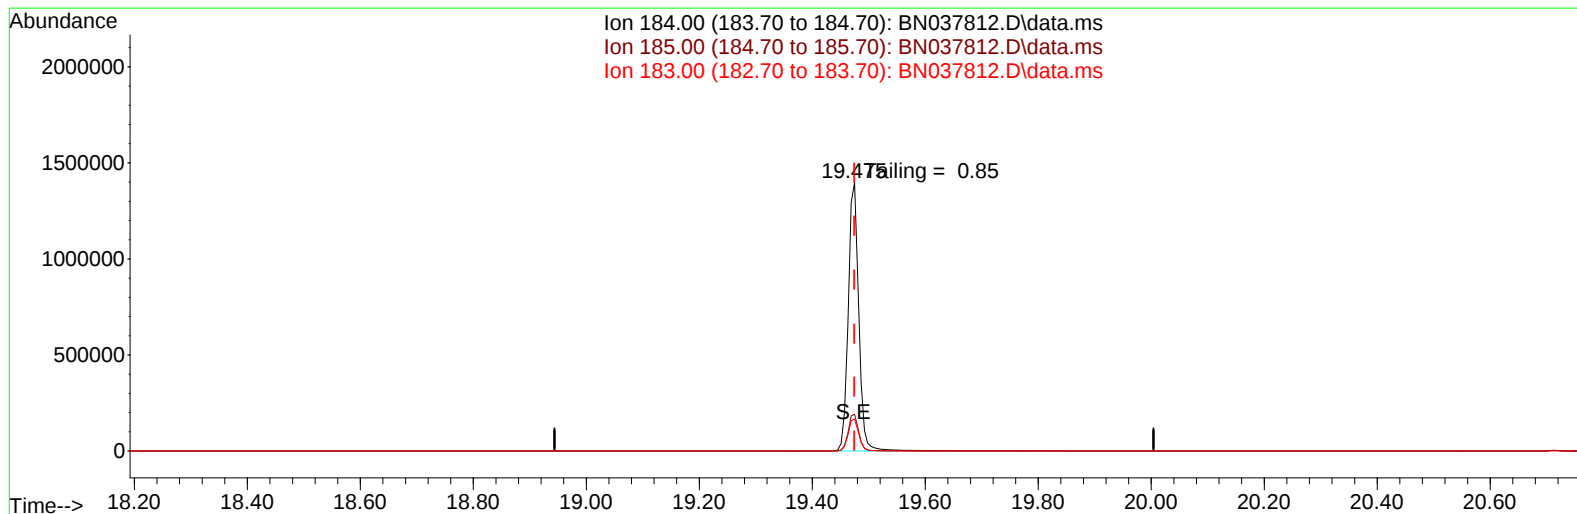

TIC: BN037812.D\data.ms

(77) Benzidine

19.475min (+ 0.001) 0.00 ng

response 1812303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2025	BNA_N	<u>BN037812.D</u>
Compound Name	Response	Retention Time
DDT	836771	20.716
DDD	28711	20.275
DDE	1832	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30543	867314	3.52

Instrument :
BNA_N
ClientSampleId :
DFTPP