
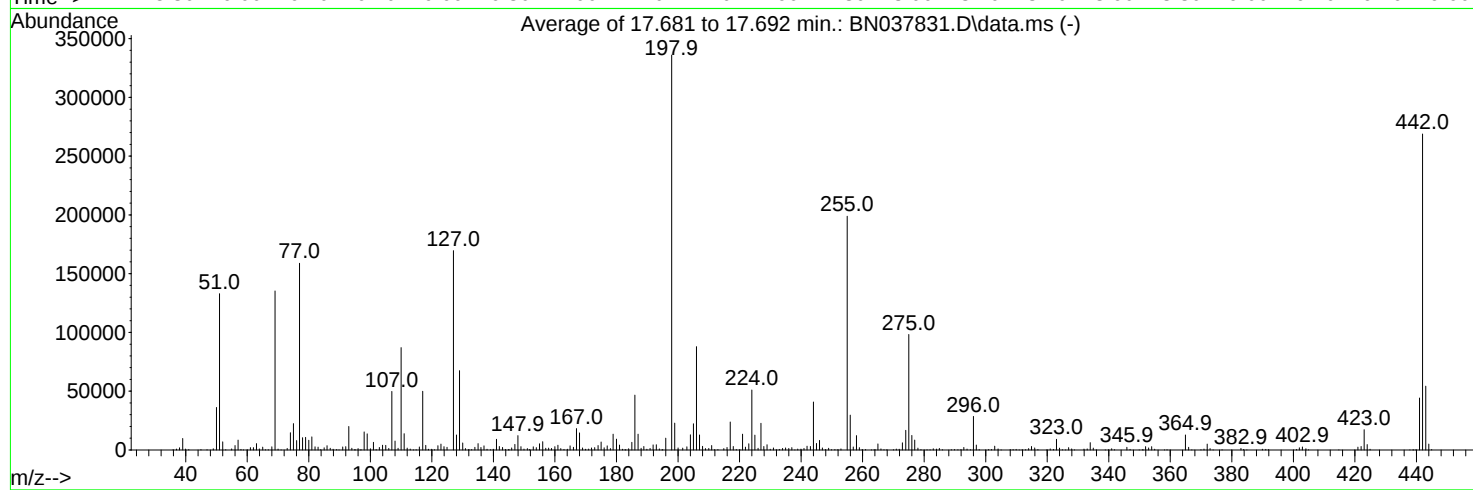


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037831.D
Acq On : 20 Sep 2025 01:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

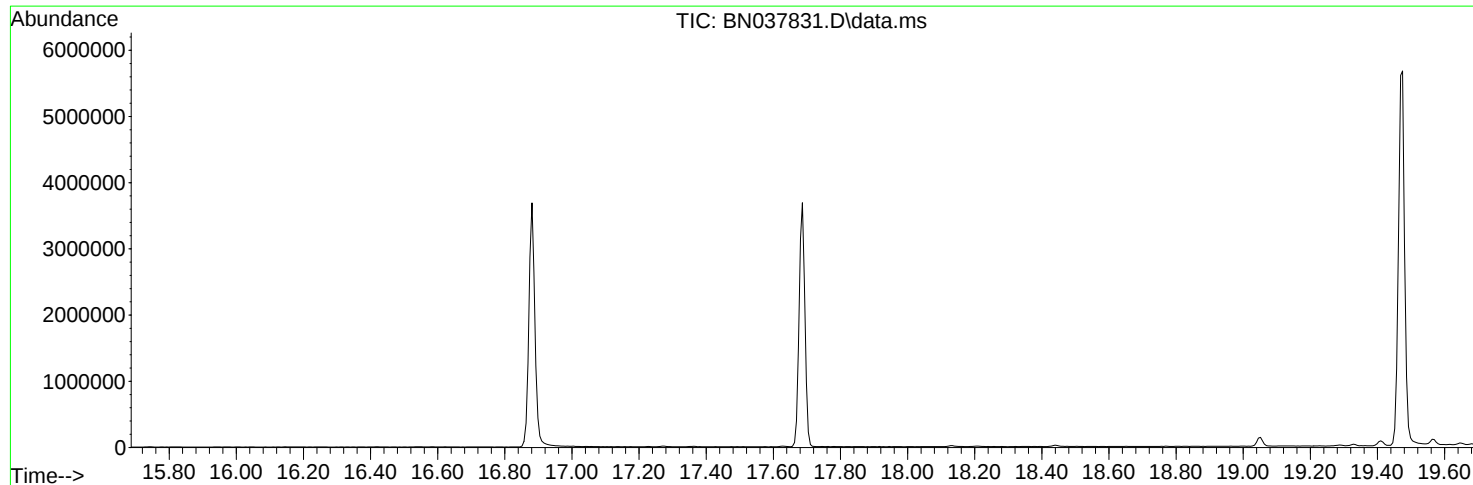




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	2623	PASS
69	69	100	100	100.0	135264	PASS
70	69	0.00	2	0.6	760	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	335979	PASS
199	198	5	9	6.8	22795	PASS
365	198	1	100	3.8	12691	PASS
441	443	0.01	150	81.3	44184	PASS
442	442	100	100	100.0	268907	PASS
443	442	15	24	20.2	54328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037831.D
Acq On : 20 Sep 2025 01:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 01:53:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

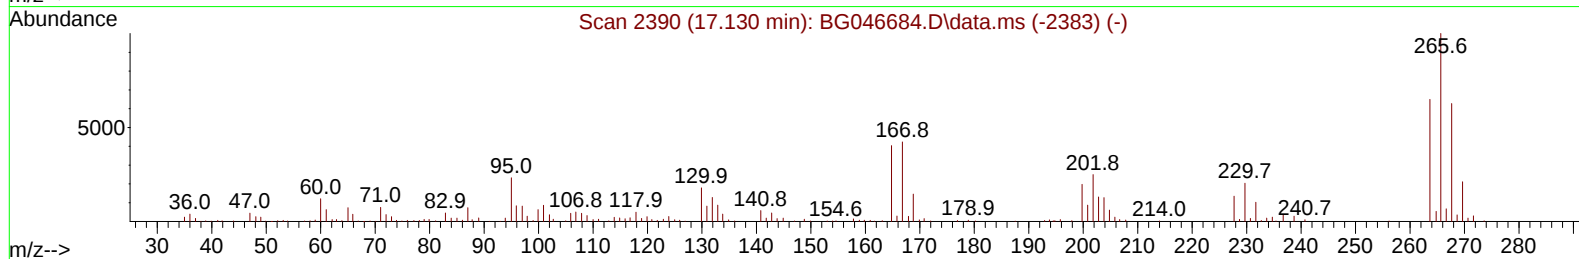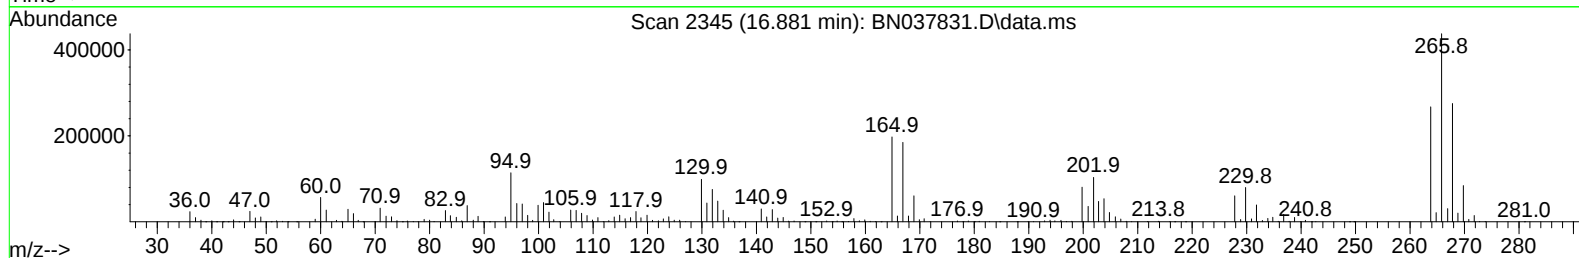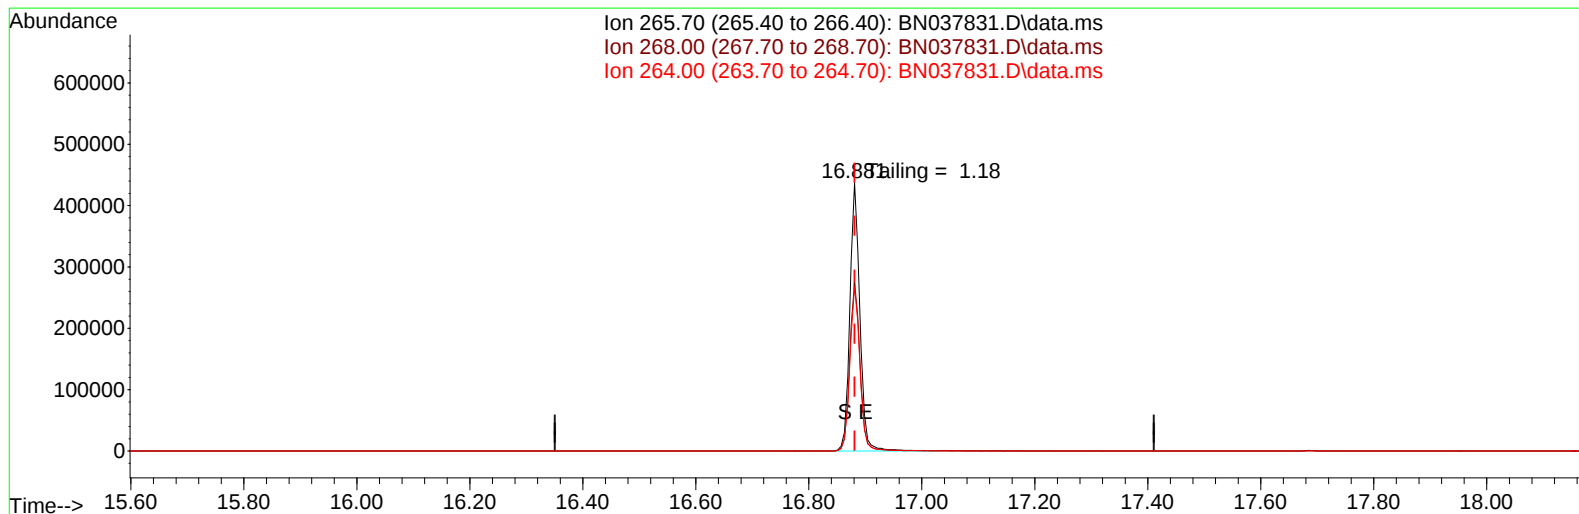

TIC: BN037831.D\data.ms

(70) Pentachlorophenol (C)

16.881min (0.000) 34698.10 ng




response 541064

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.87
264.00	61.60	61.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037831.D
Acq On : 20 Sep 2025 01:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 01:53:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

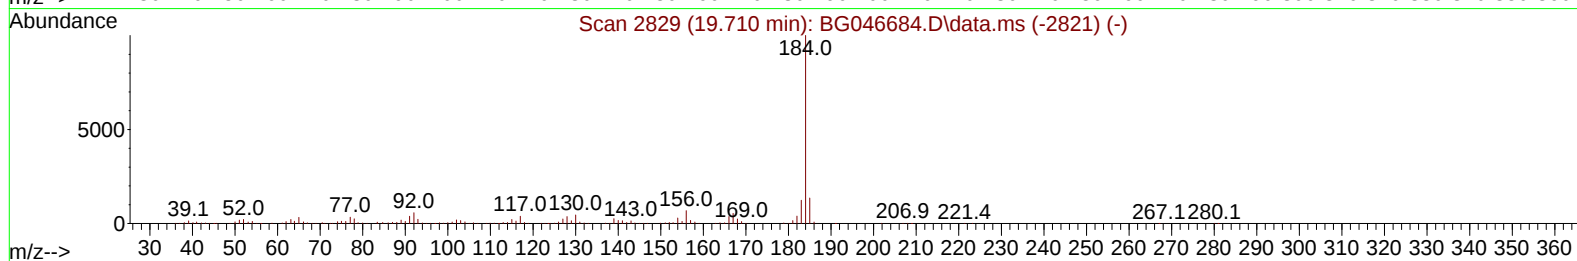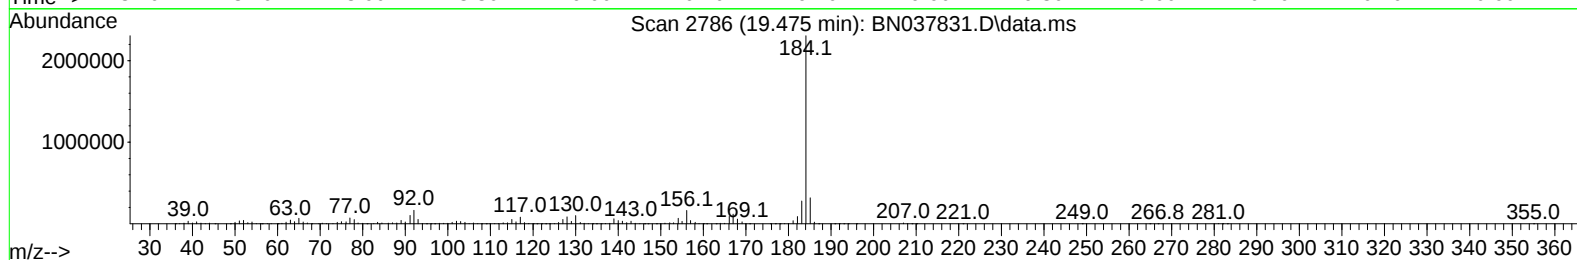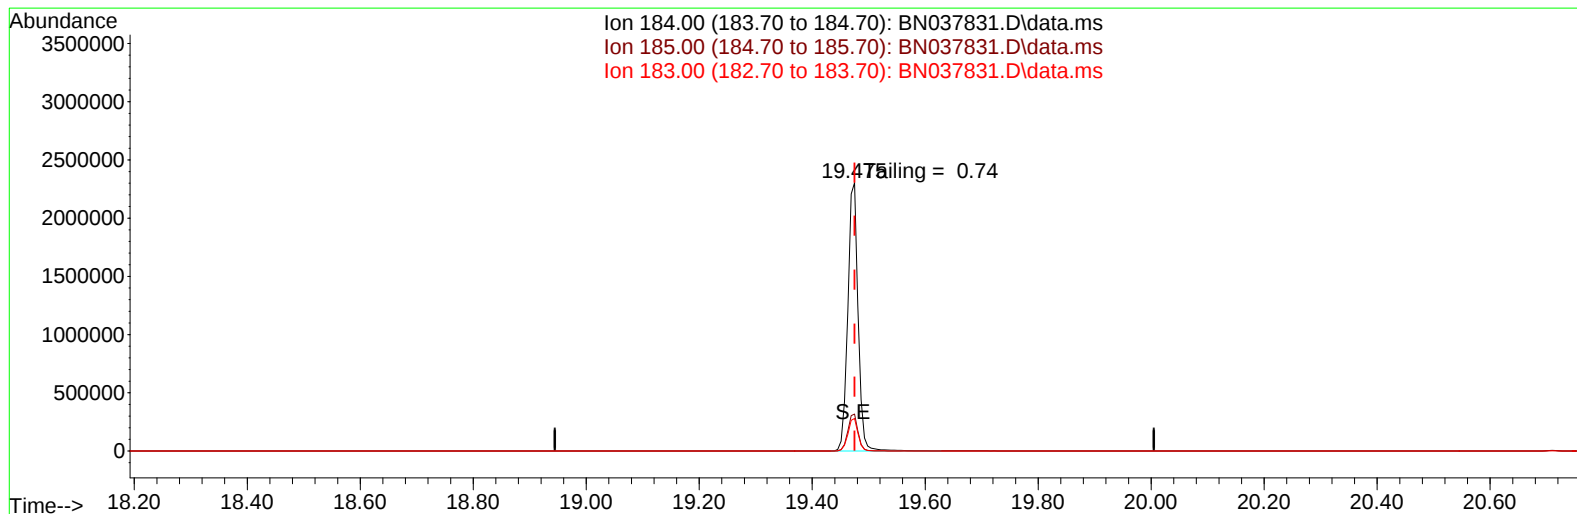

TIC: BN037831.D\data.ms

(77) Benzidine

19.475min (0.000) 0.00 ng

response 2907322

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.77
183.00	13.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2025	BNA_N	<u>BN037831.D</u>
Compound Name	Response	Retention Time
DDT	1283981	20.71
DDD	30254	20.269
DDE	1457	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31711	1315692	2.41

Instrument :
BNA_N
ClientSampleId :
DFTPP