
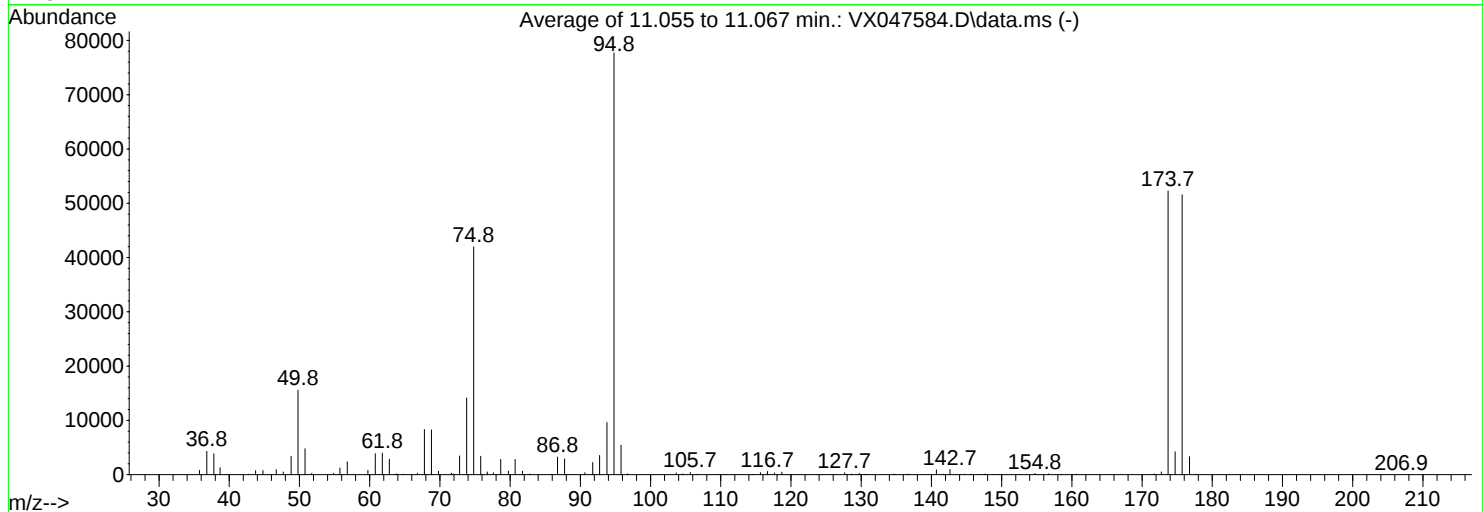


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091625\
Data File : VX047584.D
Acq On : 16 Sep 2025 08:56
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

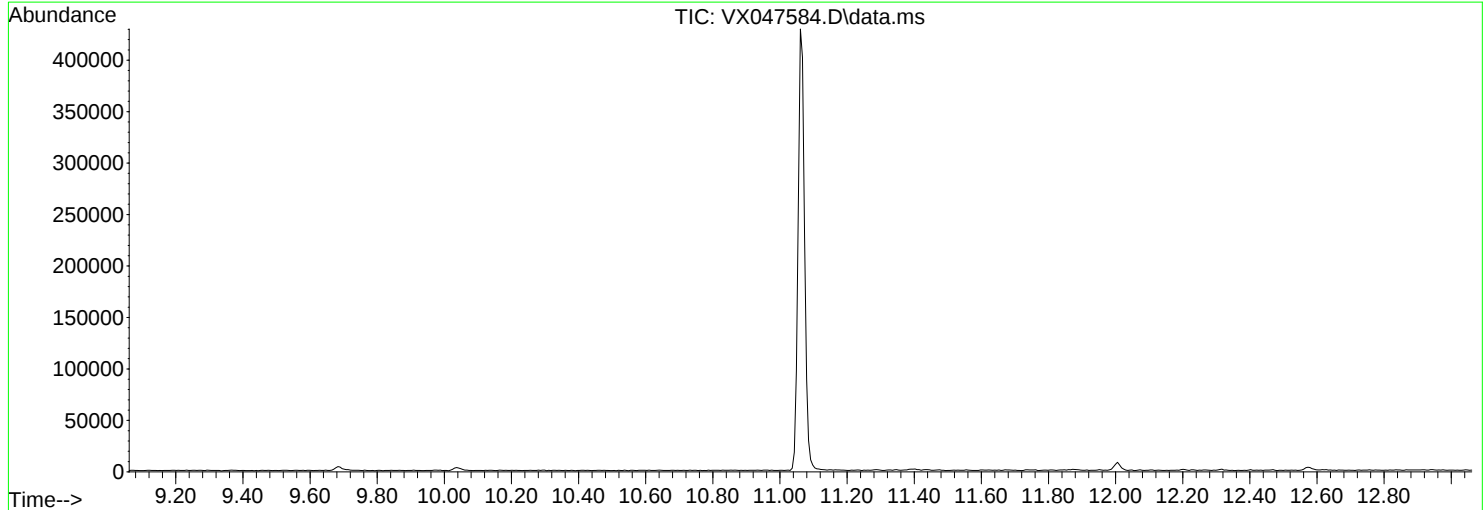

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	15566	PASS
75	95	30	60	54.0	41979	PASS
95	95	100	100	100.0	77717	PASS
96	95	5	9	7.0	5432	PASS
173	174	0.00	2	1.0	507	PASS
174	95	50	100	67.3	52275	PASS
175	174	5	9	8.1	4209	PASS
176	174	95	101	98.6	51560	PASS
177	176	5	9	6.4	3311	PASS