

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
 Data File : BN037820.D
 Acq On : 19 Sep 2025 18:34
 Operator : RC/JU
 Sample : Q3097-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20250912

Quant Time: Sep 19 23:55:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 14:20:01 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.833	152	4623	0.400 ng	0.00
7) Naphthalene-d8	10.637	136	12153	0.400 ng	-0.01
13) Acenaphthene-d10	14.484	164	5319	0.400 ng	-0.01
19) Phenanthrene-d10	17.235	188	10150	0.400 ng	# 0.00
29) Chrysene-d12	21.411	240	9405	0.400 ng	# 0.00
35) Perylene-d12	23.744	264	8969	0.400 ng	# 0.00
System Monitoring Compounds					
4) 2-Fluorophenol	5.399	112	1553	0.146 ng	0.00
5) Phenol-d6	6.980	99	986	0.072 ng	0.00
8) Nitrobenzene-d5	8.982	82	2786	0.313 ng	-0.01
11) 2-Methylnaphthalene-d10	12.227	152	4358	0.271 ng	-0.02
14) 2,4,6-Tribromophenol	15.982	330	573	0.413 ng	0.00
15) 2-Fluorobiphenyl	13.105	172	6855	0.308 ng	-0.01
27) Fluoranthene-d10	19.262	212	9689	0.380 ng	0.00
31) Terphenyl-d14	19.861	244	7908	0.414 ng	0.00
Target Compounds					
2) 1,4-Dioxane	3.297	88	5022	1.043 ng	94
34) Bis(2-ethylhexyl)phtha...	21.331	149	1373	0.141 ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037820.D
Acq On : 19 Sep 2025 18:34
Operator : RC/JU
Sample : Q3097-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912


Quant Time: Sep 19 23:55:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 14:20:01 2025
Response via : Initial Calibration

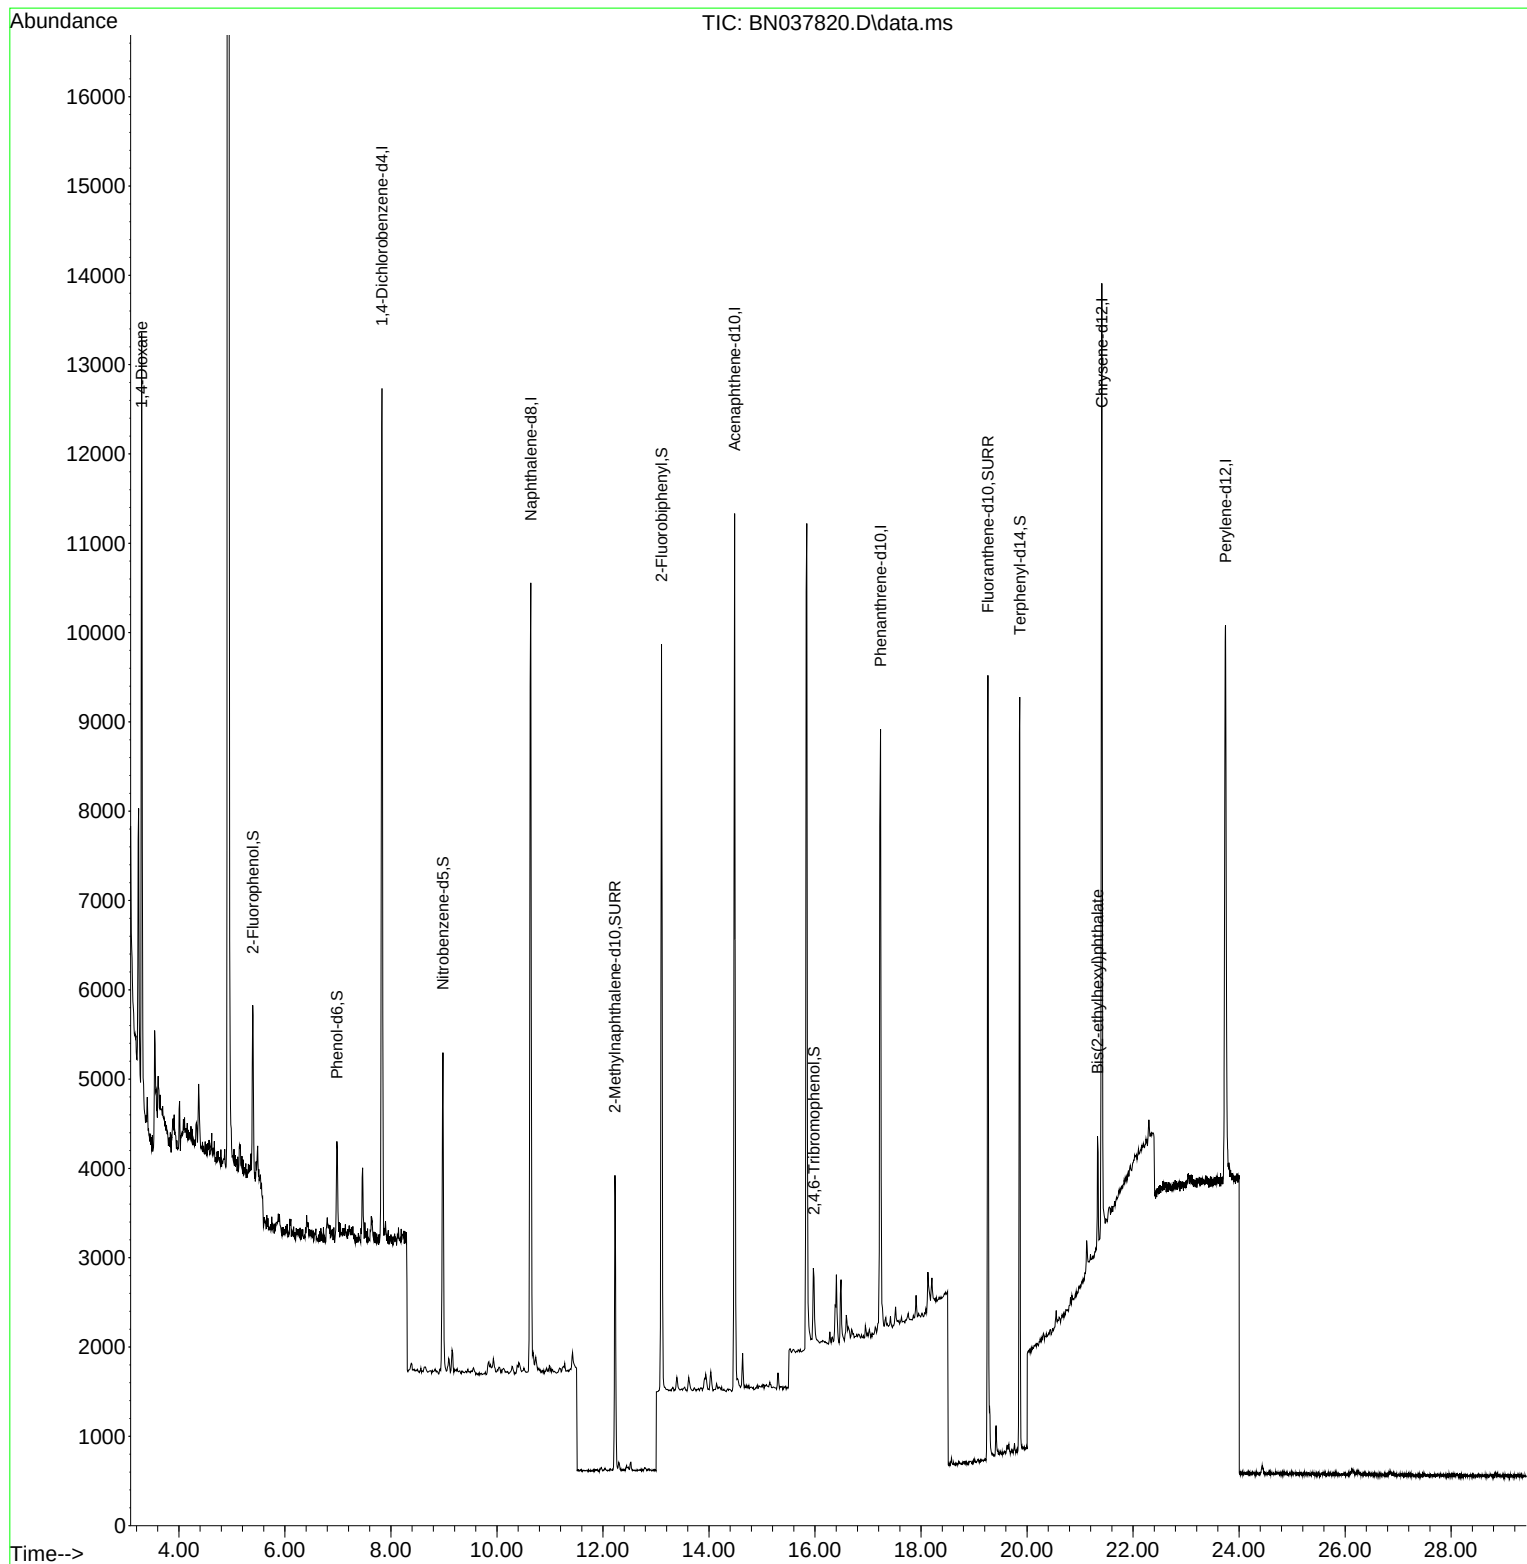






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.833 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34

Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912



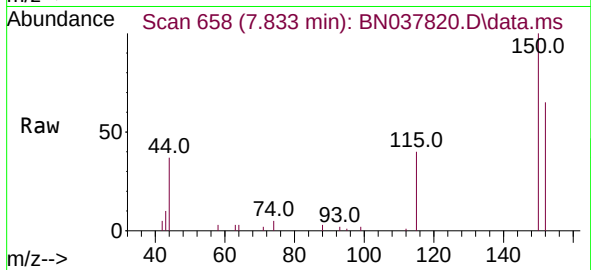



Tgt Ion:152 Resp: 4623
Ion Ratio Lower Upper
152 100
150 153.5 124.5 186.7
115 61.1 49.2 73.8

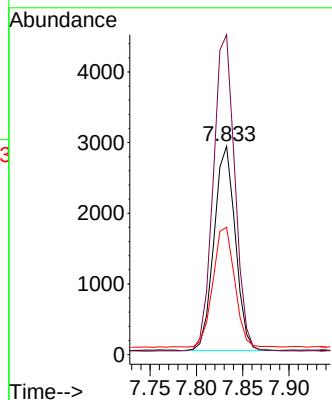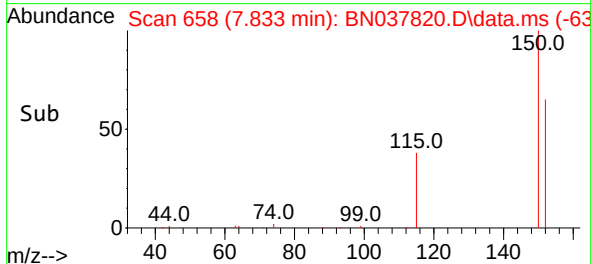

#2
1,4-Dioxane
Concen: 1.043 ng
RT: 3.297 min Scan# 30
Delta R.T. -0.007 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34

Tgt Ion: 88 Resp: 5022
Ion Ratio Lower Upper
88 100
43 39.4 26.8 40.2
58 74.2 61.9 92.9


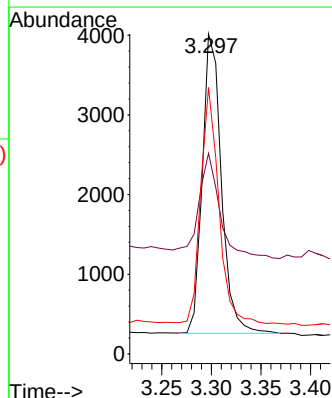

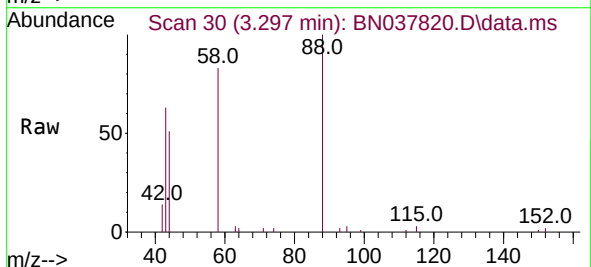




#4
2-Fluorophenol
Concen: 0.146 ng
RT: 5.399 min Scan# 31
Delta R.T. -0.000 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34




Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912


Tgt Ion:112 Resp: 1553
Ion Ratio Lower Upper
112 100
64 57.4 44.9 67.3
63 30.8 24.7 37.1

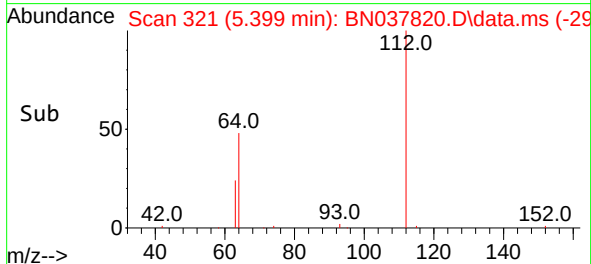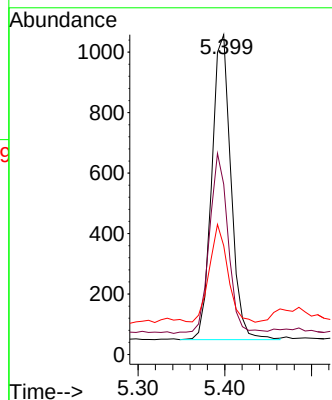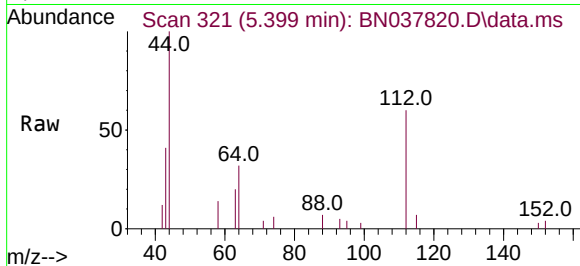

#5
Phenol-d6
Concen: 0.072 ng
RT: 6.980 min Scan# 540
Delta R.T. -0.007 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34

Tgt Ion: 99 Resp: 986
Ion Ratio Lower Upper
99 100
42 22.8 16.6 24.8
71 38.7 26.7 40.1


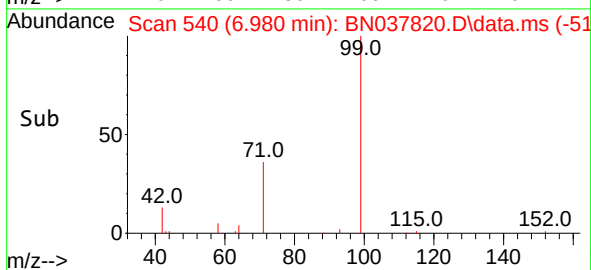
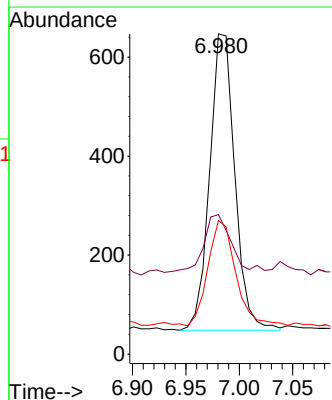
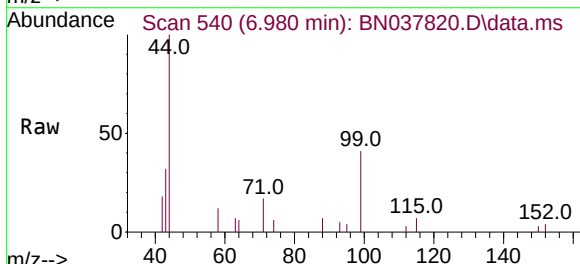




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.637 min Scan# 94
Delta R.T. -0.011 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34




Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912


Tgt Ion:	136	Resp:	12153
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.1	13.7
54	6.7	6.3	9.5
68	5.2	5.0	7.4

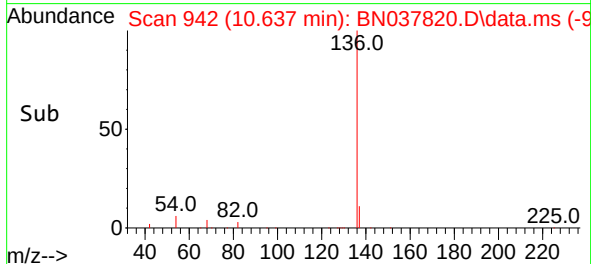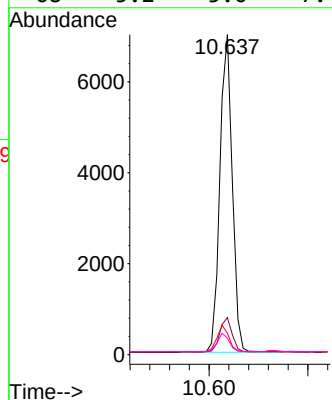

#8
Nitrobenzene-d5
Concen: 0.313 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34

Tgt Ion:	82	Resp:	2786
Ion	Ratio	Lower	Upper
82	100		
128	47.0	38.3	57.5
54	49.8	41.4	62.2


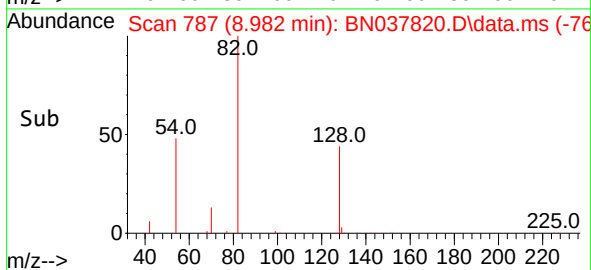
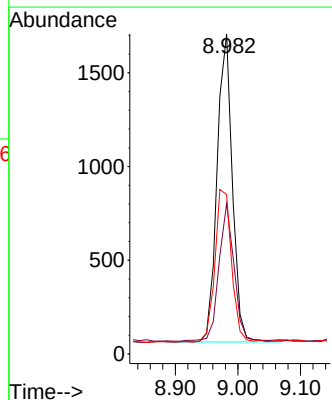
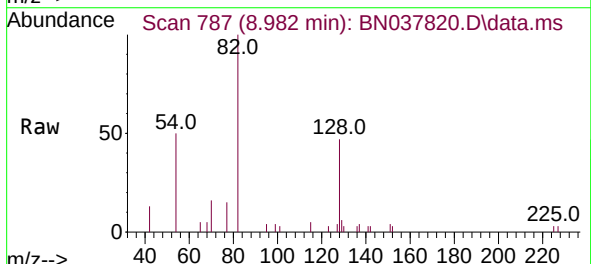




#11
2-Methylnaphthalene-d10
Concen: 0.271 ng
RT: 12.227 min Scan# 1165
Delta R.T. -0.015 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34




Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912


Tgt Ion:152 Resp: 4358
Ion Ratio Lower Upper
152 100
151 21.4 17.0 25.6

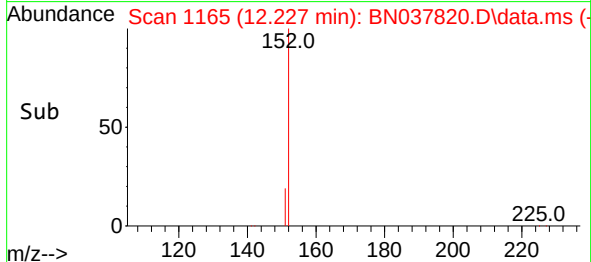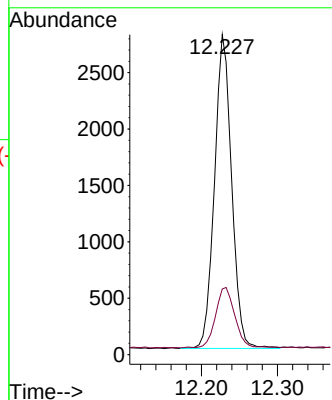

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.484 min Scan# 1457
Delta R.T. -0.011 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34


Tgt Ion:164 Resp: 5319
Ion Ratio Lower Upper
164 100
162 105.3 83.1 124.7
160 56.1 44.3 66.5

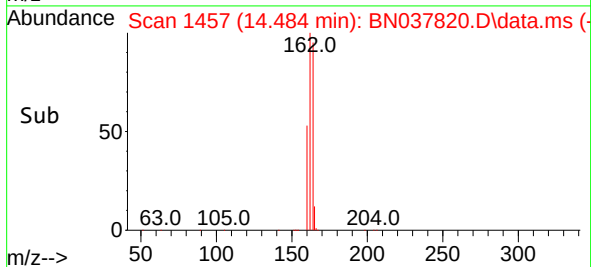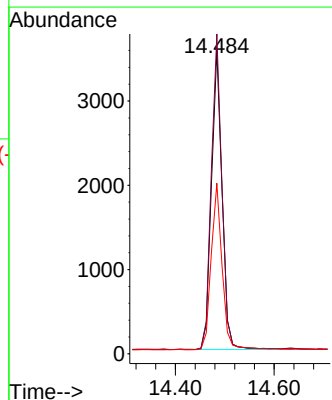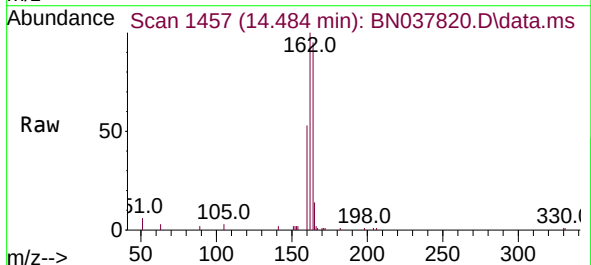






#14
2,4,6-Tribromophenol
Concen: 0.413 ng
RT: 15.982 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34


Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912





Tgt Ion:330 Resp: 573
Ion Ratio Lower Upper
330 100
332 100.0 75.3 112.9
141 45.2 35.0 52.4

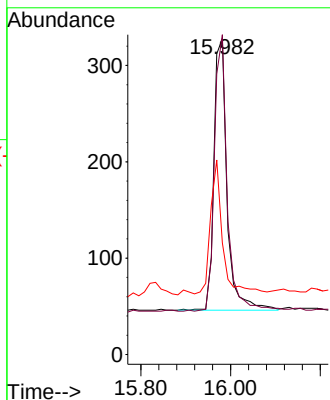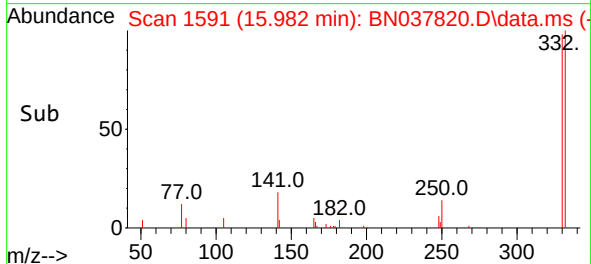


#15
2-Fluorobiphenyl
Concen: 0.308 ng
RT: 13.105 min Scan# 1328
Delta R.T. -0.011 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34

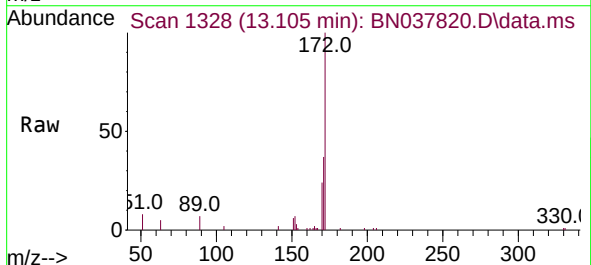

Tgt Ion:172 Resp: 6855
Ion Ratio Lower Upper
172 100
171 36.6 28.6 43.0
170 24.1 19.8 29.8



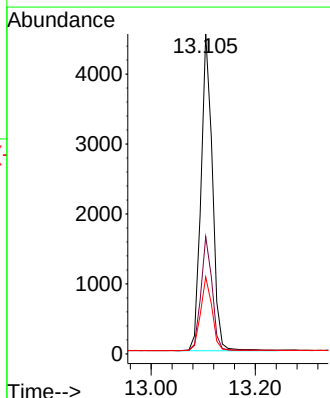
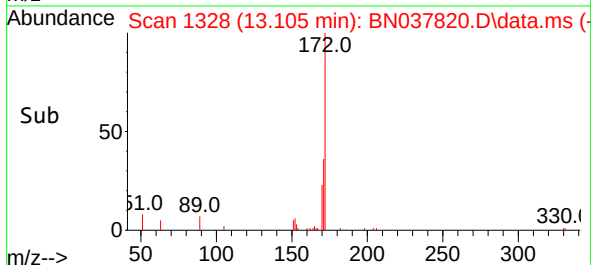




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.235 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34




Instrument :
BNA_N
ClientSampleId :
RE134D1-20250912


Tgt Ion:188 Resp: 10150
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.3 10.6 15.8#

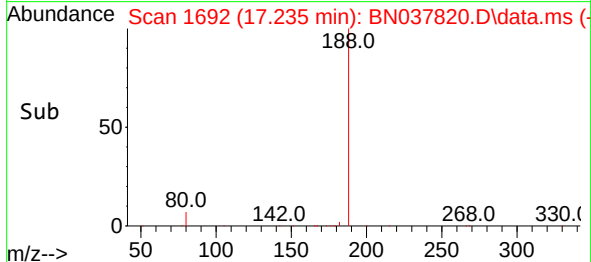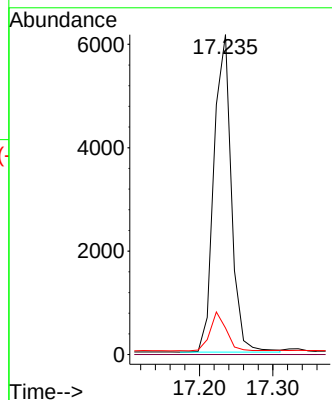

#27
Fluoranthene-d10
Concen: 0.380 ng
RT: 19.262 min Scan# 1956
Delta R.T. -0.009 min
Lab File: BN037820.D
Acq: 19 Sep 2025 18:34

Tgt Ion:212 Resp: 9689
Ion Ratio Lower Upper
212 100
106 16.1 12.2 18.2
104 9.5 6.9 10.3

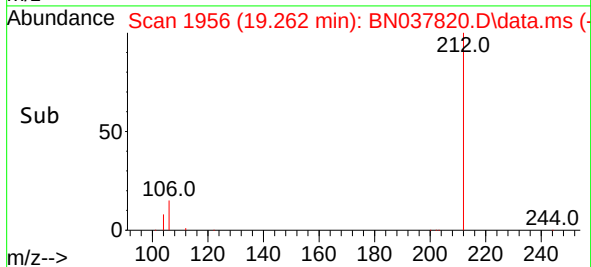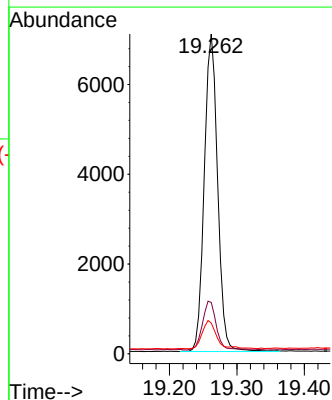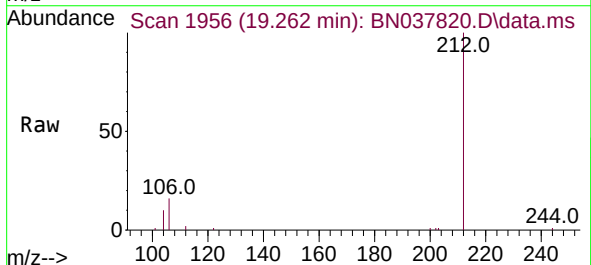



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.411 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN037820.D

Acq: 19 Sep 2025 18:34

Instrument :

BNA_N

ClientSampleId :

RE134D1-20250912





Tgt Ion:240 Resp: 9405

Ion Ratio Lower Upper

240 100

120 14.0 9.2 13.8#

236 28.7 22.6 33.8

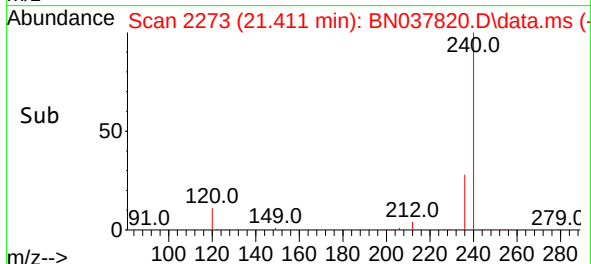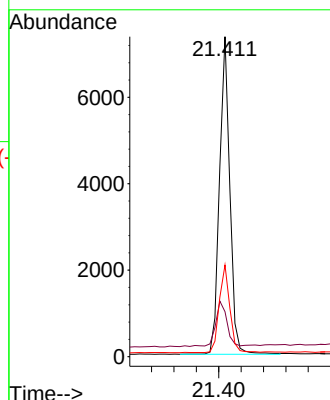

#31

Terphenyl-d14

Concen: 0.414 ng

RT: 19.861 min Scan# 2085

Delta R.T. -0.009 min

Lab File: BN037820.D

Acq: 19 Sep 2025 18:34




Tgt Ion:244 Resp: 7908


Ion Ratio Lower Upper

244 100

212 9.8 7.5 11.3

122 16.1 13.2 19.8

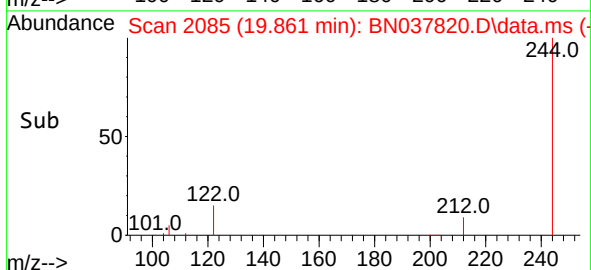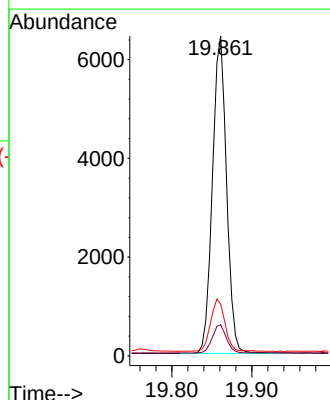




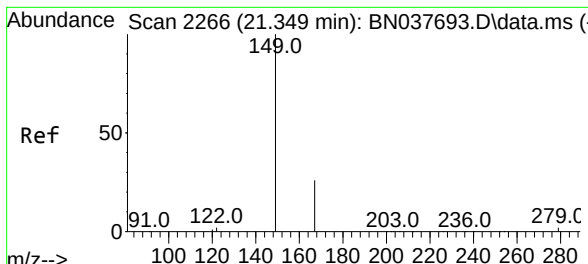


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.141 ng
 RT: 21.331 min Scan# 21
 Delta R.T. -0.018 min
 Lab File: BN037820.D
 Acq: 19 Sep 2025 18:34

Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20250912

Tgt Ion:149 Resp: 1373

Ion	Ratio	Lower	Upper
149	100		
167	25.7	20.8	31.2
279	4.9	3.3	4.9

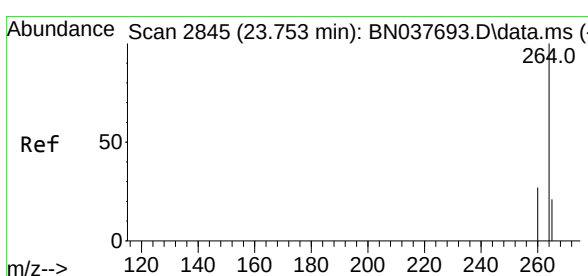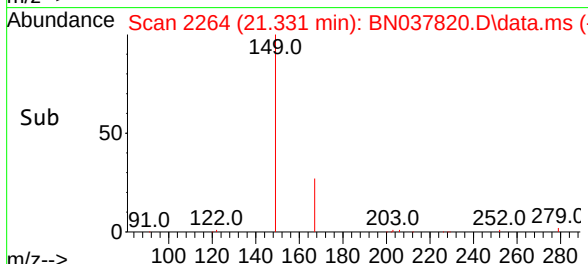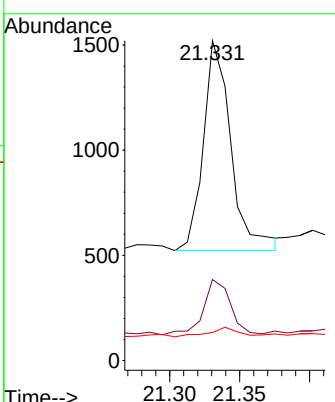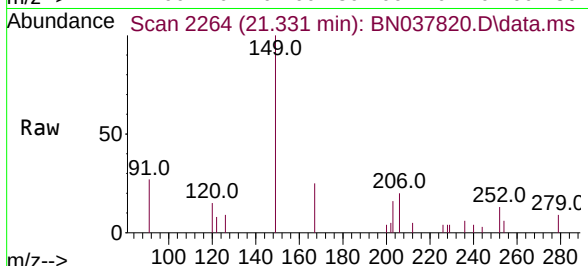

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.744 min Scan# 2842
 Delta R.T. -0.009 min
 Lab File: BN037820.D
 Acq: 19 Sep 2025 18:34

Tgt Ion:264 Resp: 8969

Ion	Ratio	Lower	Upper
264	100		
260	26.5	21.8	32.8
265	77.2	39.4	59.2

