


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092225\
Data File : VX047688.D
Acq On : 22 Sep 2025 09:07
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

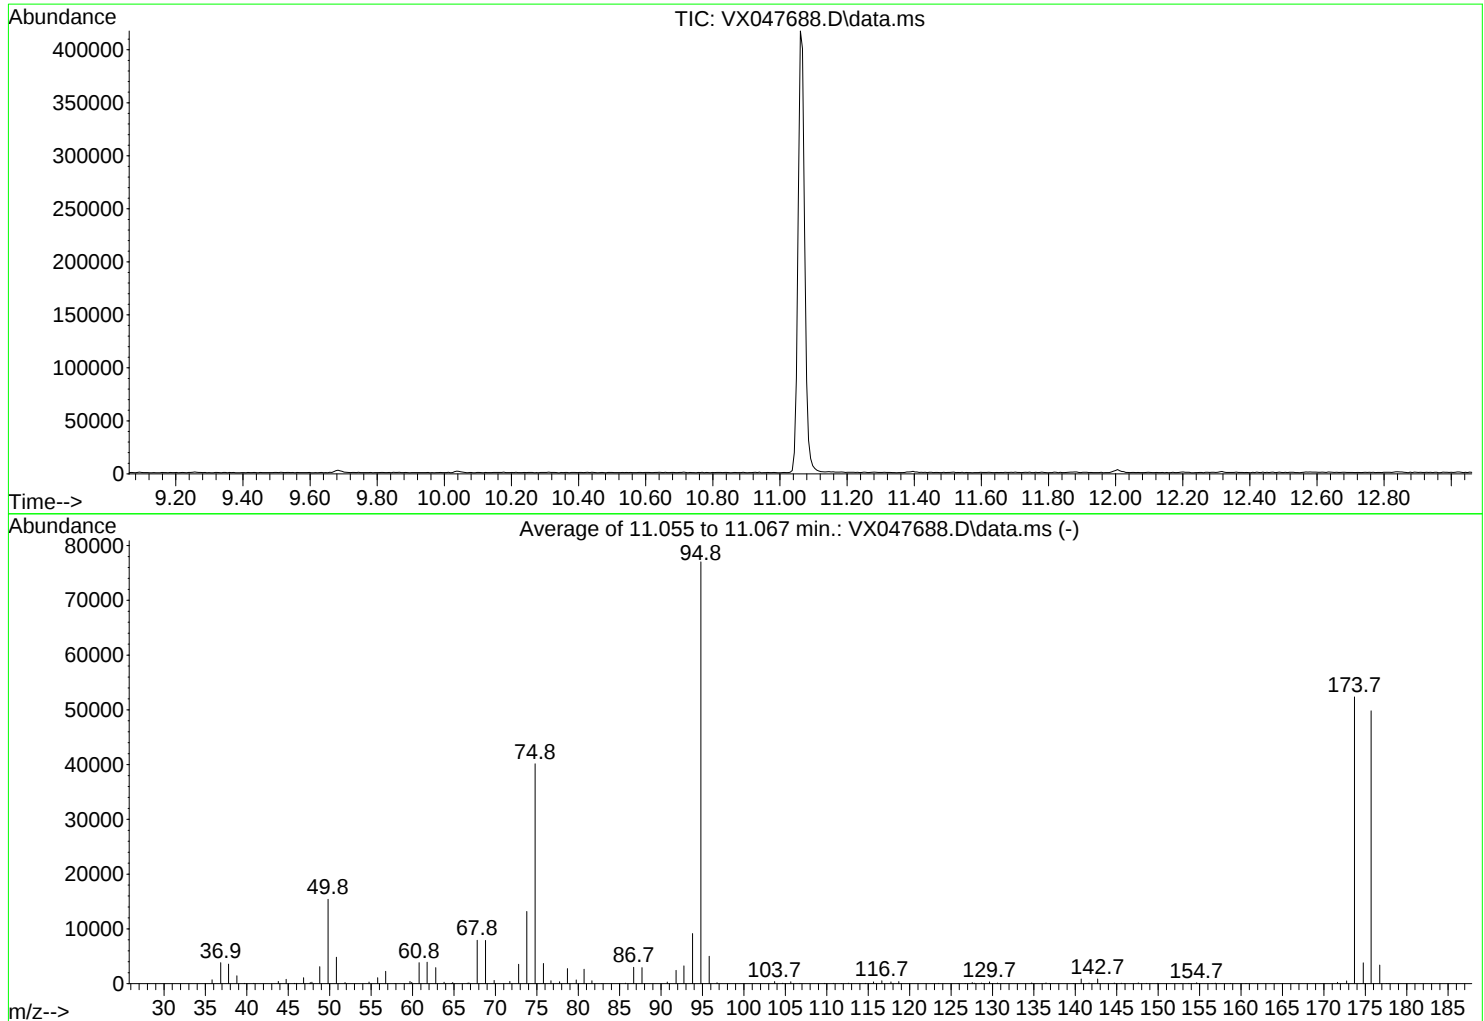

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1628

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	15414	PASS
75	95	30	60	52.1	40141	PASS
95	95	100	100	100.0	77029	PASS
96	95	5	9	6.5	4992	PASS
173	174	0.00	2	0.9	486	PASS
174	95	50	100	68.0	52360	PASS
175	174	5	9	7.2	3790	PASS
176	174	95	101	95.1	49808	PASS
177	176	5	9	6.8	3382	PASS