



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091725\
Data File : VN087868.D
Acq On : 17 Sep 2025 08:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090425W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 05 03:29:53 2025

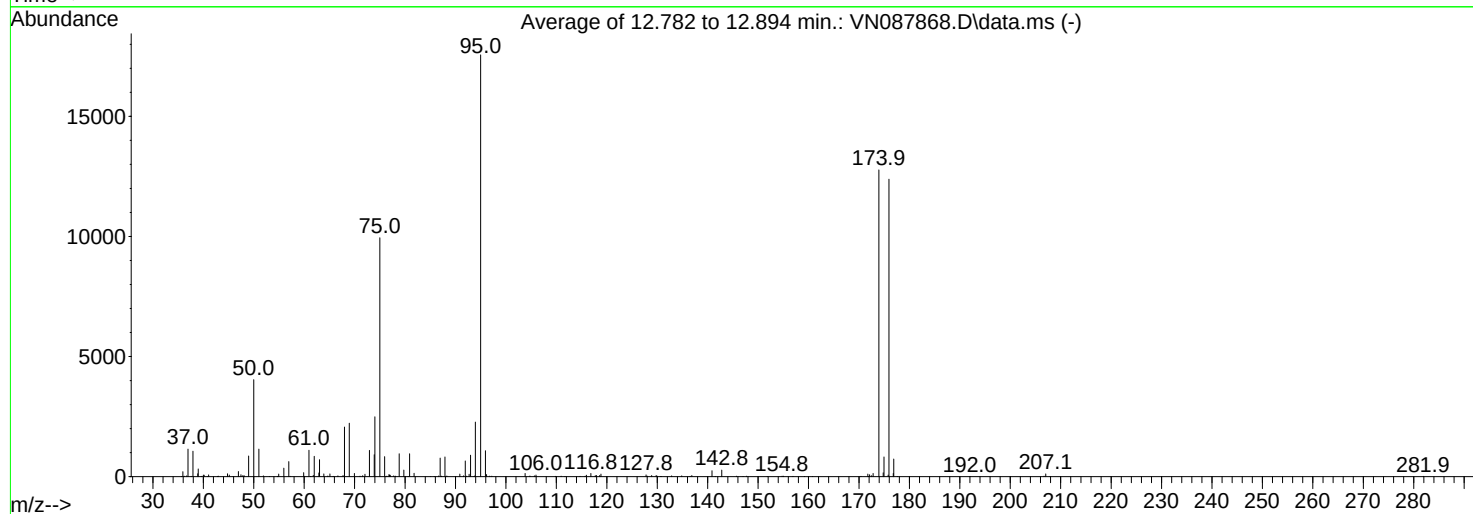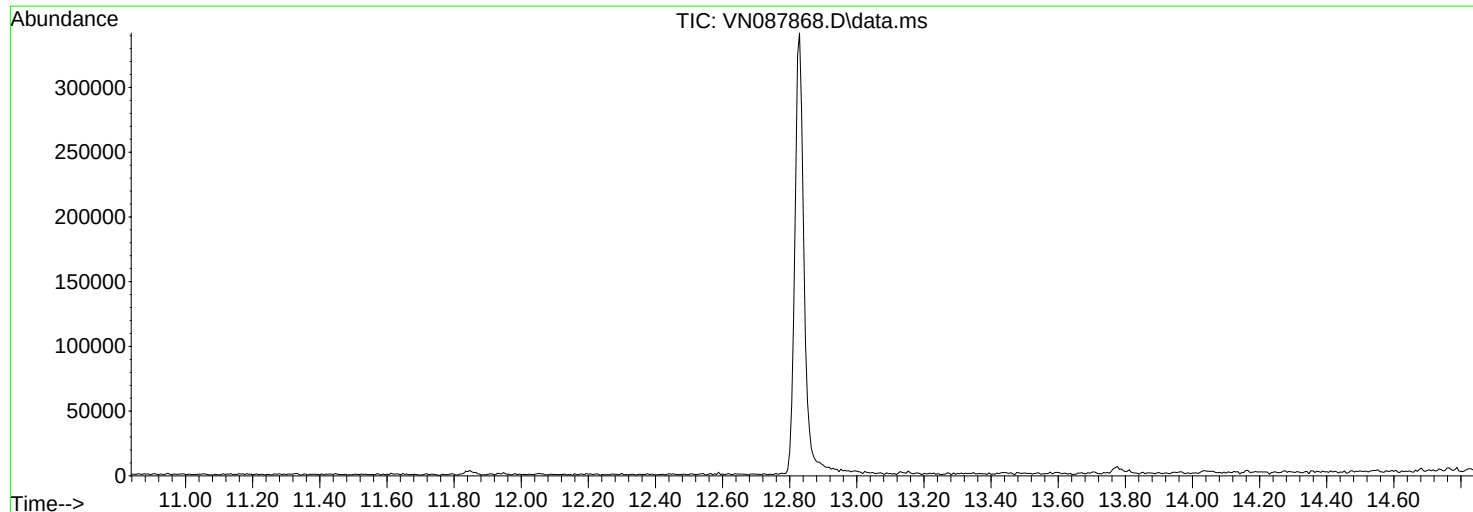

AutoFind: Averaged scan 1841 to 1860; Bkg corrected with scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.0	4036	PASS
75	95	30	60	56.6	9947	PASS
95	95	100	100	100.0	17560	PASS
96	95	5	9	6.1	1076	PASS
173	174	0.00	2	1.1	135	PASS
174	95	50	100	72.7	12770	PASS
175	174	5	9	6.4	820	PASS
176	174	95	101	97.0	12386	PASS
177	176	5	9	5.9	730	PASS