

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091625\
 Data File : P0113779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2025 21:05
 Operator : YP/AJ
 Sample : Q3099-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 15A15B15C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/17/2025
 Supervised By :mohammad ahmed 09/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:14:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.650	172.6E6	102.2E6	19.570	19.133
2) SA Decachlor...	8.668	8.616	82230960	26237698	12.291m	12.567m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091625\
Data File : PO113779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 21:05
Operator : YP/AJ
Sample : Q3099-10
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
15A15B15C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2025
Supervised By :mohammad ahmed 09/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:14:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

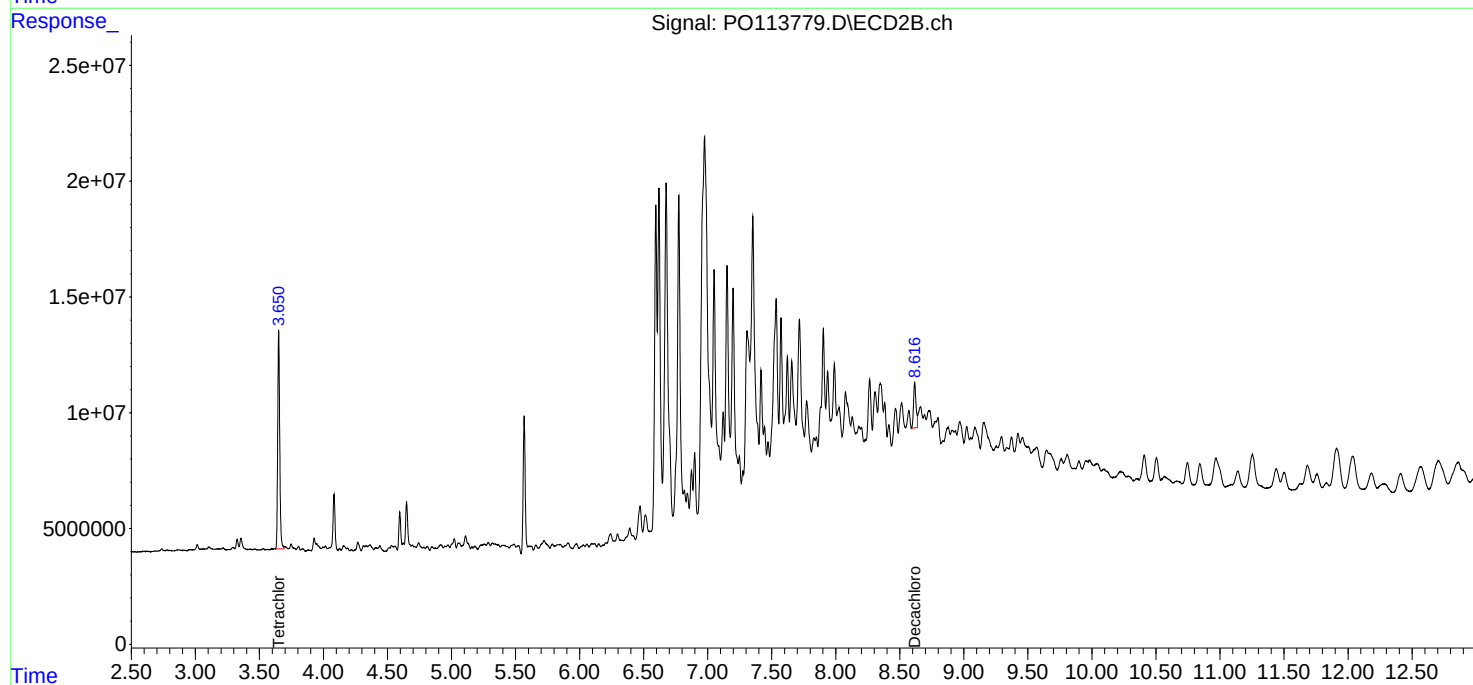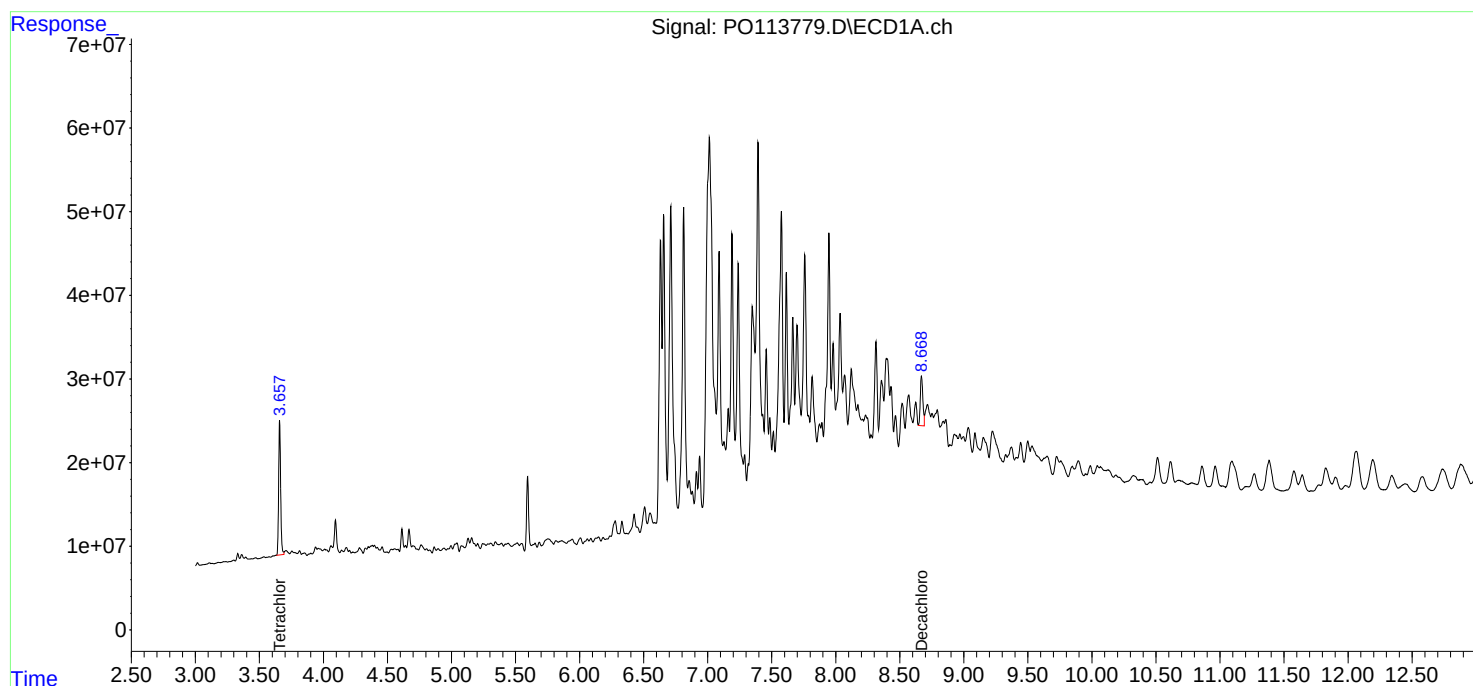

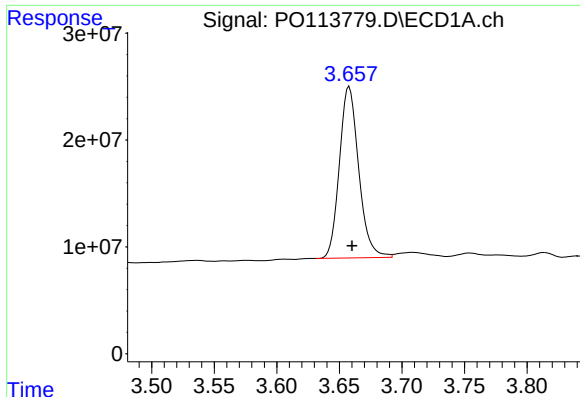


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.002 min
Response: 172603742
Conc: 19.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
15A15B15C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2025
Supervised By :mohammad ahmed 09/19/2025

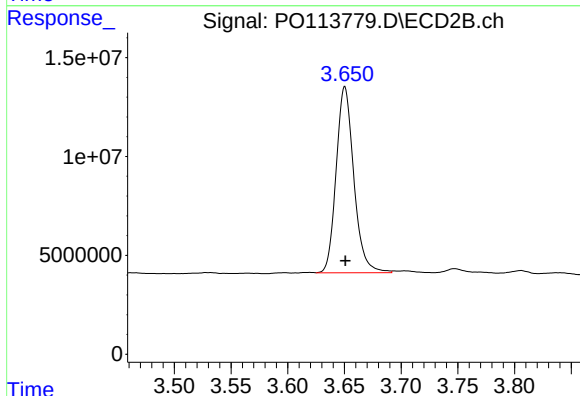


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 102188095
Conc: 19.13 ng/ml

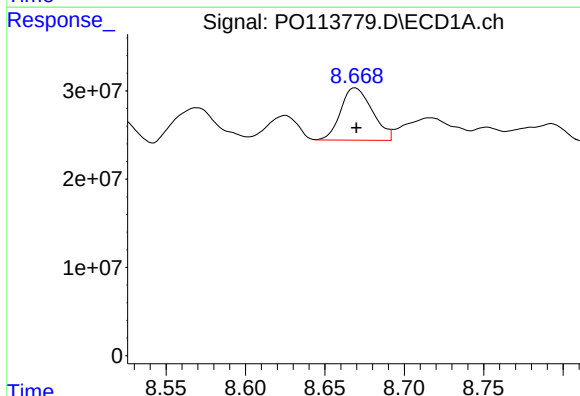

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.001 min
Response: 82230960
Conc: 12.29 ng/ml m

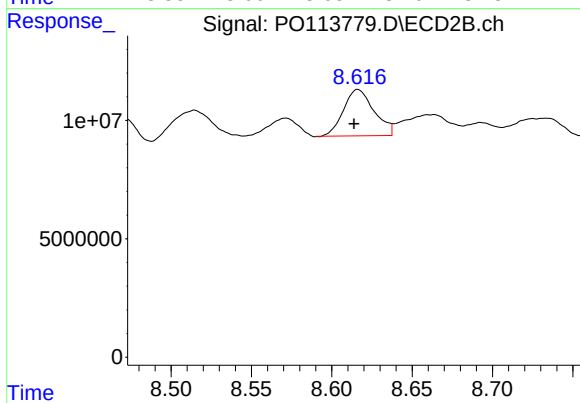

#2 Decachlorobiphenyl

R.T.: 8.616 min
Delta R.T.: 0.002 min
Response: 26237698
Conc: 12.57 ng/ml m