

LB137213 INSTRUMENT ID: CV1


Method: 7470A Operator: Admin Date of Analysis: 17 Sep 2025 13:56:20

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50	-	19	PPB	Std	0.0000	7470A	17 Sep 2025 13:57:46
S	0.2 - 1	50.2	-	740	PPB	Std	0.2000	7470A	17 Sep 2025 14:00:03
S	2.5 - 1	52.5	-	9931	PPB	Std	2.5000	7470A	17 Sep 2025 14:02:20
S	5.0 - 1	55.0	-	20028	PPB	Std	5.0000	7470A	17 Sep 2025 14:04:37
S	7.5 - 1	57.5	-	29255	PPB	Std	7.5000	7470A	17 Sep 2025 14:06:56
S	10.0 - 1	510.0	-	39856	PPB	Std	10.0000	7470A	17 Sep 2025 14:18:36
U	ICV34 - 1	ICV34	4.2787	16950	PPB	SMPL	-7470A		17 Sep 2025 14:21:36
U	ICB34 - 1	ICB34	-0.0222	-100	PPB	SMPL	-7470A		17 Sep 2025 14:23:53
U	CCV07 - 1	CCV07	4.9577	19642	PPB	SMPL	-7470A		17 Sep 2025 14:26:11
U	CCB07 - 1	CCB07	-0.0285	-125	PPB	SMPL	-7470A		17 Sep 2025 14:28:26
U	CRA - 1	CRA	0.1920	749	PPB	SMPL	-7470A		17 Sep 2025 14:30:45
U	HighStd - 1	HighStd	9.8672	39105	PPB	SMPL	-7470A		17 Sep 2025 14:33:00
U	ChkStd - 1	ChkStd	7.3009	28931	PPB	SMPL	-7470A		17 Sep 2025 14:35:16
U	PB169732BL - 1	PBW	-0.0449	-190	PPB	SMPL	-7470A		17 Sep 2025 14:37:36
U	PB169732BS - 1	LCSW	4.3266	17140	PPB	SMPL	-7470A		17 Sep 2025 14:39:55
U	Q3103-01 - 1	TW-WTS-14	-0.0184	-85	PPB	SMPL	-7470A		17 Sep 2025 14:42:11
U	Q3103-01DUP - 1	TW-WTS-14DUP	0.0116	34	PPB	SMPL	-7470A		17 Sep 2025 14:46:11
U	Q3103-01MS - 1	TW-WTS-14MS	3.4389	13621	PPB	SMPL	-7470A		17 Sep 2025 14:48:27
U	Q3103-01MSD - 1	TW-WTS-14MSD	3.8087	15087	PPB	SMPL	-7470A		17 Sep 2025 14:50:44
U	Q3113-01 - 1	TRE-25-0101	0.2028	792	PPB	SMPL	-7470A		17 Sep 2025 14:53:02
U	CCV08 - 1	CCV08	4.7292	18736	PPB	SMPL	-7470A		17 Sep 2025 14:55:20
U	CCB08 - 1	CCB08	0.0015	-6	PPB	SMPL	-7470A		17 Sep 2025 14:57:37
U	Q3103-01LX5 - 1		0.0356	129	PPB	SMPL	-7470A		17 Sep 2025 14:59:55
U	Q3103-01A - 1		4.1490	16436	PPB	SMPL	-7470A		17 Sep 2025 15:02:10
U	CCV09 - 1	CCV09	4.8941	19390	PPB	SMPL	-7470A		17 Sep 2025 15:04:25
U	CCB09 - 1	CCB09	-0.0371	-159	PPB	SMPL	-7470A		17 Sep 2025 15:06:44

LB137213
INSTRUMENT ID: CV1

Reviewed By: jaswal
On: 9/18/2025 9:40:45 AM
Inst Id: CV1
LB: LB137213

7470A

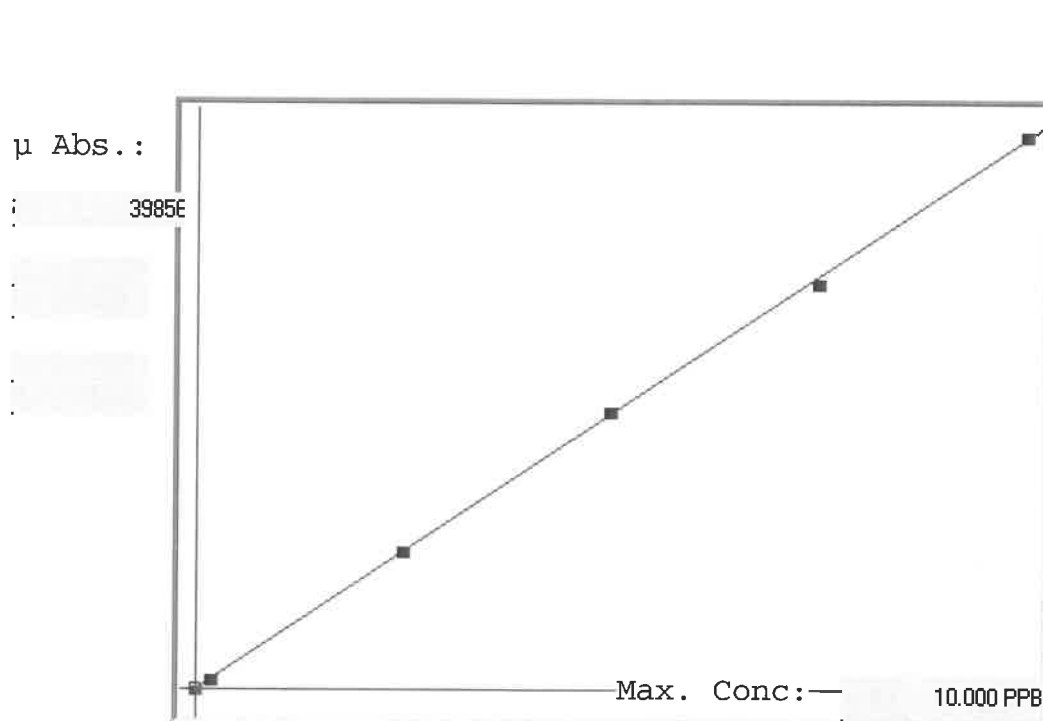

Linear

A= 0.0000e+000

B= 2.5225e-004

C= 3.0420e-003

Rho= 0.9998760

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	0.008	0.008	19	0.000	19	0				-5
0.2	0.200	0.190	-0.010	740	0.0 %	740	0				0
2.5	2.500	2.508	0.008	9931	0.0 %	9931	0				+1
5.0	5.000	5.055	0.055	20028	0.0 %	20028					-2
7.5	7.500	7.383	-0.117	29255	0.0 %	29255					1
10.0	10.000	10.057	0.057	39856	0.0 %	39856					