


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091925\
Data File : BP025791.D
Acq On : 19 Sep 2025 09:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

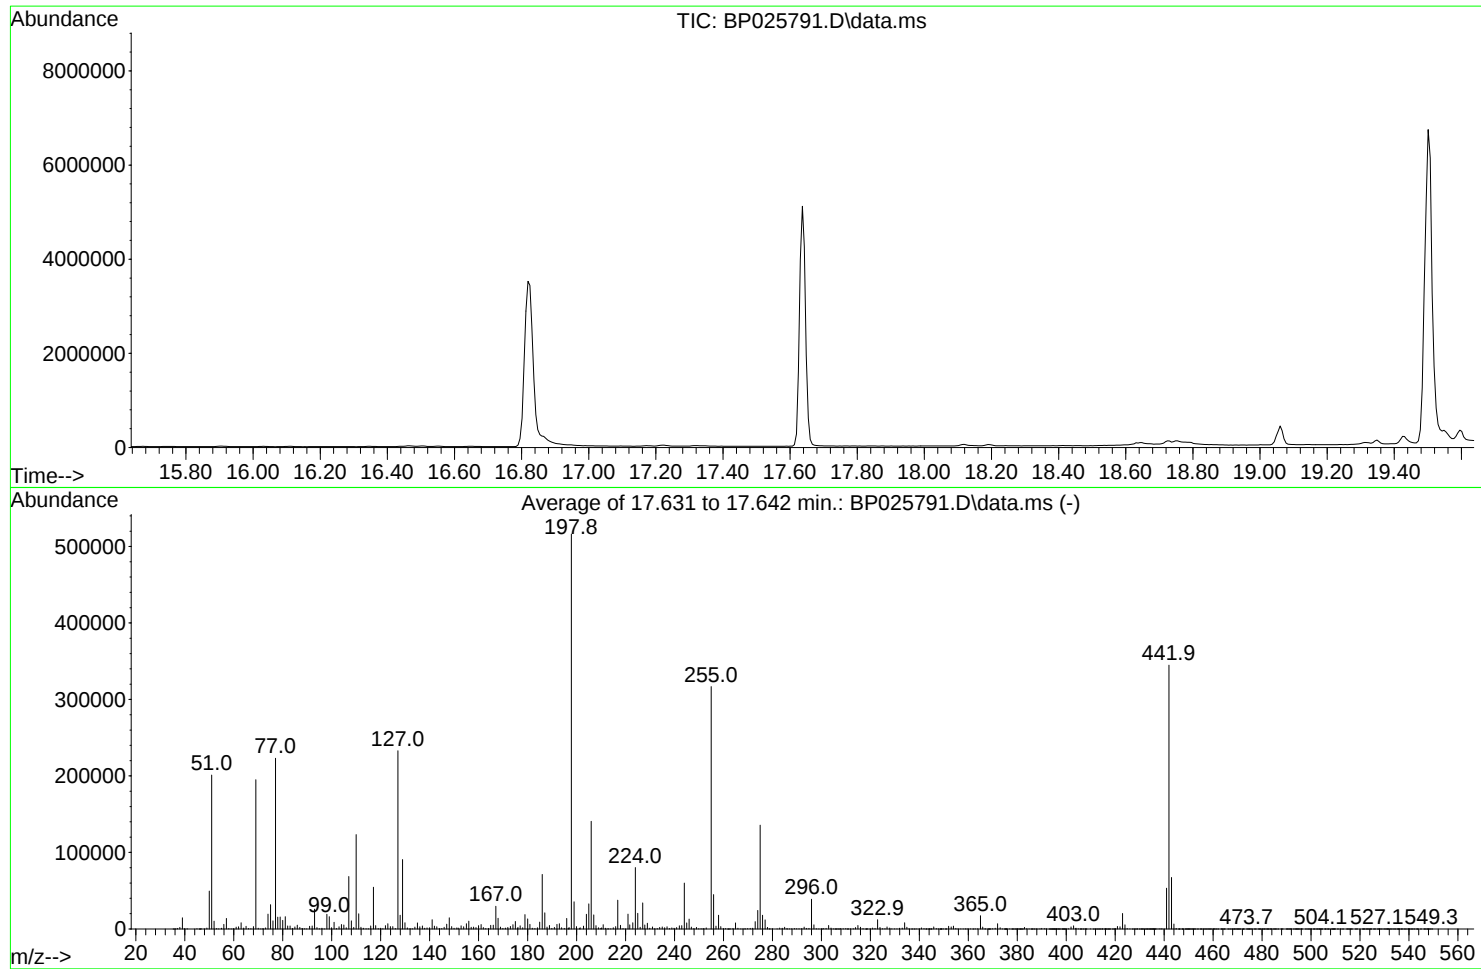




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2486

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	3128	PASS
69	69	100	100	100.0	195186	PASS
70	69	0.00	2	0.5	1034	PASS
197	198	0.00	2	0.4	1886	PASS
198	198	100	100	100.0	516192	PASS
199	198	5	9	6.9	35363	PASS
365	198	1	100	3.4	17349	PASS
441	443	0.01	150	79.2	53216	PASS
442	442	100	100	100.0	344742	PASS
443	442	15	24	19.5	67192	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091925\
Data File : BP025791.D
Acq On : 19 Sep 2025 09:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 19 11:12:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

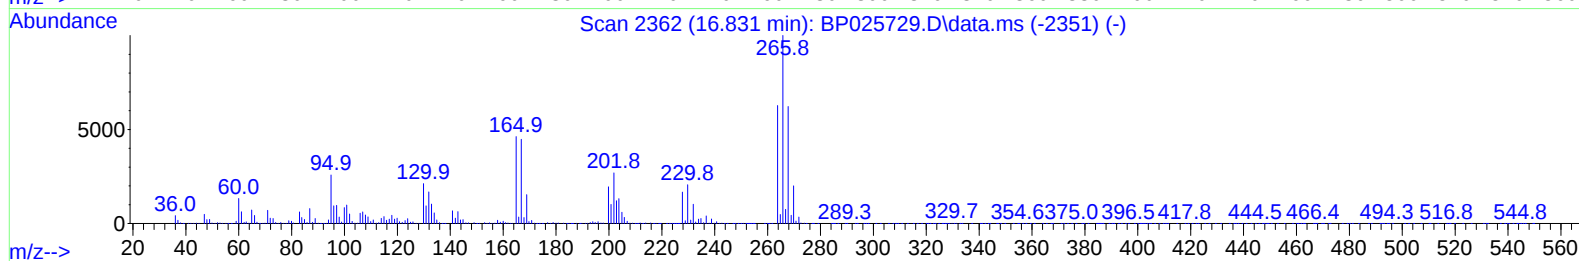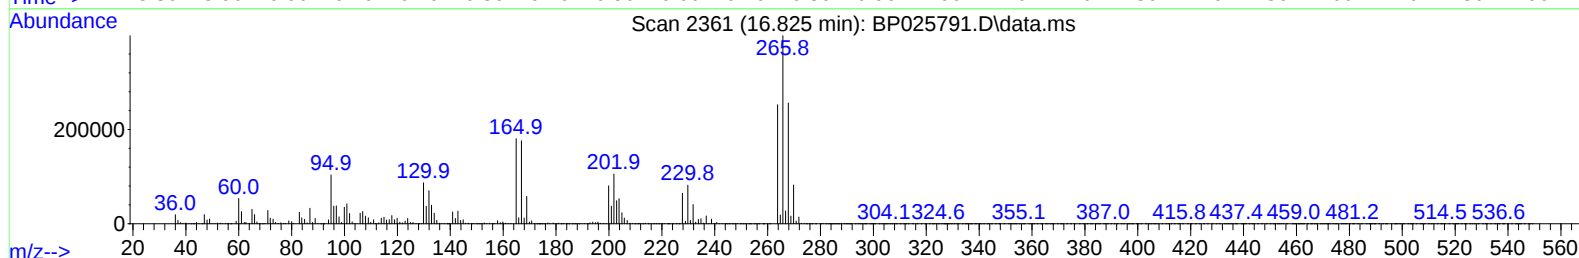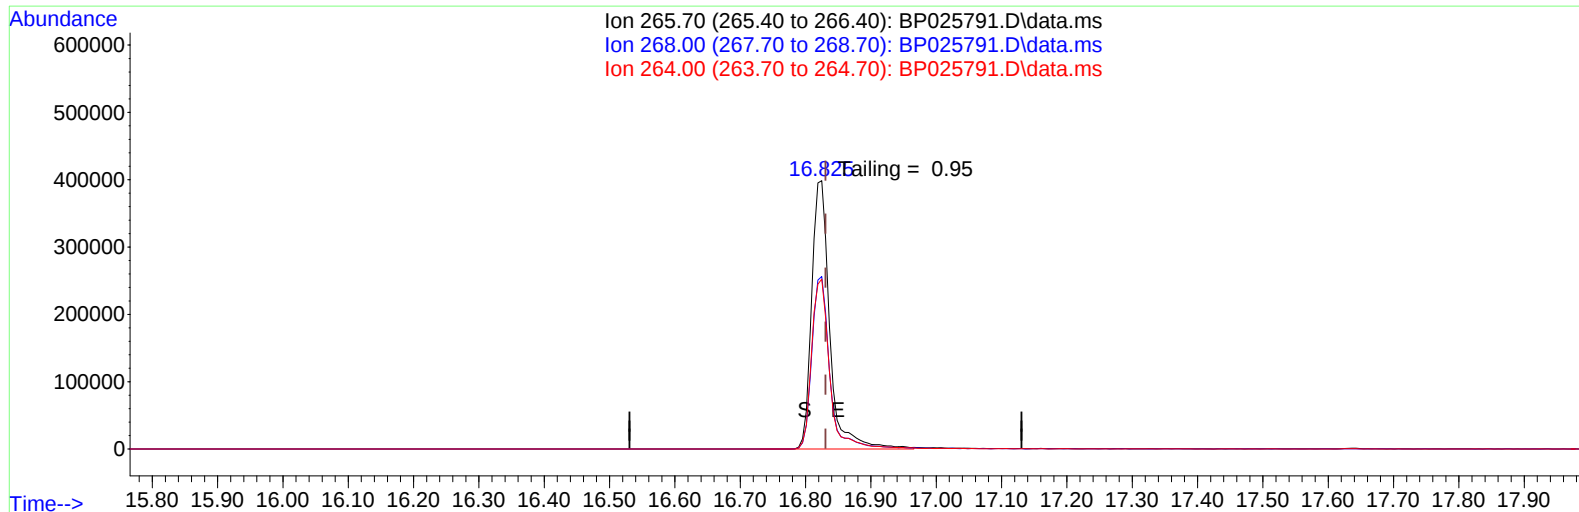

TIC: BP025791.D\data.ms

(70) Pentachlorophenol (C)

16.825min (-0.006) 12969.34 ng




response 772758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.28
264.00	62.70	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091925\
Data File : BP025791.D
Acq On : 19 Sep 2025 09:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 19 11:12:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

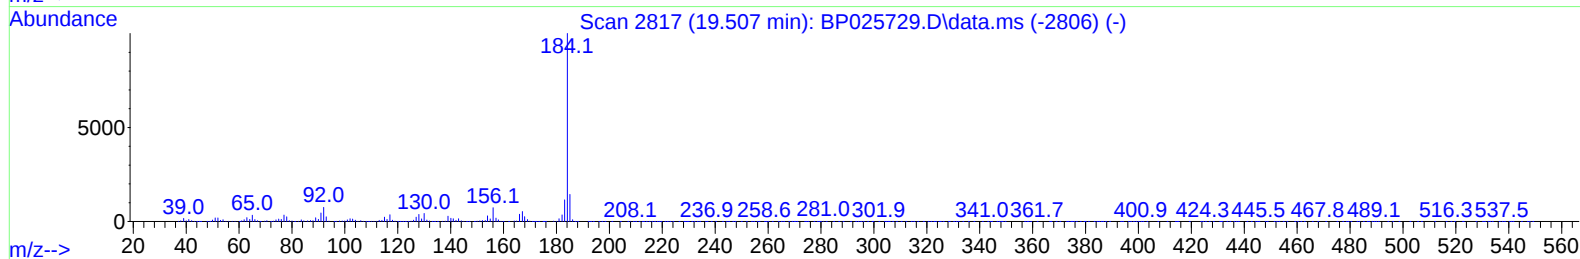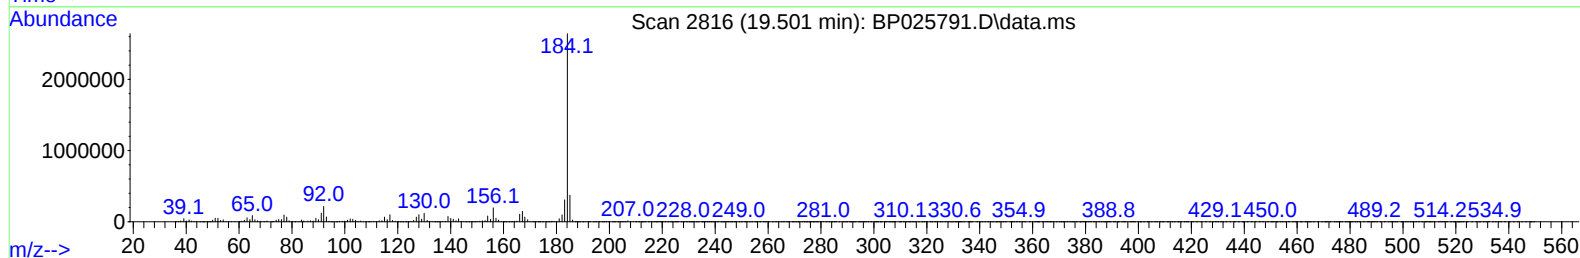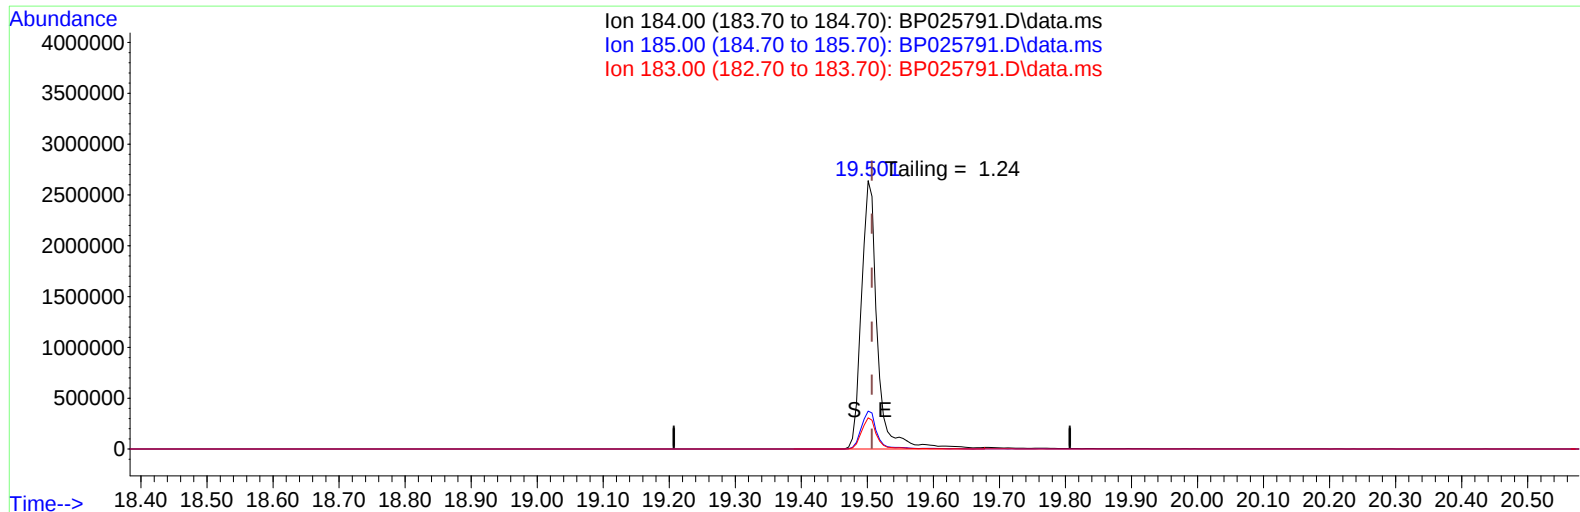

TIC: BP025791.D\data.ms

(77) Benzidine

19.501min (-0.006) 14332.79 ng

response 4314810

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.50	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2025	BNA_P	<u>BP025791.D</u>
Compound Name	Response	Retention Time
DDT	2212712	20.795
DDD	41408	20.336
DDE	8406	19.801
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49814	2262526	2.20

Instrument :
BNA_P
ClientSampleId :
DFTPP