Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091625\
Data File : VX047589.D
Acq On : 16 Sep 2025 11:40
Operator : JC/MD
Sample : VSTDICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Sep 17 06:15:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:04:35 2025
Response via : Initial Calibration

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED

Reviewed By :John Carlone 09/17/2025
Supervised By :Mahesh Dadoda 09/18/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.532	168	169280	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.739	114	298913	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	258399	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	122218	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.934	65	275758	102.341	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 204.680%#			
35) Dibromofluoromethane	5.361	113	212419	105.962	ug/l	-0.01
Spiked Amount 50.000	Range 75 - 124		Recovery = 211.920%#			
50) Toluene-d8	8.629	98	724078	104.386	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 208.780%#			
62) 4-Bromofluorobenzene	11.061	95	270289	102.672	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 205.340%#			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.173	85	172727	98.537	ug/l	100
3) Chloromethane	1.301	50	229165	99.472	ug/l	100
4) Vinyl Chloride	1.380	62	229175	101.621	ug/l	100
5) Bromomethane	1.611	94	143113	100.076	ug/l	99
6) Chloroethane	1.691	64	152487	101.167	ug/l	99
7) Trichlorofluoromethane	1.892	101	344488	102.878	ug/l	100
8) Diethyl Ether	2.130	74	142038	103.695	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.331	101	199843	102.067	ug/l	99
10) Methyl Iodide	2.453	142	313092	102.531	ug/l	99
11) Tert butyl alcohol	2.947	59	152108	506.863	ug/l	98
12) 1,1-Dichloroethene	2.319	96	206097	102.473	ug/l	93
13) Acrolein	2.233	56	150793	545.276	ug/l	97
14) Allyl chloride	2.660	41	415140	100.028	ug/l	99
15) Acrylonitrile	3.056	53	581240	522.897	ug/l	100
16) Acetone	2.374	43	510542	435.772	ug/l	100
17) Carbon Disulfide	2.514	76	537888	97.693	ug/l	98
18) Methyl Acetate	2.697	43	292867	112.324	ug/l	100
19) Methyl tert-butyl Ether	3.105	73	748952	102.011	ug/l	100
20) Methylene Chloride	2.782	84	242548	97.805	ug/l	97
21) trans-1,2-Dichloroethene	3.087	96	217759	100.566	ug/l	98
22) Diisopropyl ether	3.745	45	811840	100.934	ug/l	88
23) Vinyl Acetate	3.709	43	3314707	514.916	ug/l	99
24) 1,1-Dichloroethane	3.599	63	435815	101.944	ug/l	98
25) 2-Butanone	4.532	43	700827	479.558	ug/l	97
26) 2,2-Dichloropropane	4.465	77	357292	100.542	ug/l	99
27) cis-1,2-Dichloroethene	4.471	96	266550	100.516	ug/l	100
28) Bromochloromethane	4.873	49	198788	106.512	ug/l	99
29) Tetrahydrofuran	4.977	42	443530	504.502	ug/l	99
30) Chloroform	5.074	83	433937	100.447	ug/l	100
31) Cyclohexane	5.452	56	332995	93.523	ug/l	96
32) 1,1,1-Trichloroethane	5.367	97	372323	101.607	ug/l	99
36) 1,1-Dichloropropene	5.672	75	281650	96.149	ug/l	98
37) Ethyl Acetate	4.690	43	318793	101.641	ug/l	99
38) Carbon Tetrachloride	5.660	117	314745	98.891	ug/l	98
39) Methylcyclohexane	7.360	83	327858	98.600	ug/l	98
40) Benzene	6.019	78	880885	99.009	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091625\
Data File : VX047589.D
Acq On : 16 Sep 2025 11:40
Operator : JC/MD
Sample : VSTDICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Sep 17 06:15:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:04:35 2025
Response via : Initial Calibration

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED

Reviewed By :John Carlone 09/17/2025
Supervised By :Mahesh Dadoda 09/18/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.891	41	168753	104.220	ug/l	99
42) 1,2-Dichloroethane	6.062	62	331465	97.916	ug/l	100
43) Isopropyl Acetate	6.318	43	516875	100.482	ug/l	99
44) Trichloroethene	7.104	130	217753	101.234	ug/l	96
45) 1,2-Dichloropropane	7.409	63	228150	100.145	ug/l	100
46) Dibromomethane	7.562	93	164987	99.519	ug/l	99
47) Bromodichloromethane	7.806	83	345991	101.136	ug/l	98
48) Methyl methacrylate	7.671	41	260358	101.612	ug/l	100
49) 1,4-Dioxane	7.641	88	56717	2190.315	ug/l	99
51) 4-Methyl-2-Pentanone	8.555	43	1431253	501.834	ug/l	100
52) Toluene	8.702	92	536148	97.811	ug/l	99
53) t-1,3-Dichloropropene	8.958	75	355881	101.986	ug/l	100
54) cis-1,3-Dichloropropene	8.348	75	380577	102.038	ug/l	99
55) 1,1,2-Trichloroethane	9.135	97	205939	97.434	ug/l	97
56) Ethyl methacrylate	9.098	69	346659	104.435	ug/l	99
57) 1,3-Dichloropropane	9.293	76	362848	99.935	ug/l	98
58) 2-Chloroethyl Vinyl ether	8.226	63	836362	499.814	ug/l	100
59) 2-Hexanone	9.415	43	996274	486.380	ug/l	100
60) Dibromochloromethane	9.506	129	251394	103.226	ug/l	99
61) 1,2-Dibromoethane	9.592	107	217751	101.147	ug/l	100
64) Tetrachloroethene	9.256	164	165559	98.284	ug/l	98
65) Chlorobenzene	10.061	112	588517	100.253	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.147	131	208621	102.988	ug/l	100
67) Ethyl Benzene	10.177	91	1031346	101.823	ug/l	100
68) m/p-Xylenes	10.287	106	763898	202.624	ug/l	99
69) o-Xylene	10.622	106	372621	102.186	ug/l	99
70) Styrene	10.634	104	649863	101.710	ug/l	100
71) Bromoform	10.781	173	161188	106.566	ug/l	98
73) Isopropylbenzene	10.945	105	954900	102.768	ug/l	100
74) N-amyl acetate	10.823	43	448344	105.812	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.195	83	281608	100.172	ug/l	98
76) 1,2,3-Trichloropropane	11.220	75	229521m	90.444	ug/l	
77) Bromobenzene	11.183	156	234666	102.541	ug/l	98
78) n-propylbenzene	11.287	91	1119728	101.941	ug/l	99
79) 2-Chlorotoluene	11.348	91	683867	101.652	ug/l	99
80) 1,3,5-Trimethylbenzene	11.433	105	787327	103.134	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.000	75	102555	105.689	ug/l	98
82) 4-Chlorotoluene	11.433	91	802929	101.054	ug/l	100
83) tert-Butylbenzene	11.695	119	791896	101.333	ug/l	100
84) 1,2,4-Trimethylbenzene	11.732	105	790557	102.144	ug/l	99
85) sec-Butylbenzene	11.872	105	945321	101.840	ug/l	100
86) p-Isopropyltoluene	11.994	119	797643	101.501	ug/l	99
87) 1,3-Dichlorobenzene	11.951	146	432248	101.689	ug/l	100
88) 1,4-Dichlorobenzene	12.024	146	431839	98.985	ug/l	100
89) n-Butylbenzene	12.311	91	757239	104.138	ug/l	99
90) Hexachloroethane	12.518	117	148048	107.304	ug/l	100
91) 1,2-Dichlorobenzene	12.317	146	414491	102.352	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	12.920	75	61029	107.225	ug/l	98
93) 1,2,4-Trichlorobenzene	13.567	180	278777	105.922	ug/l	100
94) Hexachlorobutadiene	13.707	225	92124	103.049	ug/l	99
95) Naphthalene	13.756	128	854492	106.620	ug/l	100
96) 1,2,3-Trichlorobenzene	13.939	180	263512	107.633	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091625\
Data File : VX047589.D
Acq On : 16 Sep 2025 11:40
Operator : JC/MD
Sample : VSTDICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Sep 17 06:15:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:04:35 2025
Response via : Initial Calibration

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED

Reviewed By :John Carlone 09/17/2025
Supervised By :Mahesh Dadoda 09/18/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091625\
Data File : VX047589.D
Acq On : 16 Sep 2025 11:40
Operator : JC/MD
Sample : VSTDICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Sep 17 06:15:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:04:35 2025
Response via : Initial Calibration

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED
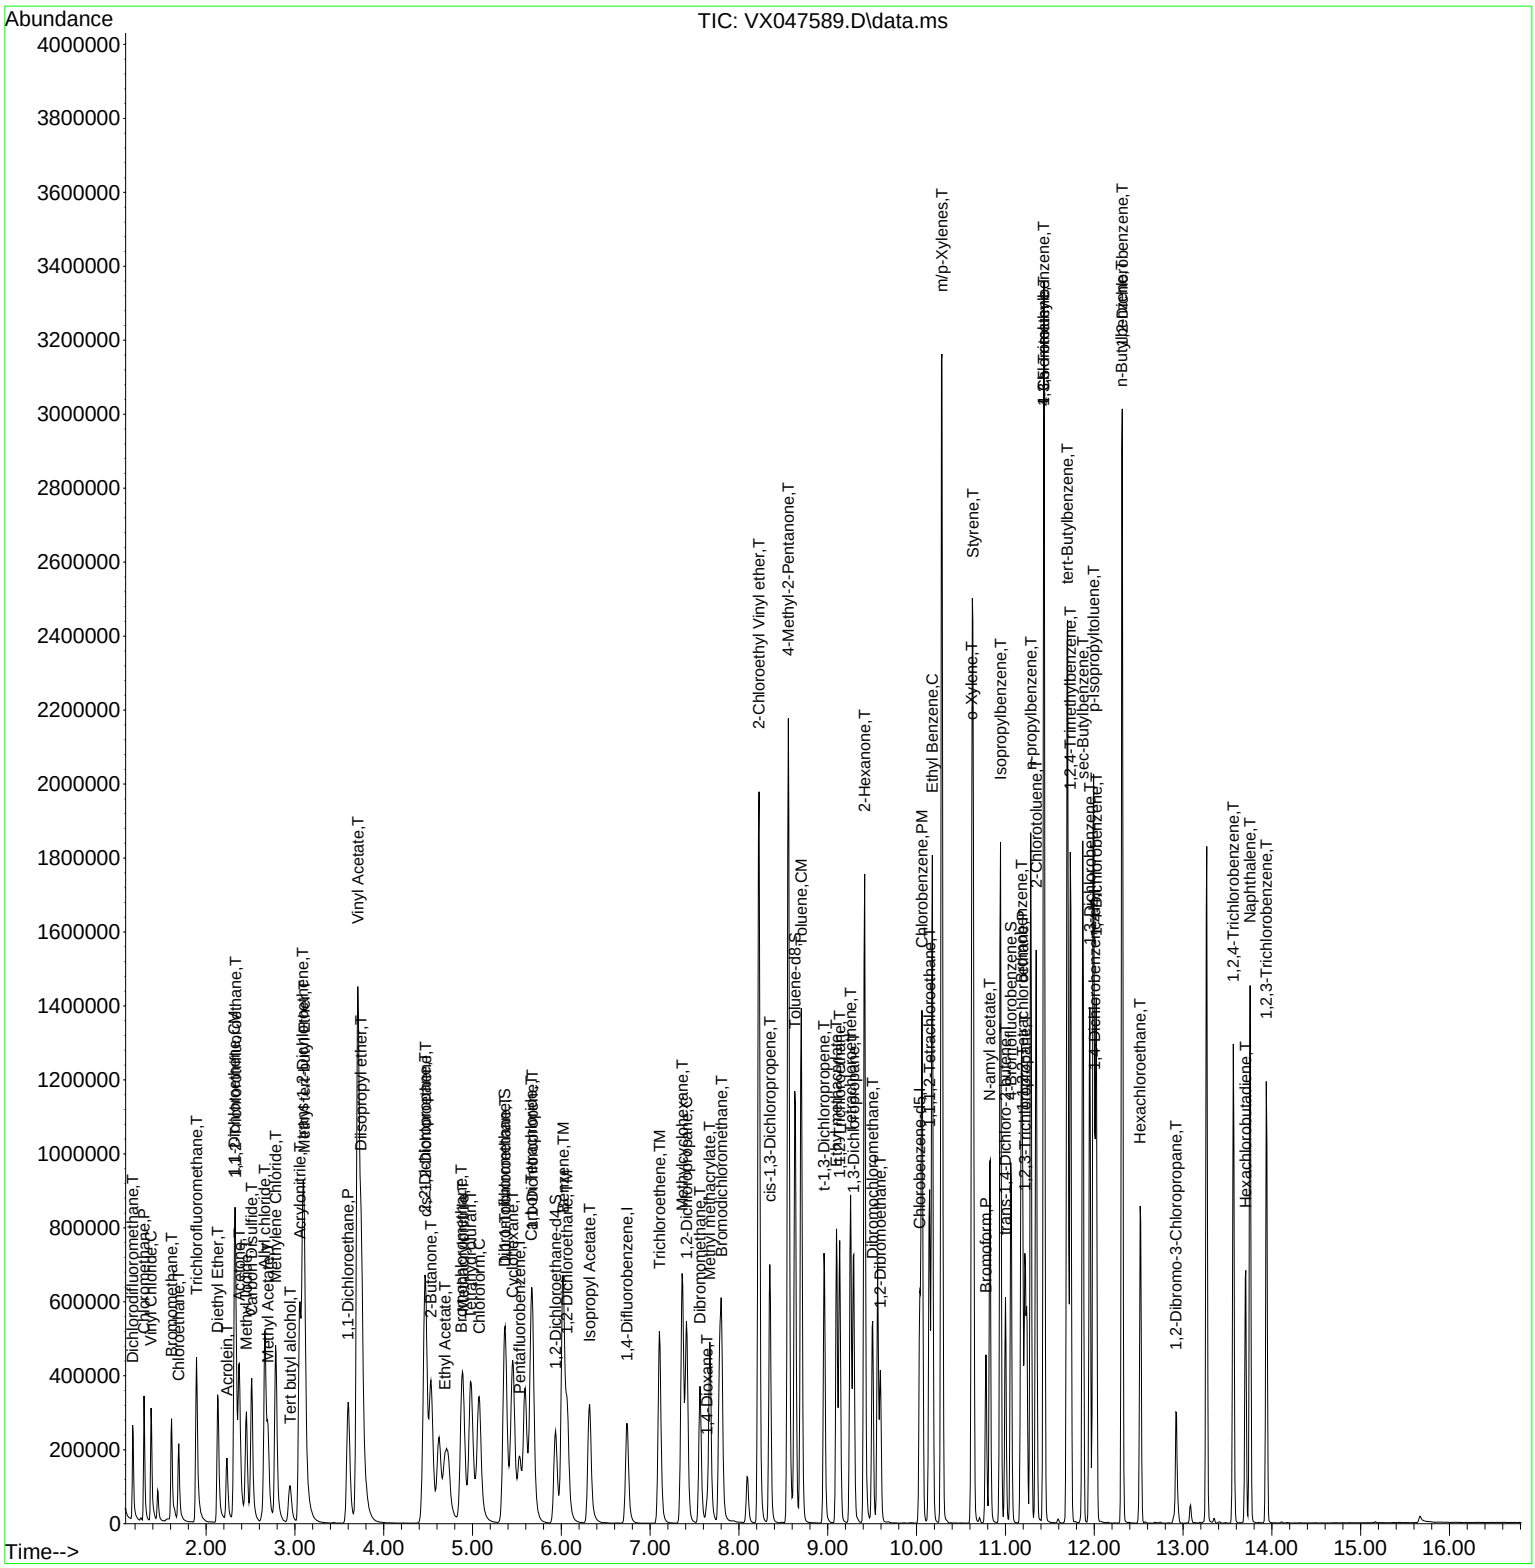
Reviewed By :John Carlone 09/17/2025
Supervised By :Mahesh Dadoda 09/18/2025