

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091625\
 Data File : VN087849.D
 Acq On : 16 Sep 2025 15:04
 Operator : JC\MD
 Sample : VN0916WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0916WBL01

Quant Time: Sep 17 01:20:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 22 02:55:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	184438	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	413572	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	397360	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	180365	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	185379	49.056	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.120%
35) Dibromofluoromethane	8.153	113	151424	50.712	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.420%
50) Toluene-d8	10.547	98	526852	47.141	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.280%
62) 4-Bromofluorobenzene	12.829	95	181702	45.717	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	91.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091625\
Data File : VN087849.D
Acq On : 16 Sep 2025 15:04
Operator : JC\MD
Sample : VN0916WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01

Quant Time: Sep 17 01:20:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 22 02:55:42 2025
Response via : Initial Calibration




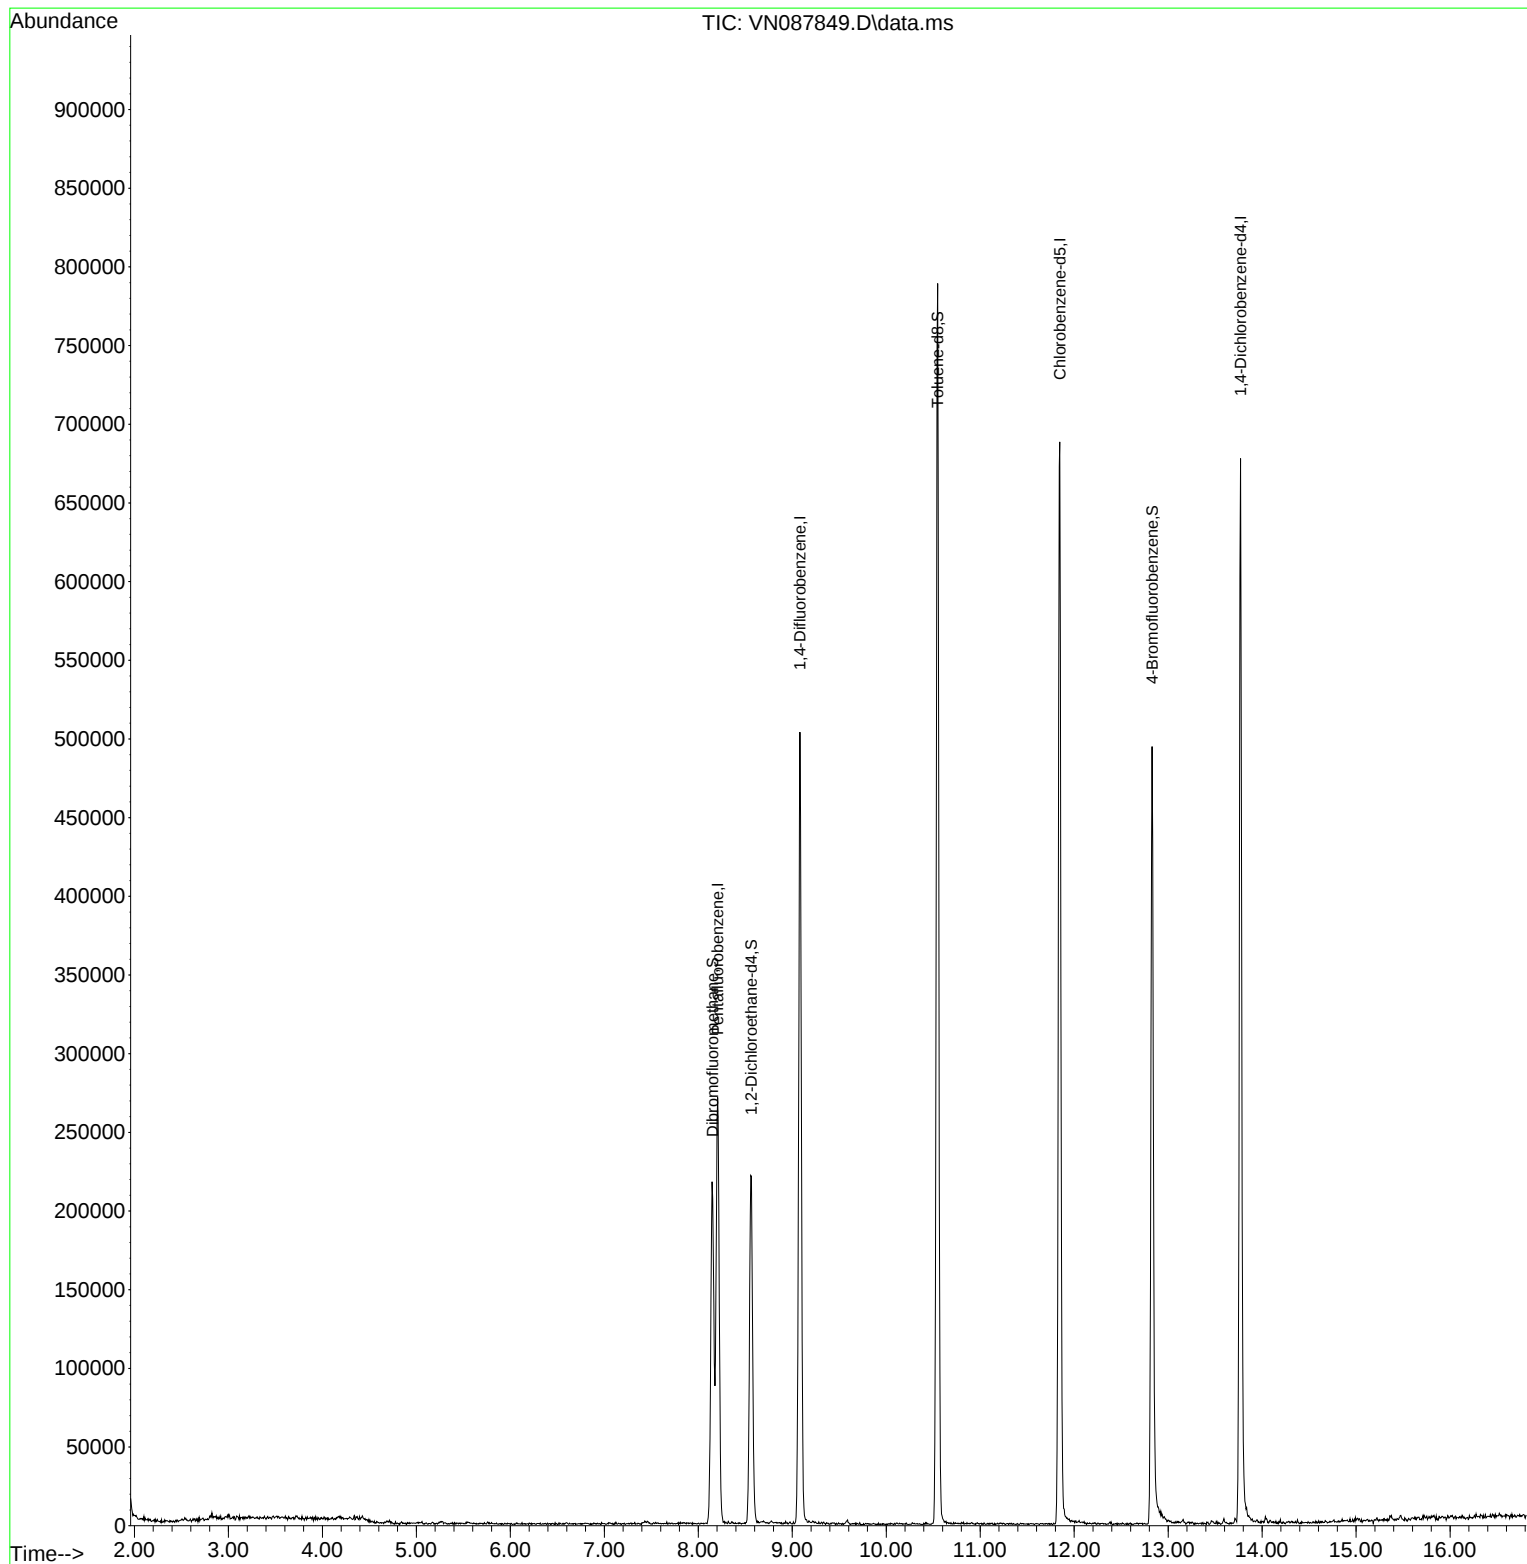


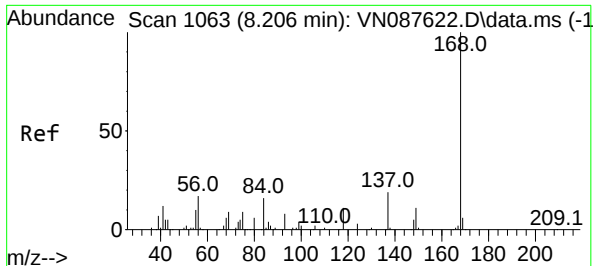

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. -0.000 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04




Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01


Tgt Ion:168 Resp: 184438
Ion Ratio Lower Upper
168 100
99 64.4 57.2 85.8

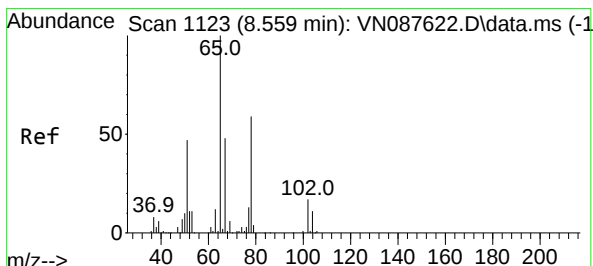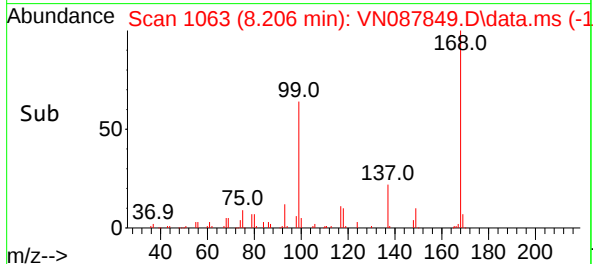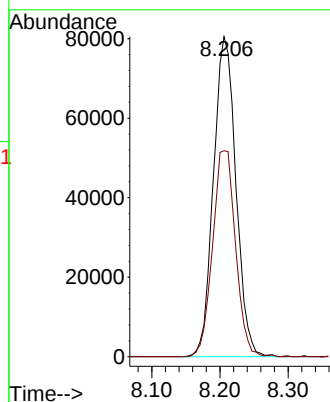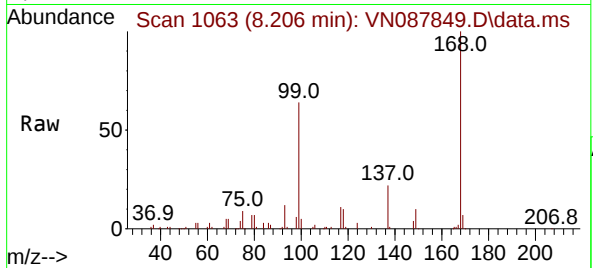

#33
1,2-Dichloroethane-d4
Concen: 49.056 ug/l
RT: 8.565 min Scan# 1124
Delta R.T. 0.006 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04

Tgt Ion: 65 Resp: 185379
Ion Ratio Lower Upper
65 100
67 50.7 0.0 100.0


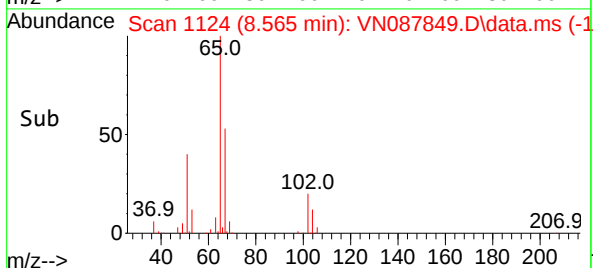
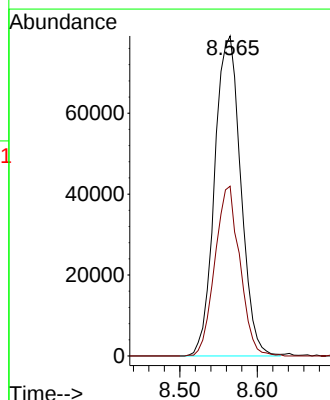
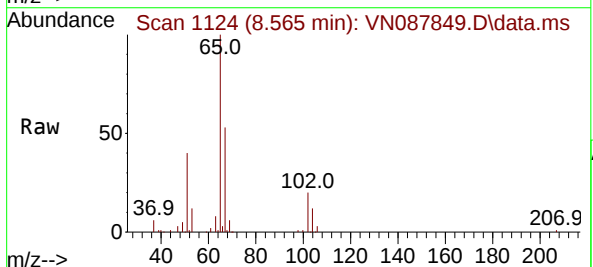


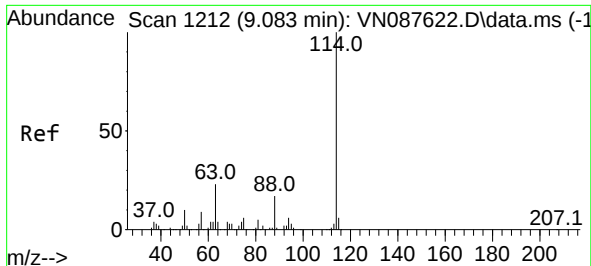

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.082 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04




Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01


Tgt Ion:114 Resp: 413572
Ion Ratio Lower Upper
114 100
63 23.6 0.0 45.2
88 16.1 0.0 33.4

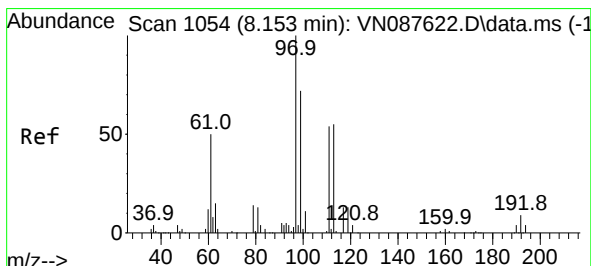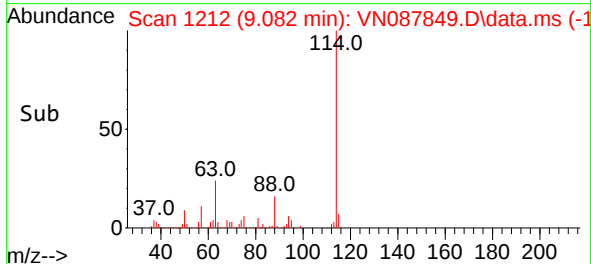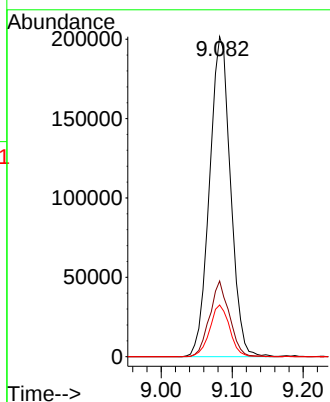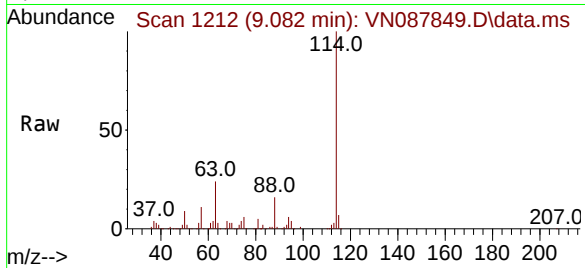

#35
Dibromofluoromethane
Concen: 50.712 ug/l
RT: 8.153 min Scan# 1054
Delta R.T. -0.000 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04

Tgt Ion:113 Resp: 151424
Ion Ratio Lower Upper
113 100
111 105.6 82.8 124.2
192 17.5 12.8 19.2


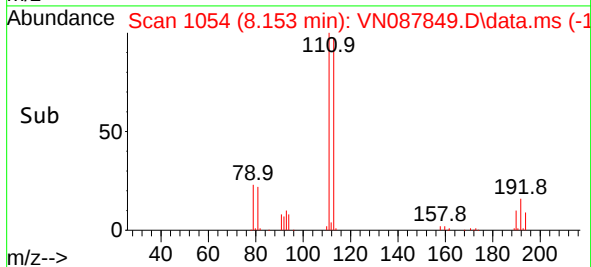
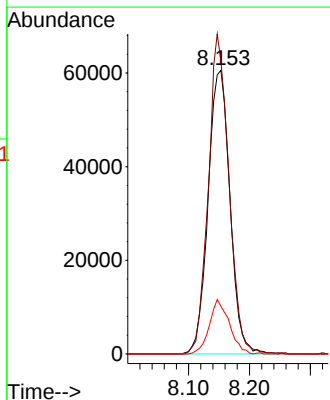
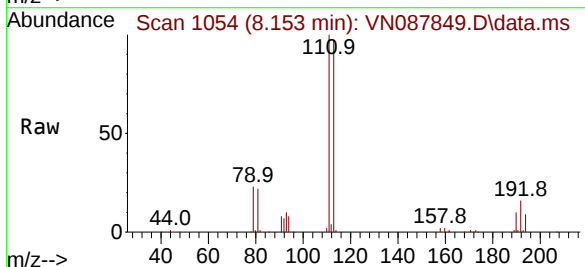


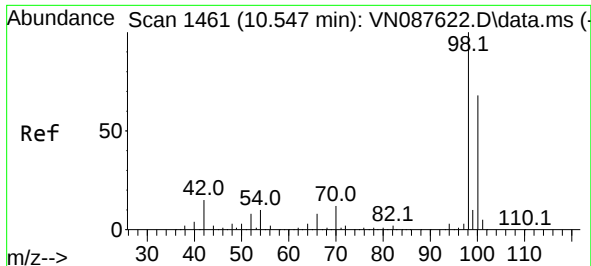

#50
Toluene-d8
Concen: 47.141 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04




Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01


Tgt Ion: 98 Resp: 526852
Ion Ratio Lower Upper
98 100
100 63.8 52.8 79.2

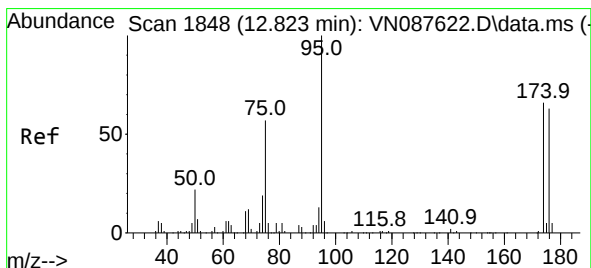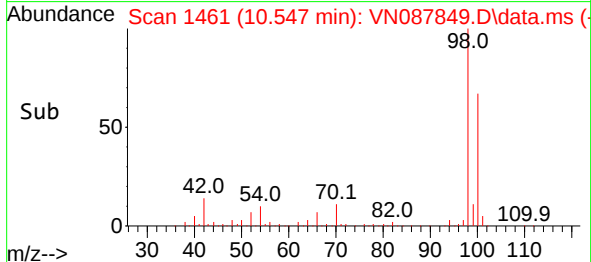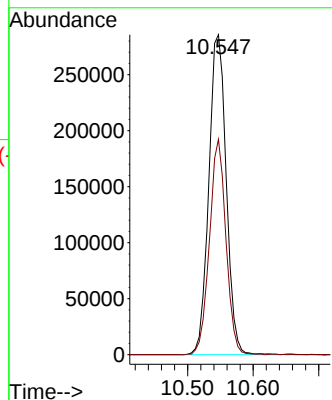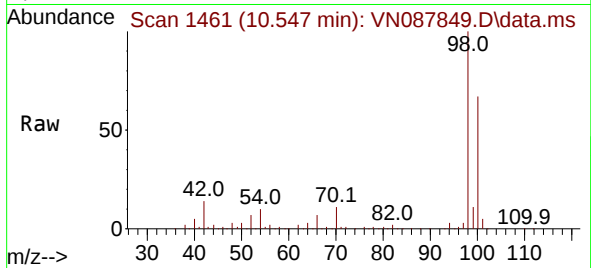

#62
4-Bromofluorobenzene
Concen: 45.717 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04

Tgt Ion: 95 Resp: 181702
Ion Ratio Lower Upper
95 100
174 70.5 0.0 138.4
176 69.5 0.0 132.6


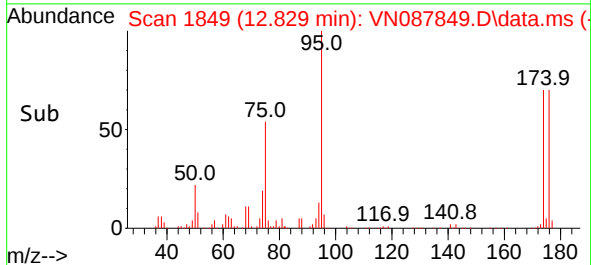
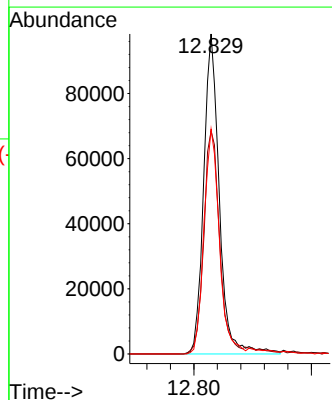
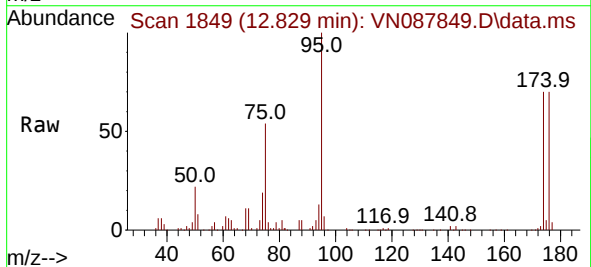


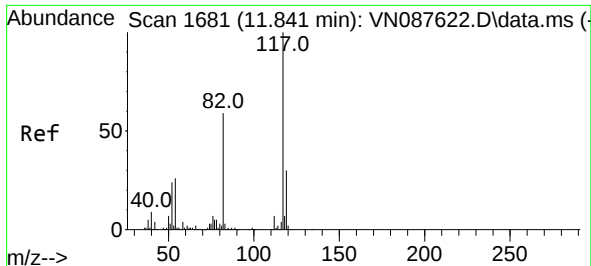

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04

Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01

Tgt Ion:117 Resp: 397360
Ion Ratio Lower Upper
117 100
82 58.5 47.4 71.2
119 32.0 24.3 36.5

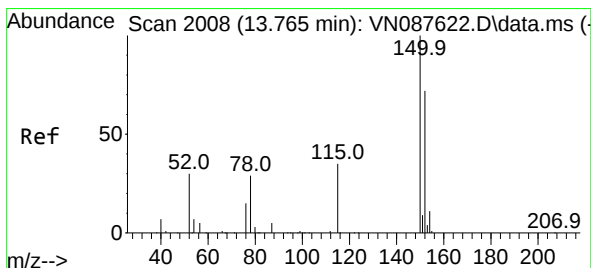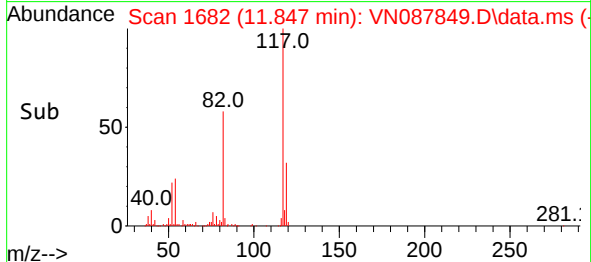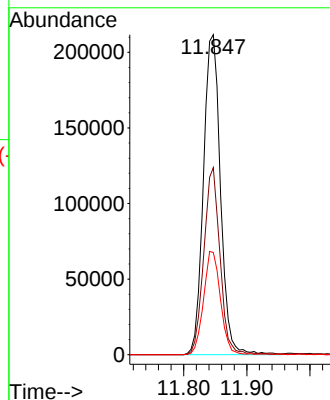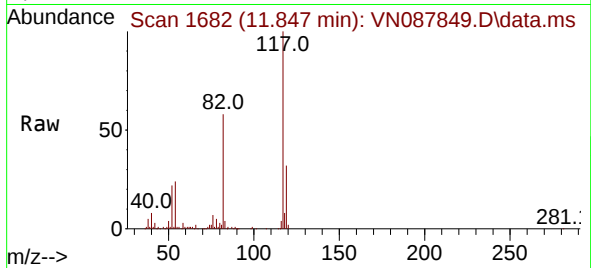

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN087849.D
Acq: 16 Sep 2025 15:04

Tgt Ion:152 Resp: 180365
Ion Ratio Lower Upper
152 100
115 63.1 32.3 96.8
150 160.4 0.0 351.0

