
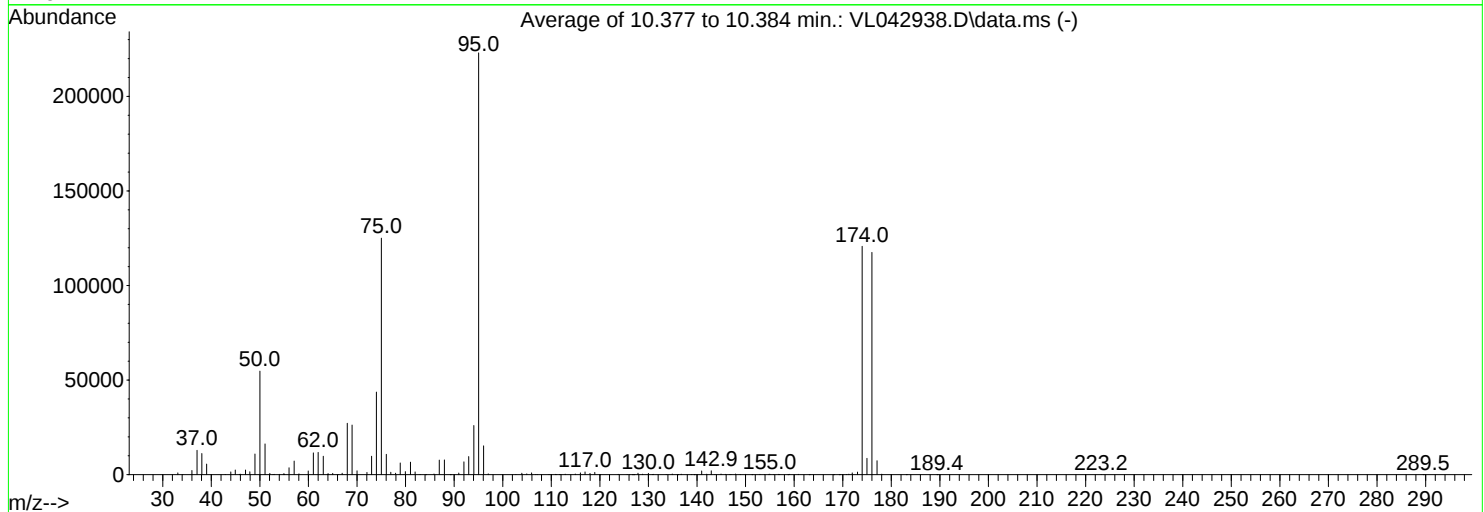


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091825\
Data File : VL042938.D
Acq On : 18 Sep 2025 07:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Sep 18 02:57:46 2025

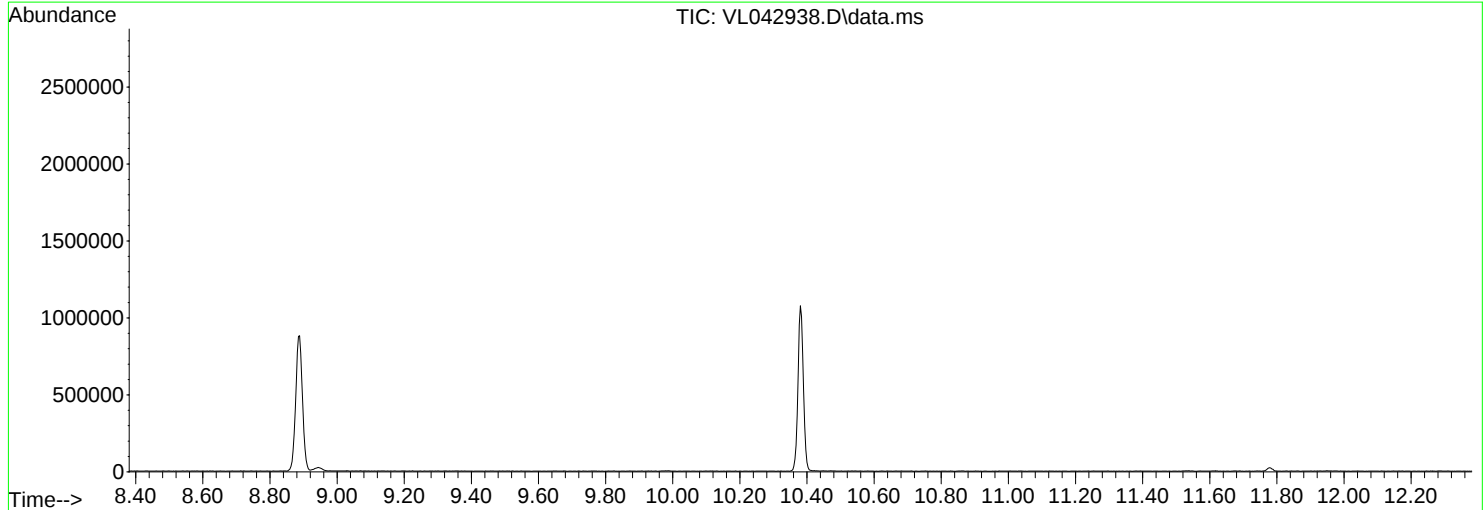

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.5	54715	PASS
75	95	30	66	56.1	125027	PASS
95	95	100	100	100.0	223019	PASS
96	95	5	9	6.8	15247	PASS
173	174	0.00	2	1.1	1327	PASS
174	95	50	120	54.1	120688	PASS
175	174	4	9	7.2	8675	PASS
176	174	93	101	97.4	117509	PASS
177	176	5	9	6.3	7359	PASS

Average of 10.377 to 10.384 min.: VL042938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	940	47.05	2452	56.00	3618	66.95	76
34.15	81	47.95	1522	57.05	7180	68.00	2712
36.00	2244	49.00	10911	58.05	408	69.00	2621
37.05	12901	50.00	54715	59.95	1973	70.00	206
38.05	11180	51.05	16251	61.00	11498	72.05	1180
39.05	5565	52.05	699	62.00	11801	73.00	9761
42.85	95	52.70	69	63.05	9721	74.00	43627
44.00	1483	52.95	144	63.90	323	75.00	125027
44.95	2417	54.05	148	64.10	440	76.05	10769
45.80	138	54.85	426	65.00	717	76.95	1298
46.05	268	55.10	322	66.10	100	77.95	803

Average of 10.377 to 10.384 min.: VL042938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	6156	92.00	6812	107.10	117	117.95	698
79.95	1630	93.00	9523	109.55	53	118.95	1181
81.00	6577	94.05	26011	110.00	115	119.95	11
81.95	1453	95.05	223019	110.85	189	123.75	137
83.00	131	96.05	15247	111.10	94	125.60	49
84.10	35	97.00	417	111.70	126	126.15	68
85.85	353	102.70	71	111.95	65	126.70	19
86.95	7683	103.95	804	112.85	237	127.00	47
88.00	7814	104.95	400	114.95	337	127.85	800
89.20	32	105.95	907	116.00	914	128.80	290
90.95	862	106.80	119	116.95	1414	130.00	665

Average of 10.377 to 10.384 min.: VL042938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.80	61	142.95	2020	153.95	86	169.30	36
131.00	189	143.70	107	154.80	211	170.00	80
133.65	61	144.95	355	155.00	246	170.80	69
134.90	371	145.90	207	155.80	50	171.25	249
136.00	20	146.75	52	156.80	195	171.95	937
136.75	255	147.00	85	157.00	83	173.05	1327
138.90	51	147.95	346	158.70	41	174.00	120688
139.40	44	148.90	110	159.05	199	175.00	8675
140.05	50	150.00	176	160.85	151	176.00	117509
140.95	1970	151.30	24	163.10	18	177.05	7359
142.00	244	152.95	145	168.10	23	178.05	280

Average of 10.377 to 10.384 min.: VL042938.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
183.10	23						
189.40	17						
223.20	63						
289.50	23						

Instrument :

MSVOA_L

ClientSampleId :

BFB