
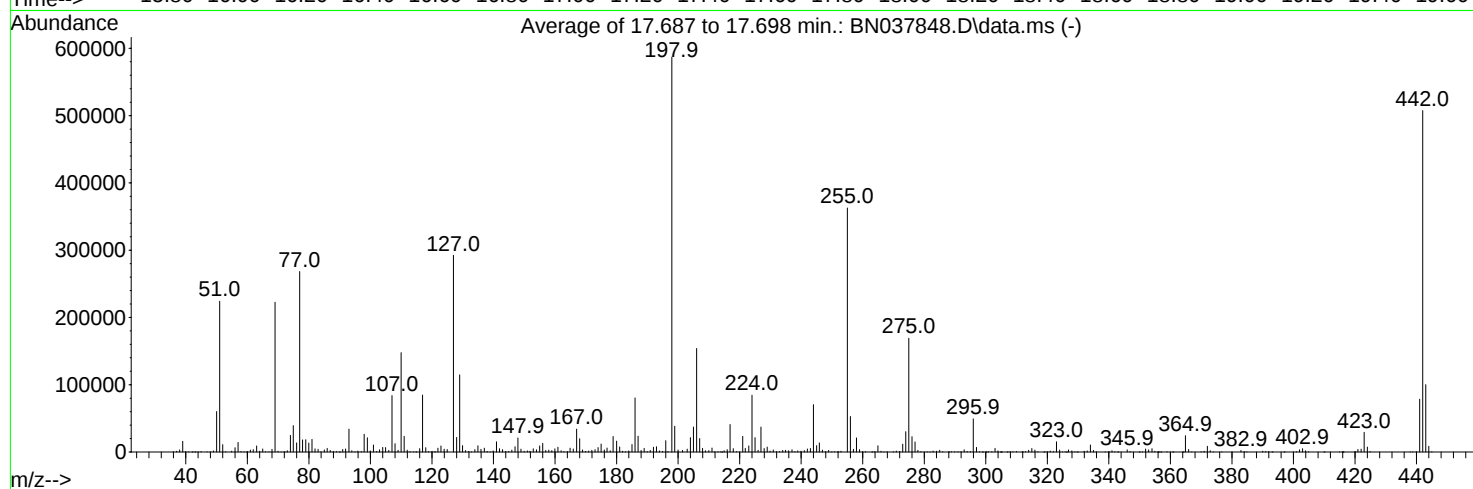


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092225\
Data File : BN037848.D
Acq On : 22 Sep 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 14:20:01 2025

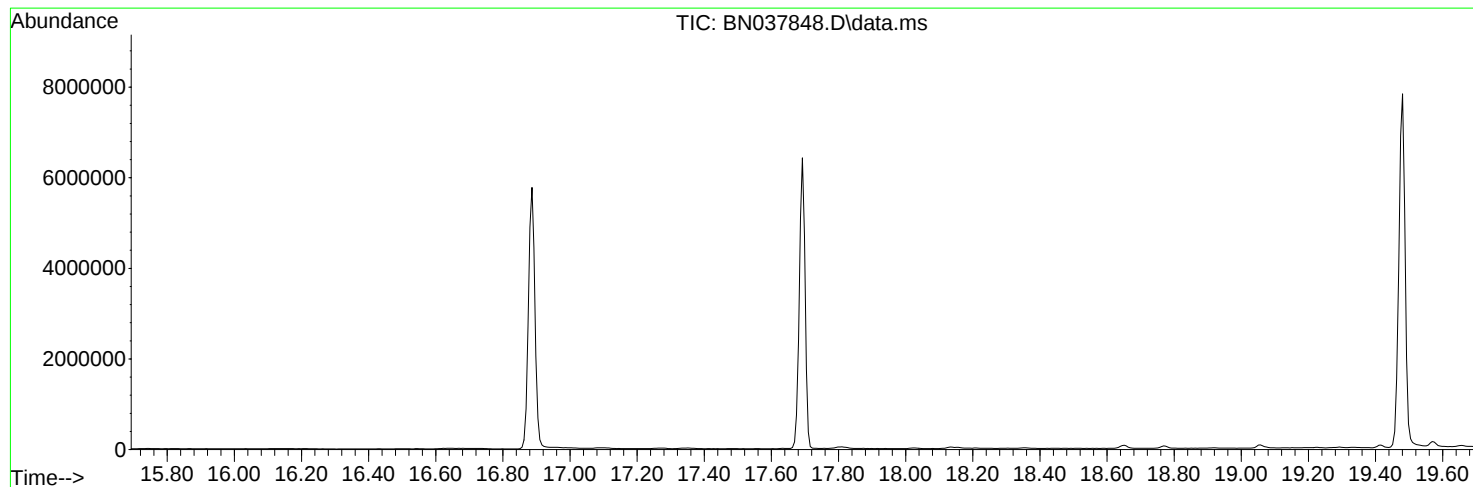




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	3978	PASS
69	69	100	100	100.0	222750	PASS
70	69	0.00	2	0.5	1151	PASS
197	198	0.00	2	0.1	725	PASS
198	198	100	100	100.0	586901	PASS
199	198	5	9	6.5	38309	PASS
365	198	1	100	4.1	24221	PASS
441	443	0.01	150	78.4	78467	PASS
442	442	100	100	100.0	507499	PASS
443	442	15	24	19.7	100147	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092225\
Data File : BN037848.D
Acq On : 22 Sep 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 13:51:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

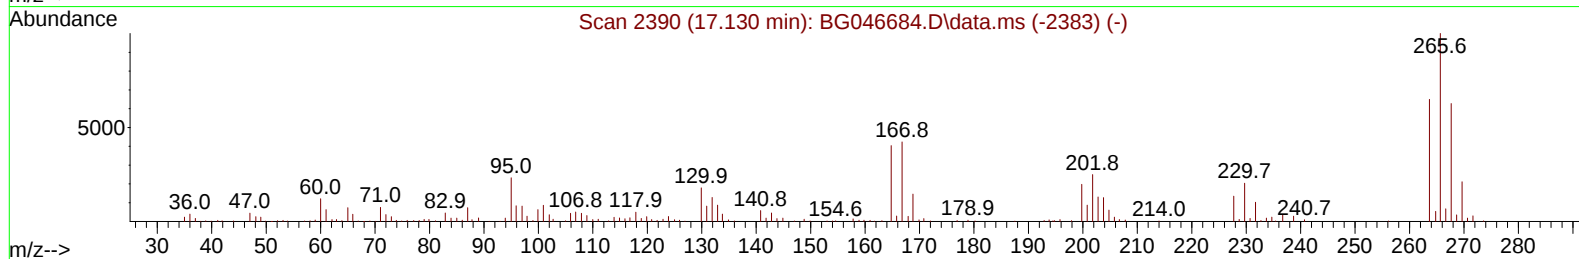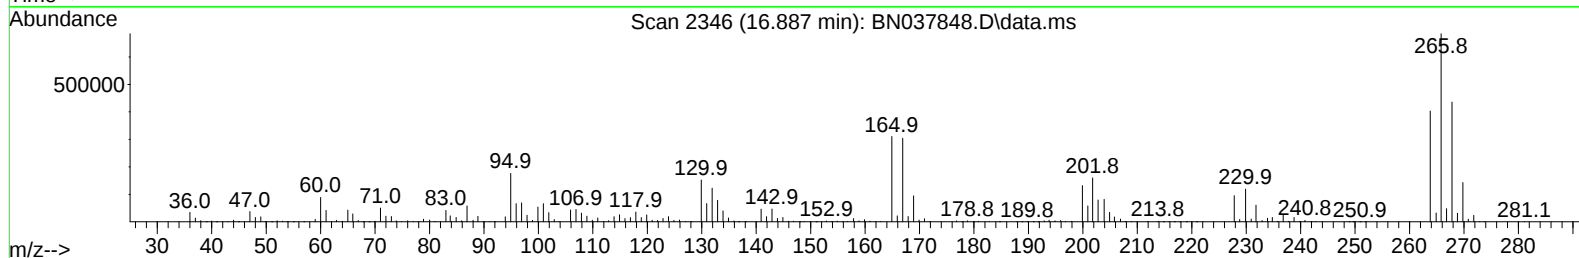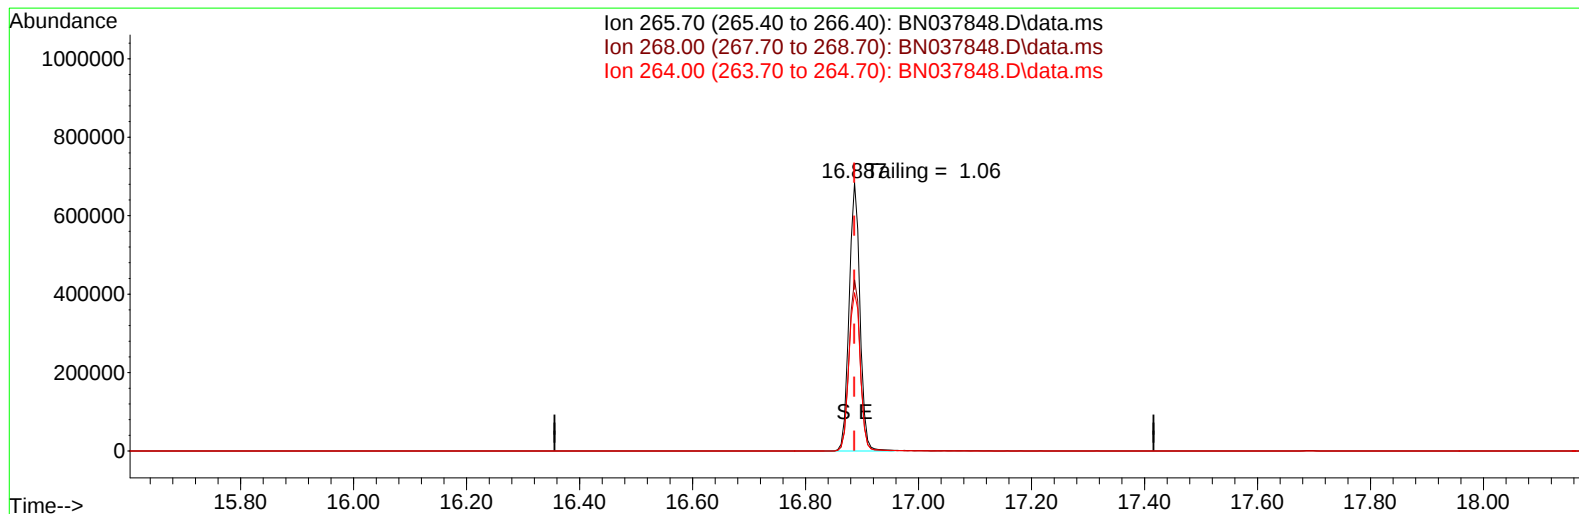

TIC: BN037848.D\data.ms

(70) Pentachlorophenol (C)

16.887min (+ 0.001) 31161.16 ng




response 916310

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.71
264.00	61.60	58.94
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092225\  
Data File : BN037848.D  
Acq On    : 22 Sep 2025  08:59  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 13:51:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

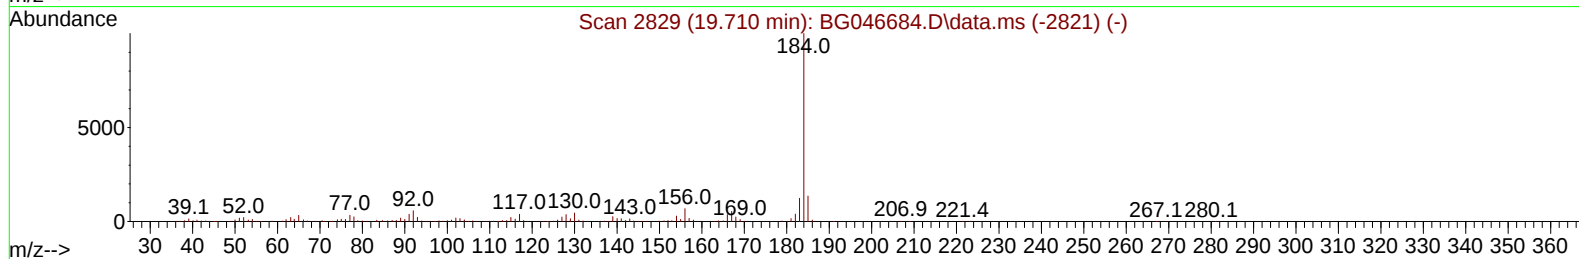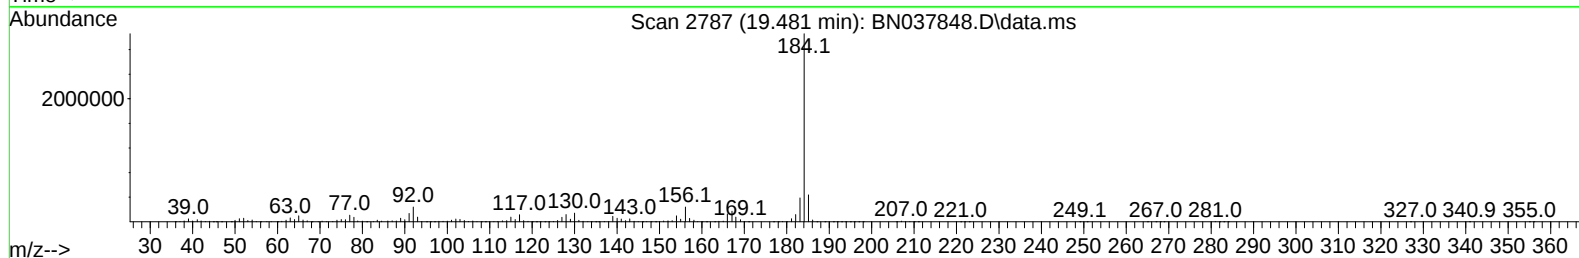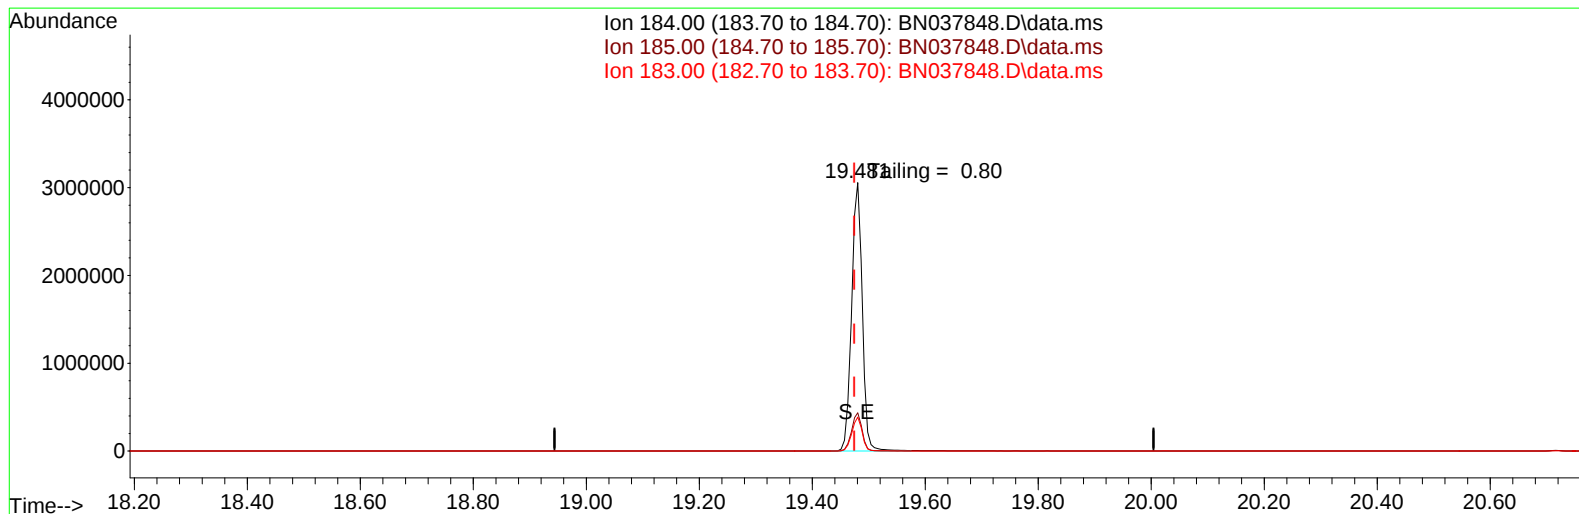

TIC: BN037848.D\data.ms

(77) Benzidine

19.481min (+ 0.006) 0.00 ng

response **4033195**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2025	BNA_N	<u>BN037848.D</u>
Compound Name	Response	Retention Time
DDT	1976892	20.716
DDD	45417	20.275
DDE	4263	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49680	2026572	2.45

Instrument :
BNA_N
ClientSampleId :
DFTPP