
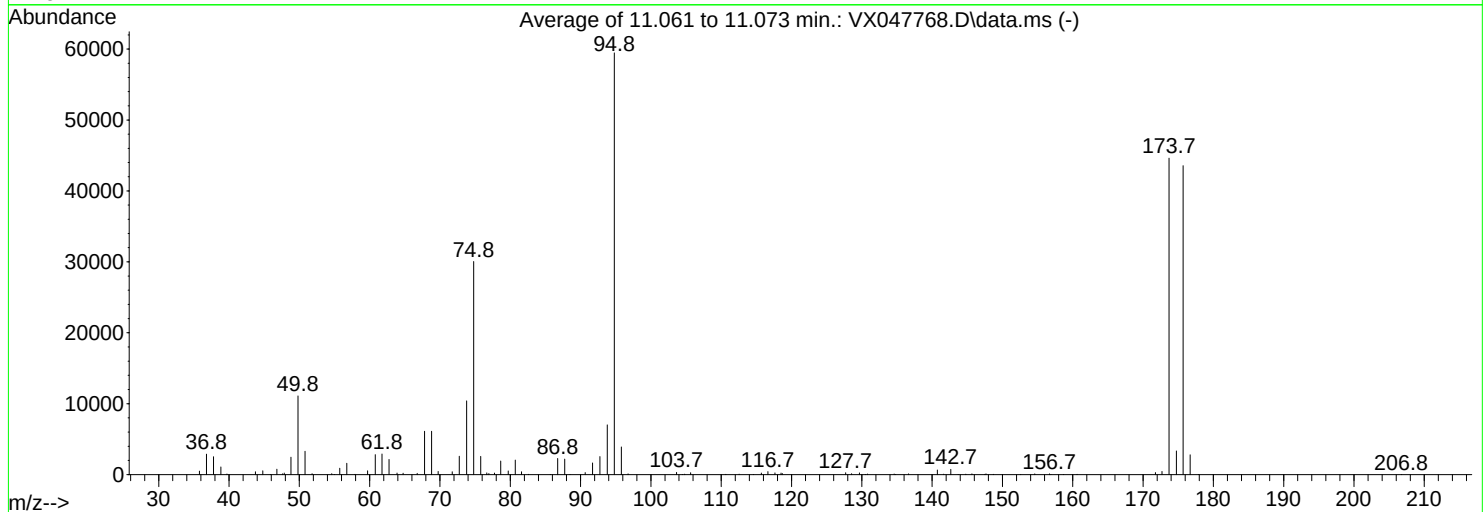


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092425\
Data File : VX047768.D
Acq On : 24 Sep 2025 11:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

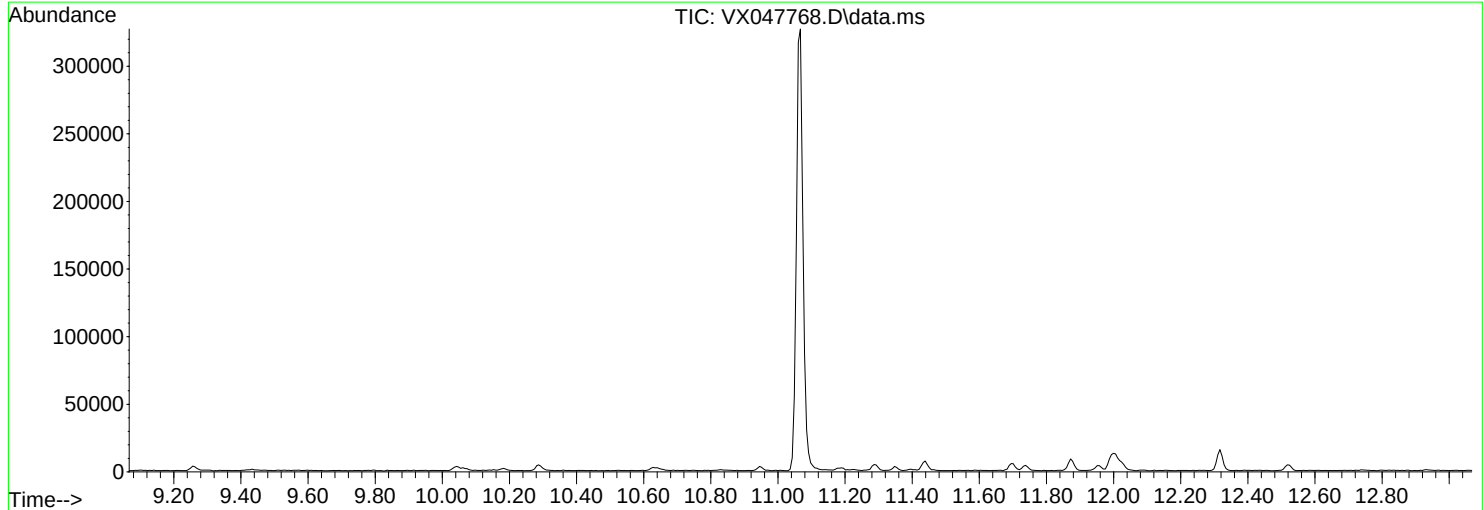

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	11093	PASS
75	95	30	60	50.5	30043	PASS
95	95	100	100	100.0	59467	PASS
96	95	5	9	6.6	3896	PASS
173	174	0.00	2	1.0	443	PASS
174	95	50	100	75.0	44629	PASS
175	174	5	9	7.5	3342	PASS
176	174	95	101	97.6	43568	PASS
177	176	5	9	6.4	2794	PASS