

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092525\
 Data File : VX047811.D
 Acq On : 25 Sep 2025 14:56
 Operator : JC/MD
 Sample : Q3128-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW6-10-20250916

Quant Time: Sep 26 01:29:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	124352	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	260863	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	264166	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	132252	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	101668	51.364	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	102.720%
35) Dibromofluoromethane	5.379	113	85144	48.668	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.340%
50) Toluene-d8	8.635	98	293211	48.436	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.880%
62) 4-Bromofluorobenzene	11.067	95	123993	53.970	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092525\
Data File : VX047811.D
Acq On : 25 Sep 2025 14:56
Operator : JC/MD
Sample : Q3128-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW6-10-20250916

Quant Time: Sep 26 01:29:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration




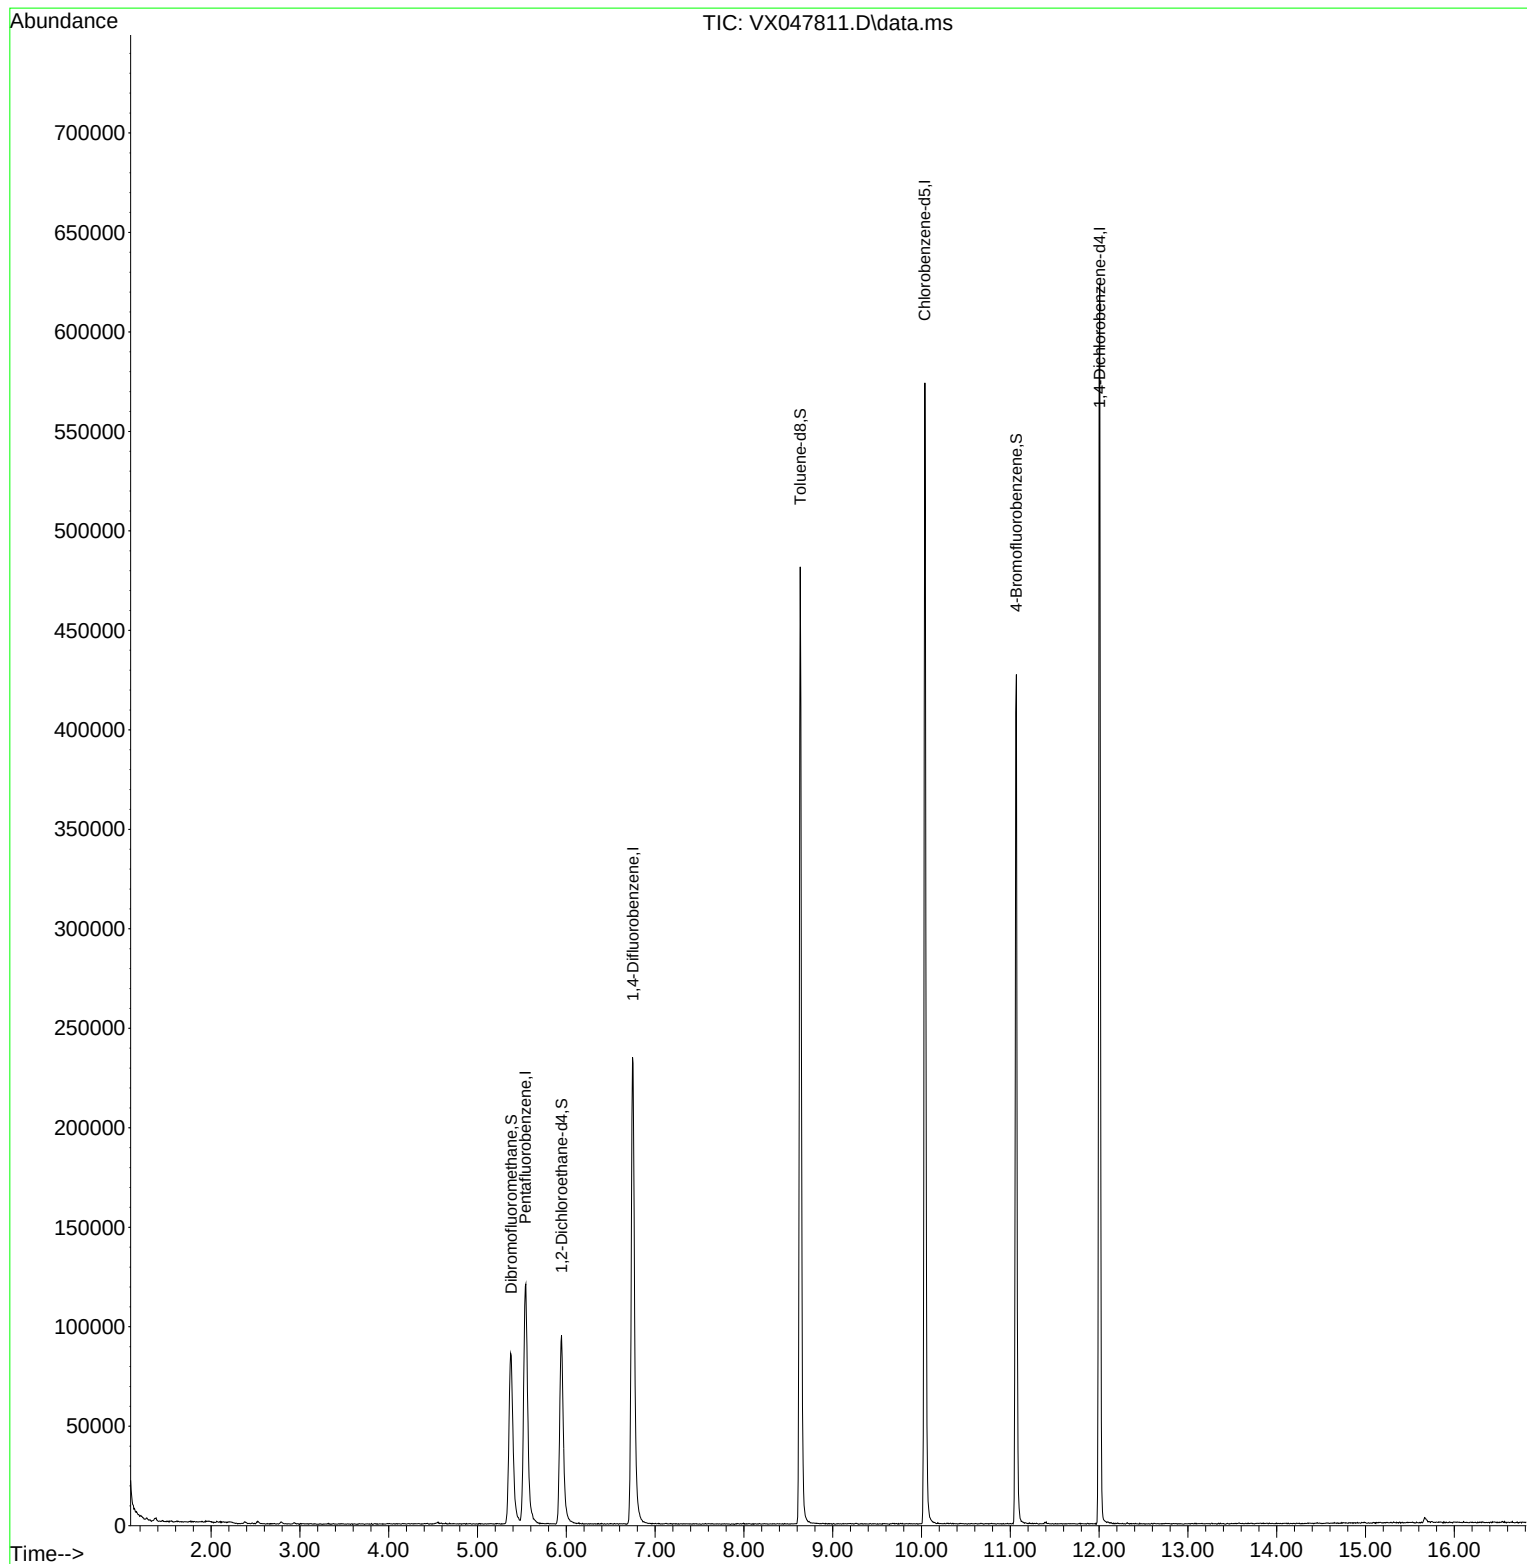


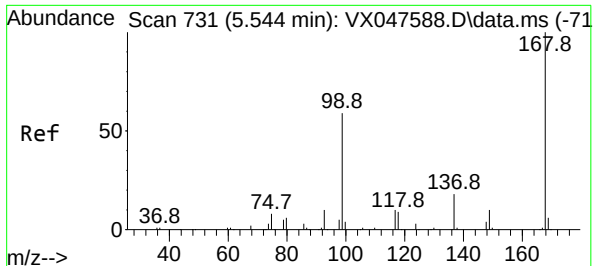

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 711
Delta R.T. -0.006 min
Lab File: VX047811.D
Acq: 25 Sep 2025 14:56




Instrument :
MSVOA_X
ClientSampleId :
BPOW6-10-20250916


Tgt Ion:168 Resp: 124352
Ion Ratio Lower Upper
168 100
99 58.4 48.8 73.2

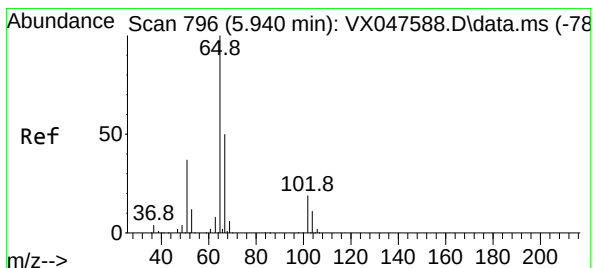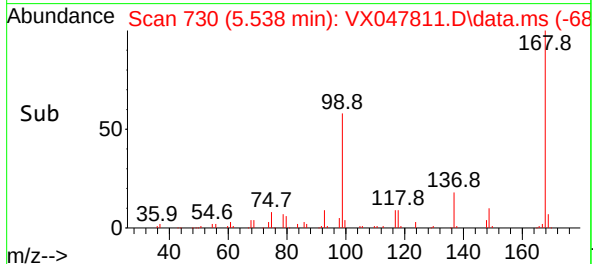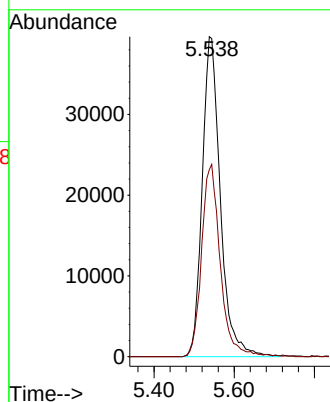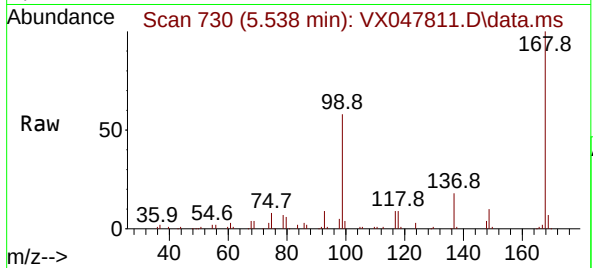

#33
1,2-Dichloroethane-d4
Concen: 51.364 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX047811.D
Acq: 25 Sep 2025 14:56

Tgt Ion: 65 Resp: 101668
Ion Ratio Lower Upper
65 100
67 51.9 0.0 103.0


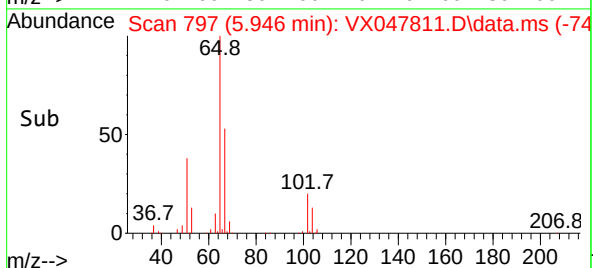
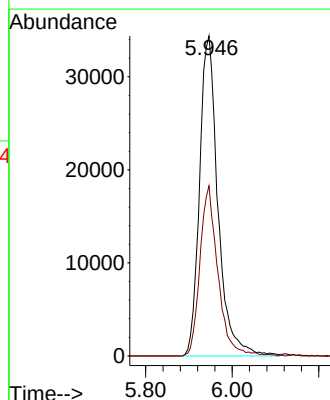
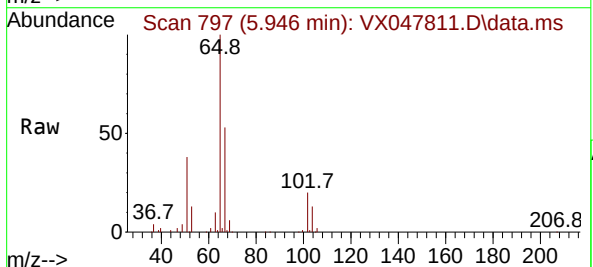


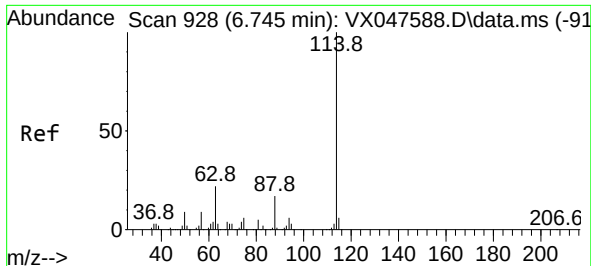

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX047811.D
Acq: 25 Sep 2025 14:56




Instrument :
MSVOA_X
ClientSampleId :
BPOW6-10-20250916


Tgt Ion:114 Resp: 260863
Ion Ratio Lower Upper
114 100
63 20.7 0.0 44.0
88 15.6 0.0 34.2

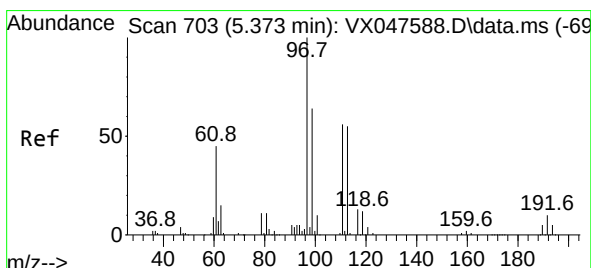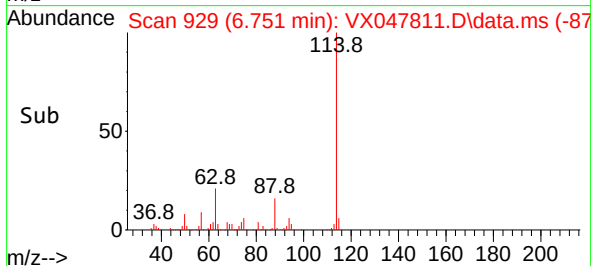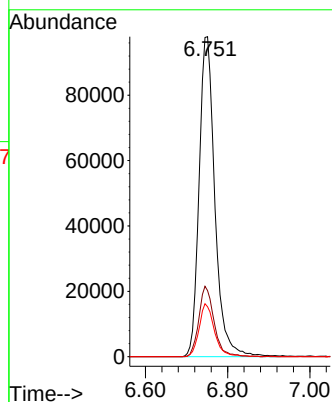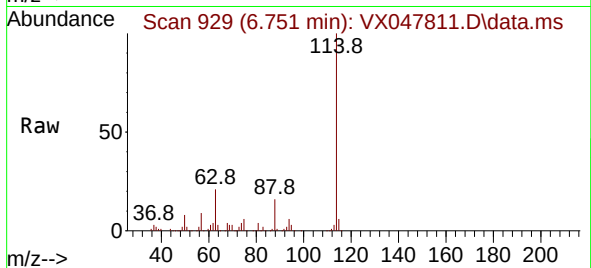

#35
Dibromofluoromethane
Concen: 48.668 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX047811.D
Acq: 25 Sep 2025 14:56

Tgt Ion:113 Resp: 85144
Ion Ratio Lower Upper
113 100
111 103.7 80.9 121.3
192 18.2 14.2 21.4


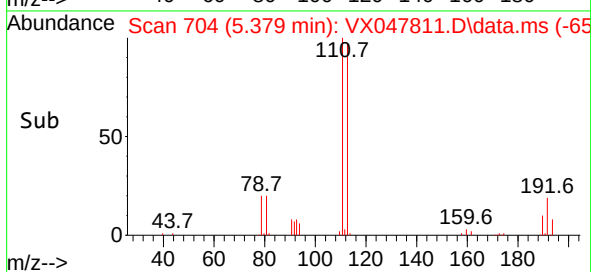
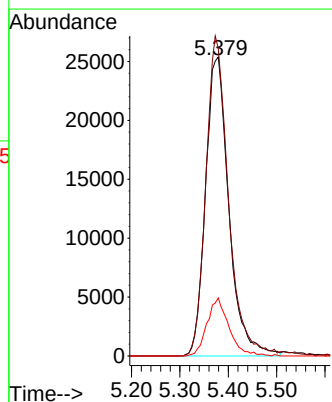
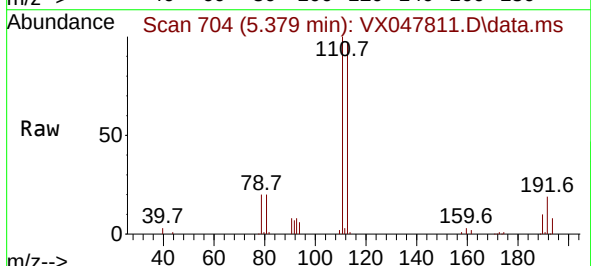


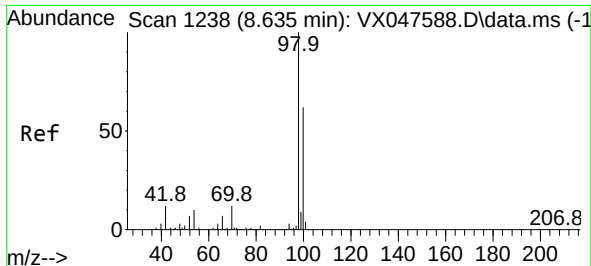

#50
Toluene-d8
Concen: 48.436 ug/l
RT: 8.635 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047811.D
Acq: 25 Sep 2025 14:56




Instrument :
MSVOA_X
ClientSampleId :
BPOW6-10-20250916


Tgt Ion: 98 Resp: 293211
Ion Ratio Lower Upper
98 100
100 66.7 53.0 79.4

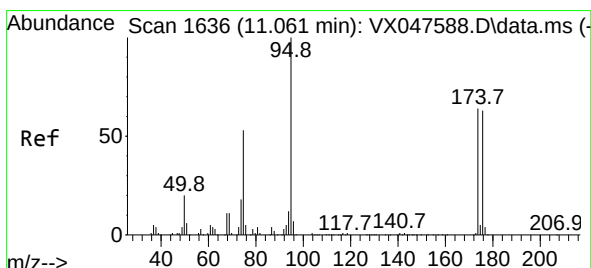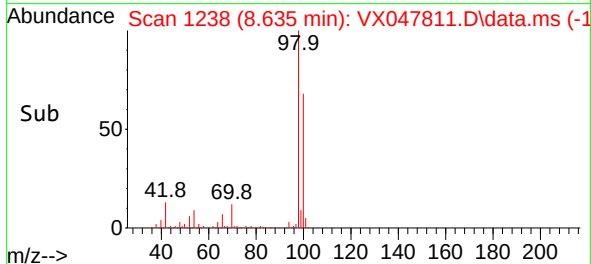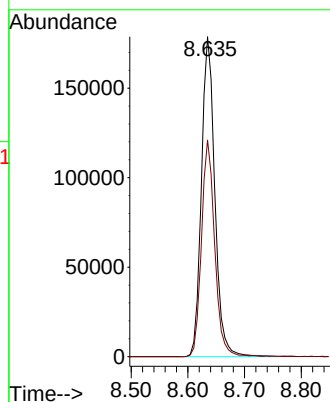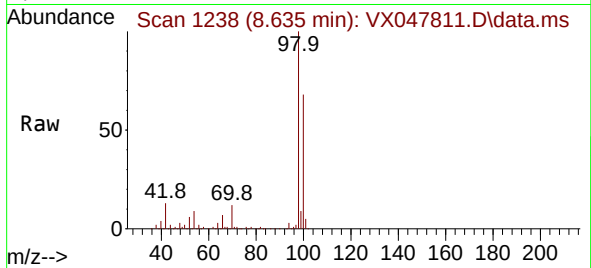

#62
4-Bromofluorobenzene
Concen: 53.970 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. 0.006 min
Lab File: VX047811.D
Acq: 25 Sep 2025 14:56

Tgt Ion: 95 Resp: 123993
Ion Ratio Lower Upper
95 100
174 72.3 0.0 141.6
176 69.3 0.0 138.4

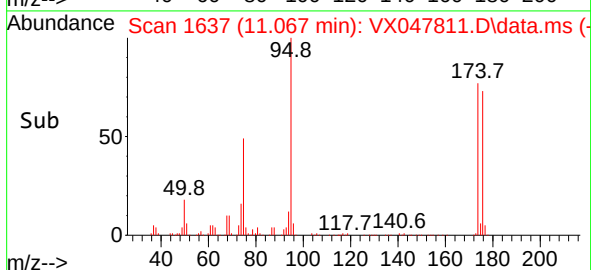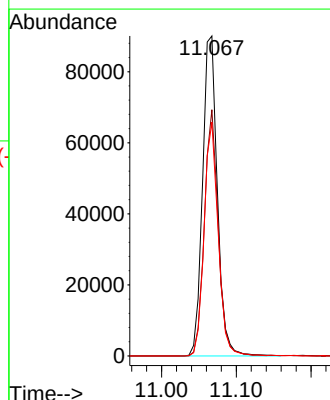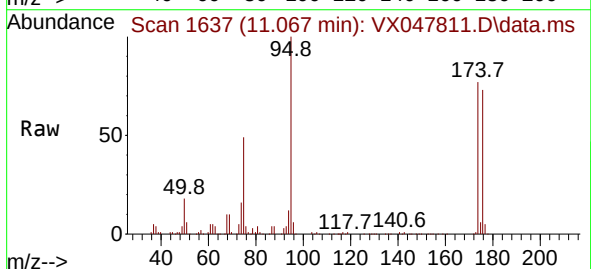

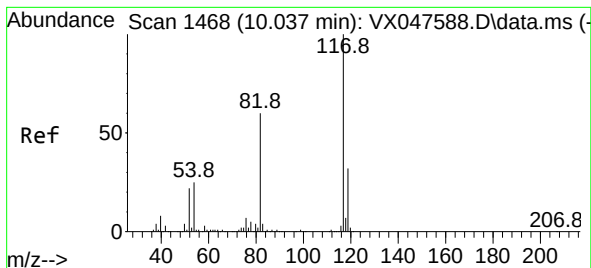

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.037 min Scan# 1468

Delta R.T. 0.000 min

Lab File: VX047811.D

Acq: 25 Sep 2025 14:56

Instrument :

MSVOA_X

ClientSampleId :

BPOW6-10-20250916





Tgt Ion:117 Resp: 264166

Ion Ratio Lower Upper

117 100

82 57.3 47.8 71.6

119 31.7 25.2 37.8

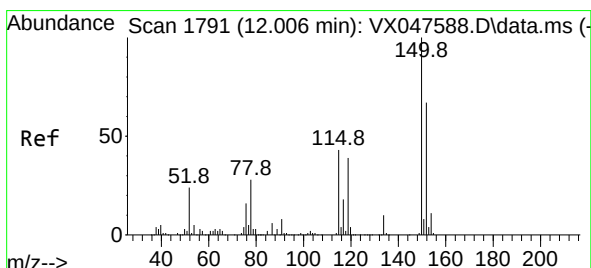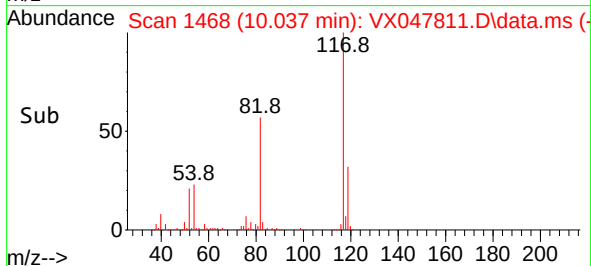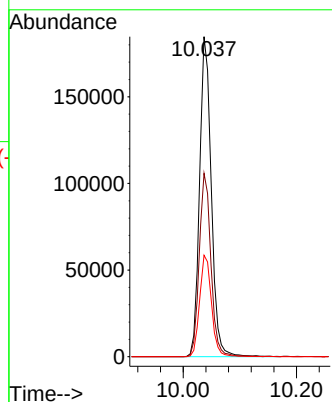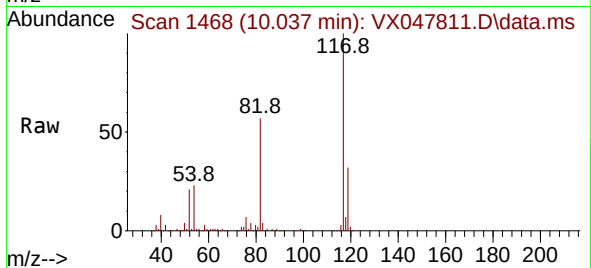

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX047811.D

Acq: 25 Sep 2025 14:56

Tgt Ion:152 Resp: 132252

Ion Ratio Lower Upper

152 100

115 62.2 44.9 134.5

150 156.2 0.0 352.0

