
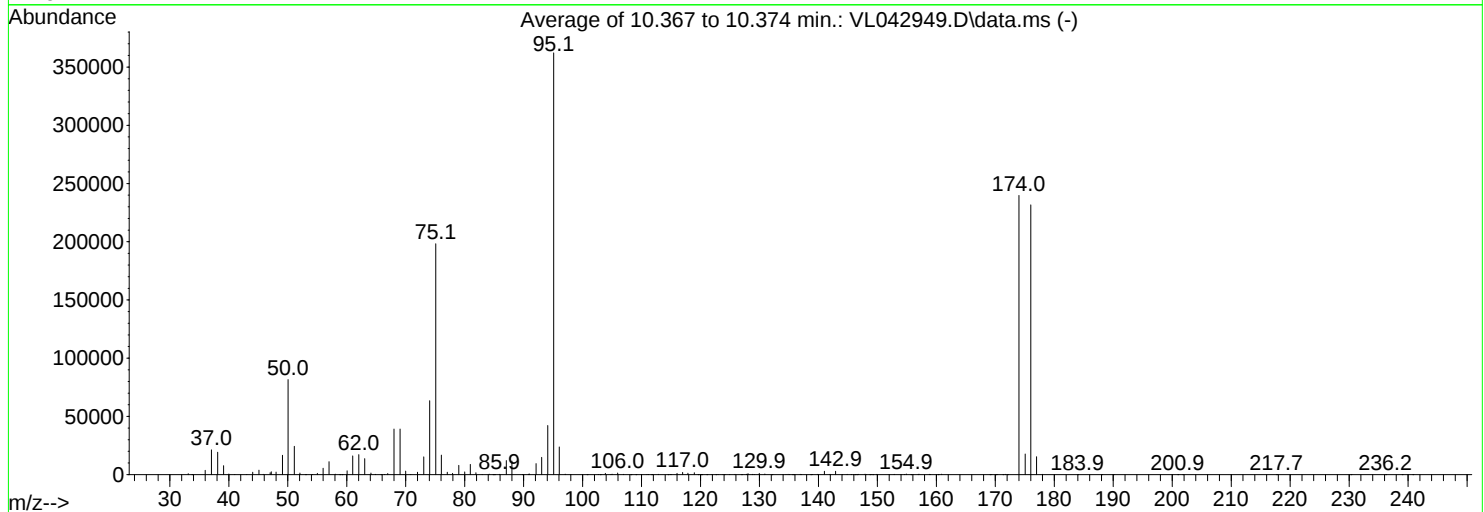


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092225\
Data File : VL042949.D
Acq On : 22 Sep 2025 08:55
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL092225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 23 02:39:16 2025

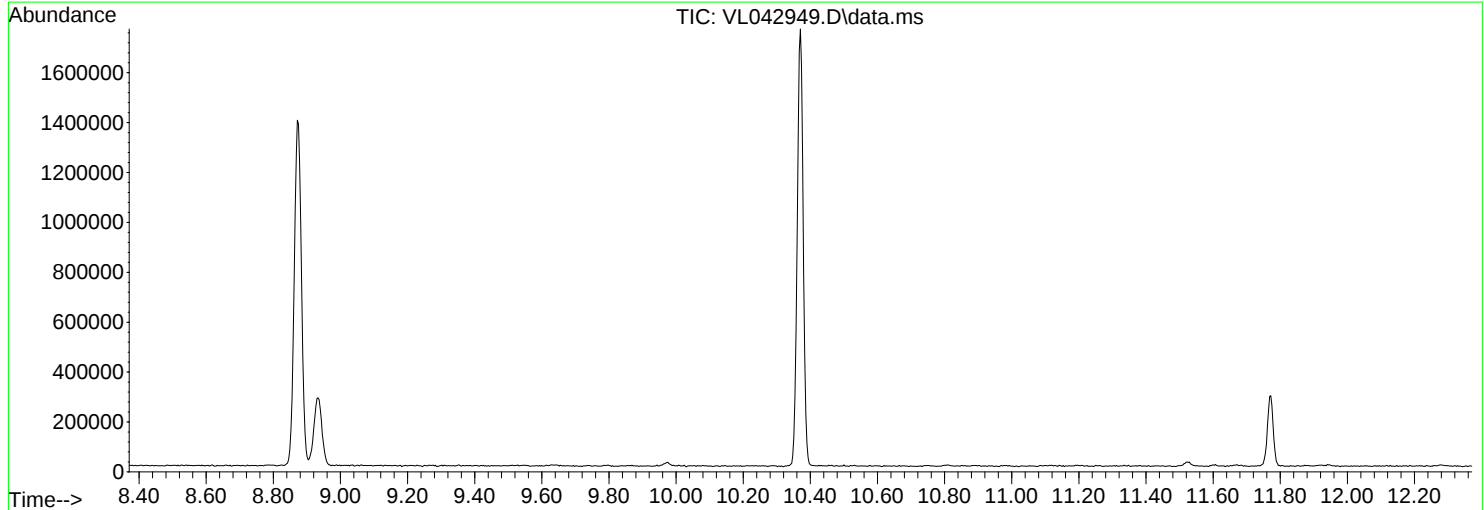

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3156

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.5	81605	PASS
75	95	30	66	54.7	198315	PASS
95	95	100	100	100.0	362228	PASS
96	95	5	9	6.6	23817	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.2	239765	PASS
175	174	4	9	7.4	17693	PASS
176	174	93	101	96.6	231701	PASS
177	176	5	9	6.6	15367	PASS

Average of 10.367 to 10.374 min.: VL042949.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	843	45.85	253	56.00	5545	65.80	3
33.75	52	47.00	1694	57.00	11198	66.40	12
36.00	3748	47.20	2450	58.05	458	66.95	97
37.05	21251	48.00	2247	58.80	12	68.00	3914
38.10	19194	49.10	16630	59.20	54	69.05	39122
39.10	7706	50.05	81605	60.05	3370	70.00	3041
40.00	611	51.10	24305	61.00	16140	70.85	223
41.00	212	52.05	1353	62.05	17219	72.00	2035
43.05	136	53.00	72	63.05	13691	73.05	15293
44.05	2095	54.20	86	64.10	1359	74.05	63454
45.10	3798	55.00	1059	64.85	245	75.10	198315

Average of 10.367 to 10.374 min.: VL042949.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	16800	85.90	337	97.05	420	109.05	56
77.05	2059	87.05	12149	98.00	81	110.00	192
77.95	1179	88.00	11664	100.75	61	110.90	139
79.00	8035	89.80	31	102.65	97	111.15	198
80.00	2335	90.80	359	103.00	49	111.70	49
80.95	8798	91.00	622	103.85	1171	111.85	96
81.90	1684	92.10	9517	104.80	150	112.85	303
82.95	138	93.05	14816	105.00	378	114.50	70
84.15	388	94.10	42269	105.95	1346	114.90	157
84.80	17	95.10	362228	106.95	255	115.05	161
85.05	75	96.05	23817	108.20	73	116.00	1147

Average of 10.367 to 10.374 min.: VL042949.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.95	1950	124.00	19	132.10	39	139.90	323
117.85	1188	124.95	84	134.00	140	141.00	2899
118.95	1697	125.85	229	134.50	114	141.95	349
119.60	51	126.95	77	134.85	336	142.90	2933
120.00	53	127.80	315	135.10	170	144.05	151
120.20	61	127.90	464	135.60	42	144.85	287
121.05	57	128.05	783	135.85	51	145.60	121
121.95	99	128.80	273	136.90	259	145.95	217
122.60	27	129.10	152	137.10	199	146.20	56
123.00	155	129.95	1180	138.70	60	146.50	40
123.80	97	130.90	521	139.00	86	146.80	278

Average of 10.367 to 10.374 min.: VL042949.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.90	407	155.70	50	170.40	165	190.00	32
148.10	181	156.05	156	171.30	71	200.95	53
148.70	34	156.90	168	171.75	267	201.80	37
148.95	87	157.05	367	172.05	48	217.70	32
149.20	38	158.80	225	174.00	239765	230.30	17
149.90	259	159.00	184	175.05	17693	236.20	53
152.00	157	160.30	45	176.00	231701	239.00	24
152.85	262	160.90	377	177.00	15367	240.80	20
154.00	172	169.10	53	178.00	351		
154.60	207	169.40	85	183.95	49		
154.90	569	170.10	37	188.00	21		