
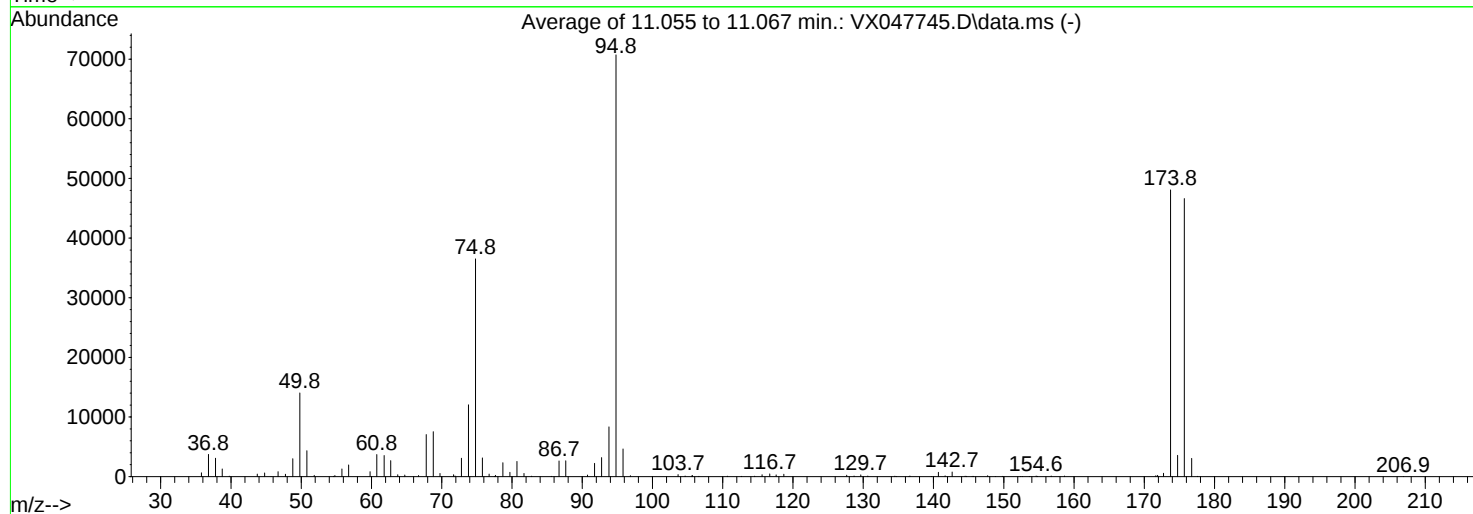


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047745.D
Acq On : 24 Sep 2025 01:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

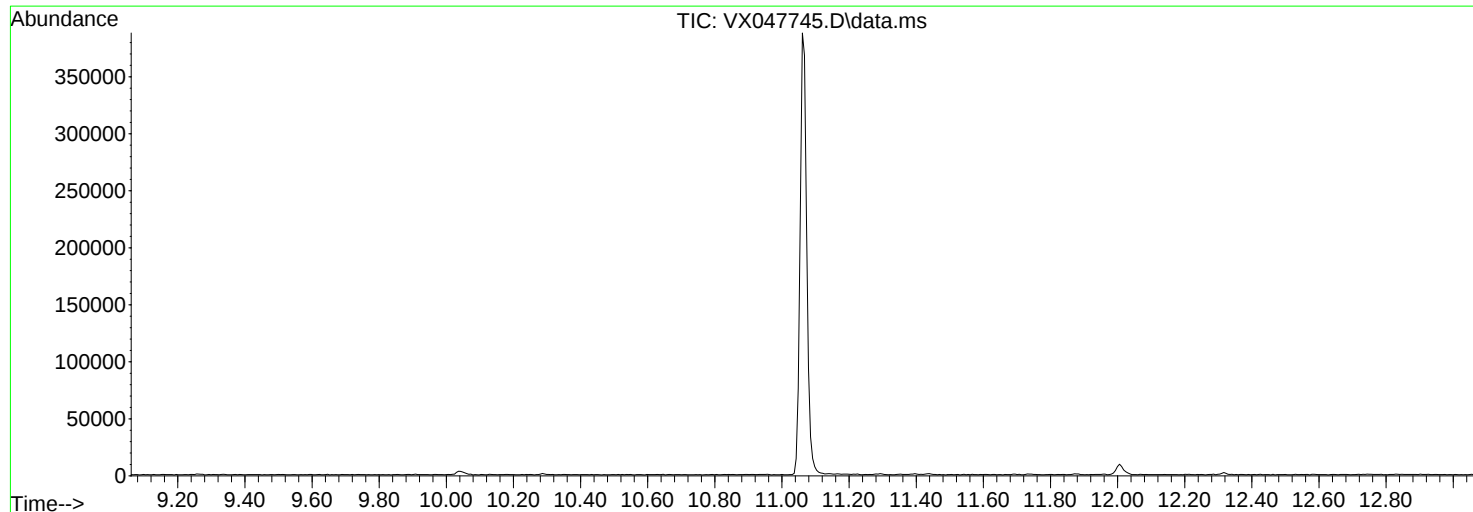

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	14045	PASS
75	95	30	60	51.6	36501	PASS
95	95	100	100	100.0	70720	PASS
96	95	5	9	6.6	4644	PASS
173	174	0.00	2	1.2	568	PASS
174	95	50	100	68.0	48067	PASS
175	174	5	9	7.4	3558	PASS
176	174	95	101	97.0	46629	PASS
177	176	5	9	6.5	3052	PASS